
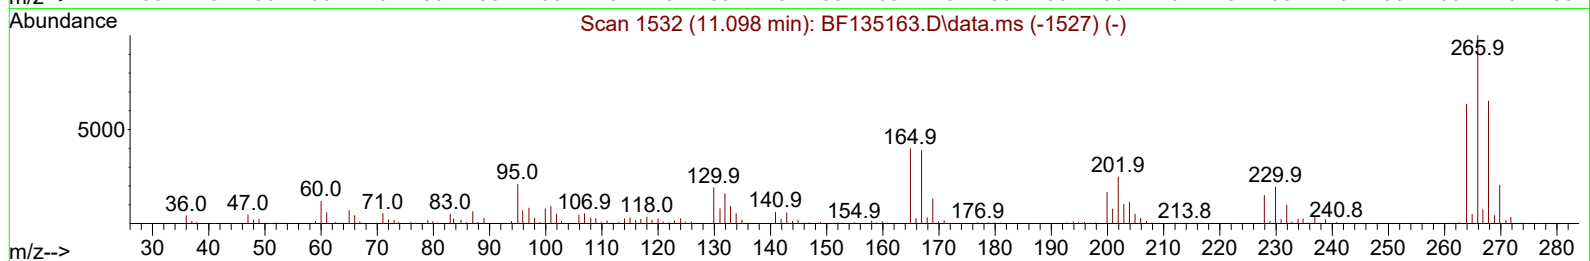
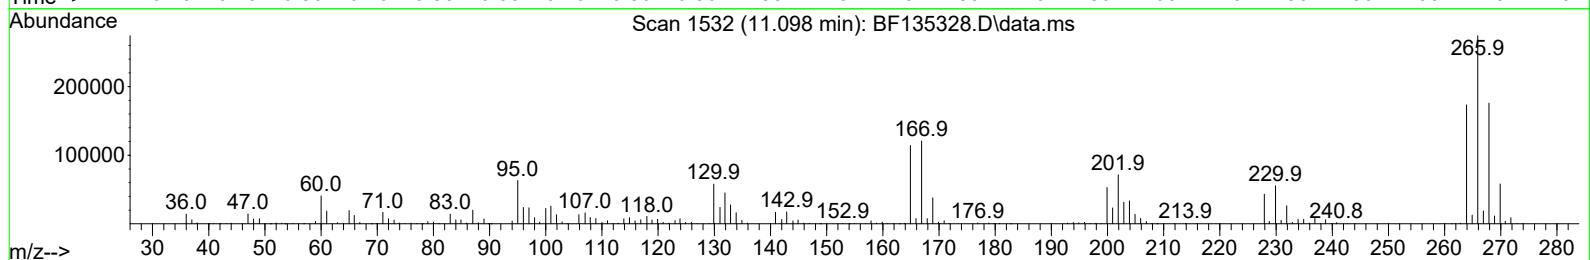


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135328.D
Acq On : 19 Sep 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 13:01:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

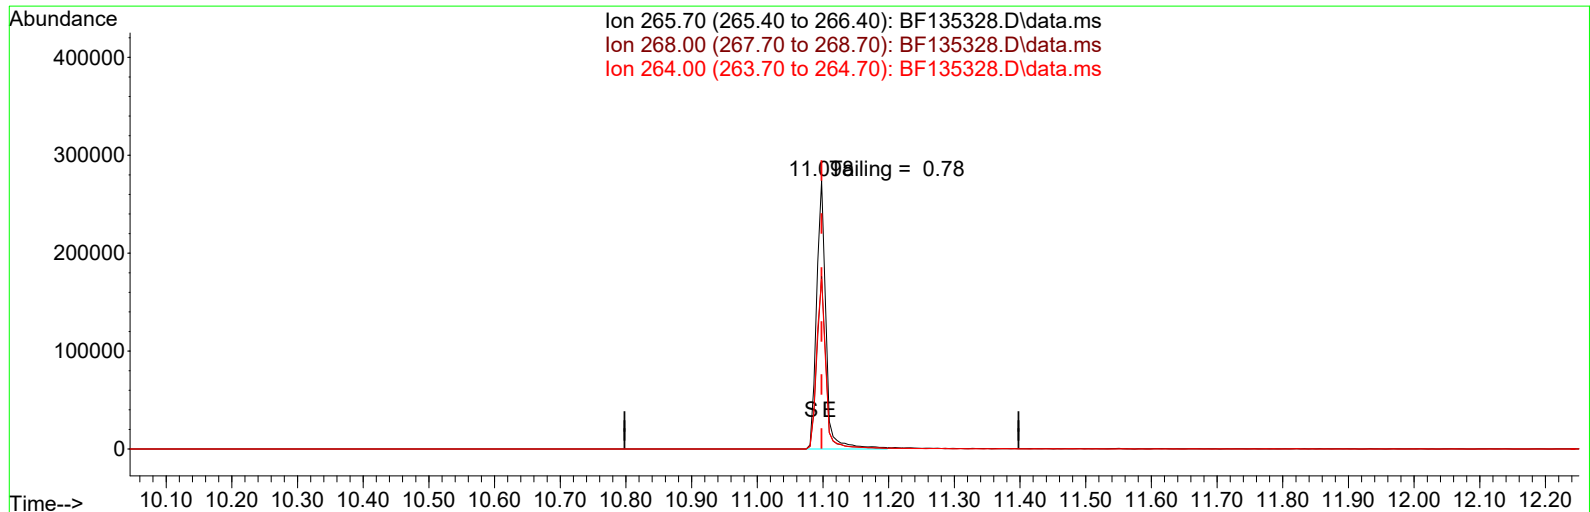

TIC: BF135328.D\data.ms

(70) Pentachlorophenol (C)




11.098min (+ 0.000) 150252.26 ng

response 276902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.23
264.00	63.50	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135328.D
Acq On : 19 Sep 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 13:01:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

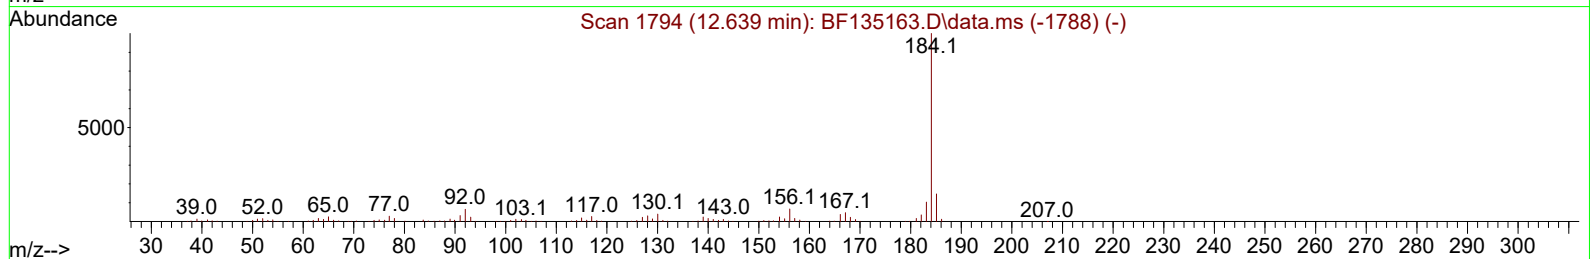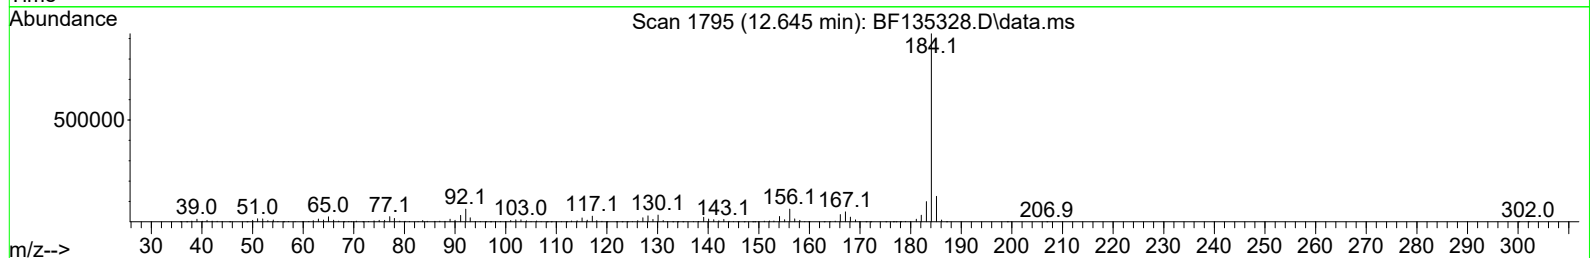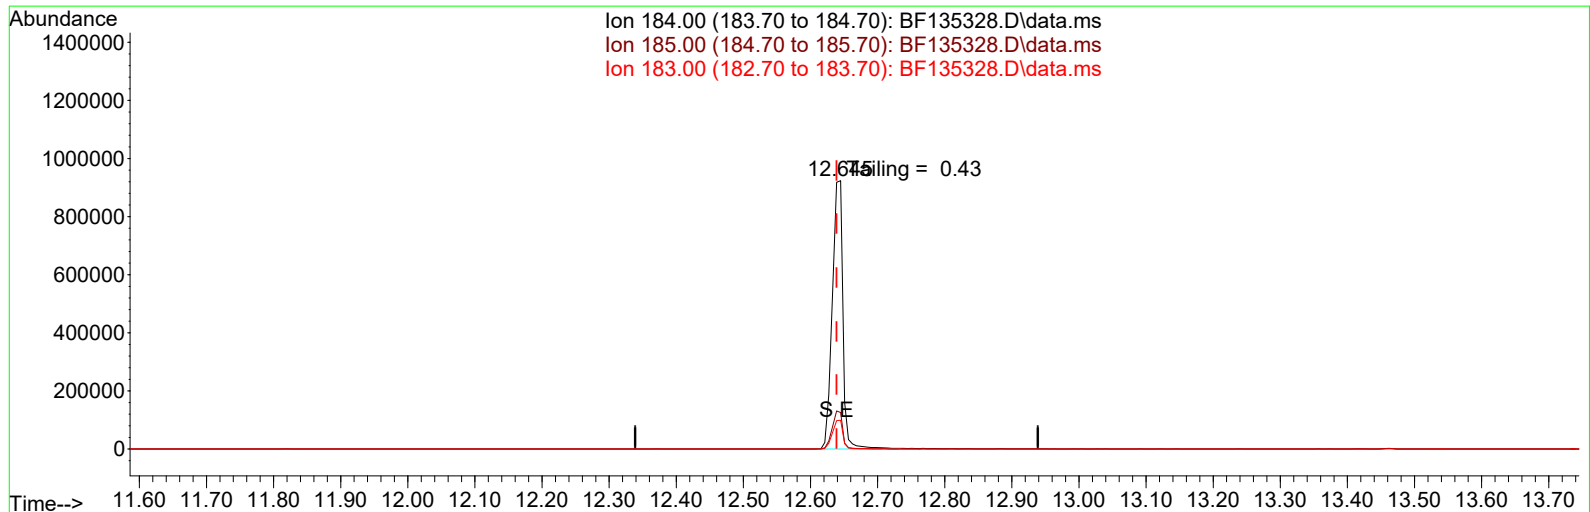

TIC: BF135328.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 79401.29 ng

response 1019929

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.58
183.00	10.30	10.73
0.00	0.00	0.00