

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
 Data File : BF135330.D
 Acq On : 19 Sep 2023 10:45
 Operator : CG\JU
 Sample : PB155601BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155601BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	566	rBV	3622323	3872738	88.91%	14.139%
2	6.404	729	734	737	rBV	3463308	3953772	90.77%	14.435%
3	6.757	790	794	805	rBV	967741	778962	17.88%	2.844%
4	7.322	885	890	893	rBV	2319297	2666355	61.21%	9.734%
5	8.033	1007	1011	1015	rBV	1112476	1019590	23.41%	3.722%
6	9.116	1189	1195	1198	rBV	4216629	4355809	100.00%	15.902%
7	9.792	1305	1310	1314	rBV	1339912	1143907	26.26%	4.176%
8	10.586	1440	1445	1449	rBV	2523532	2733643	62.76%	9.980%
9	11.286	1560	1564	1567	rBV	1455169	1227745	28.19%	4.482%
10	12.886	1831	1836	1840	rBV	3754812	4238962	97.32%	15.476%
11	13.945	2011	2016	2023	rBV	756145	750132	17.22%	2.739%
12	15.409	2260	2265	2273	rBV	487175	649468	14.91%	2.371%




Sum of corrected areas: 27391083

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135330.D
Acq On : 19 Sep 2023 10:45
Operator : CG\JU
Sample : PB155601BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155601BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

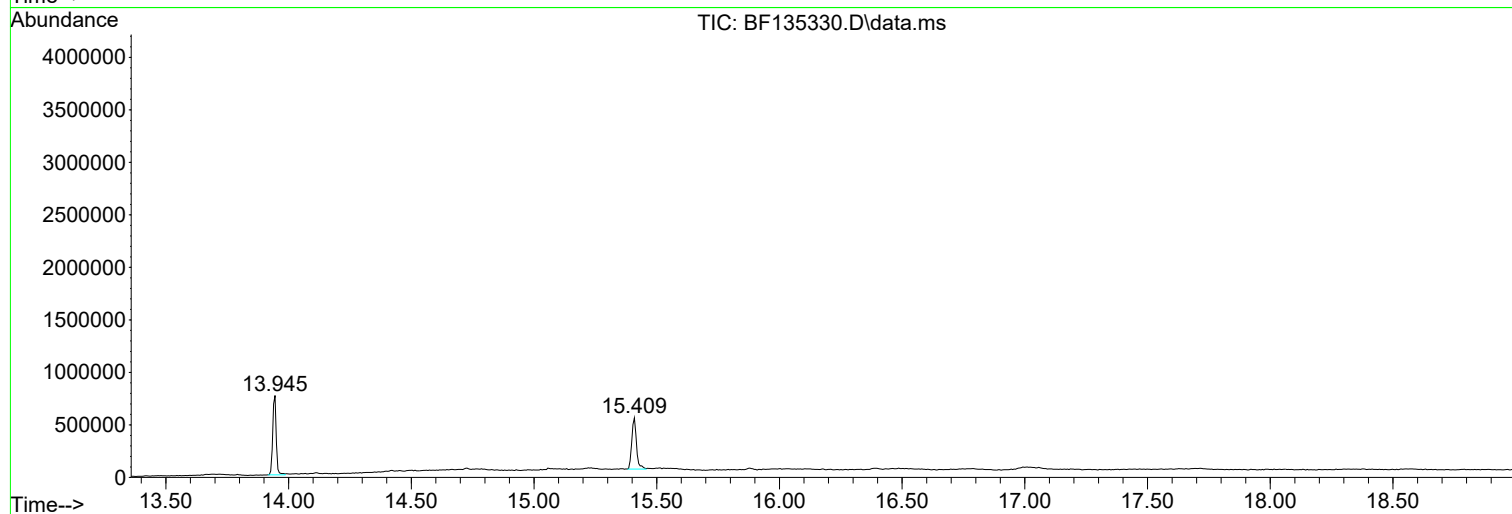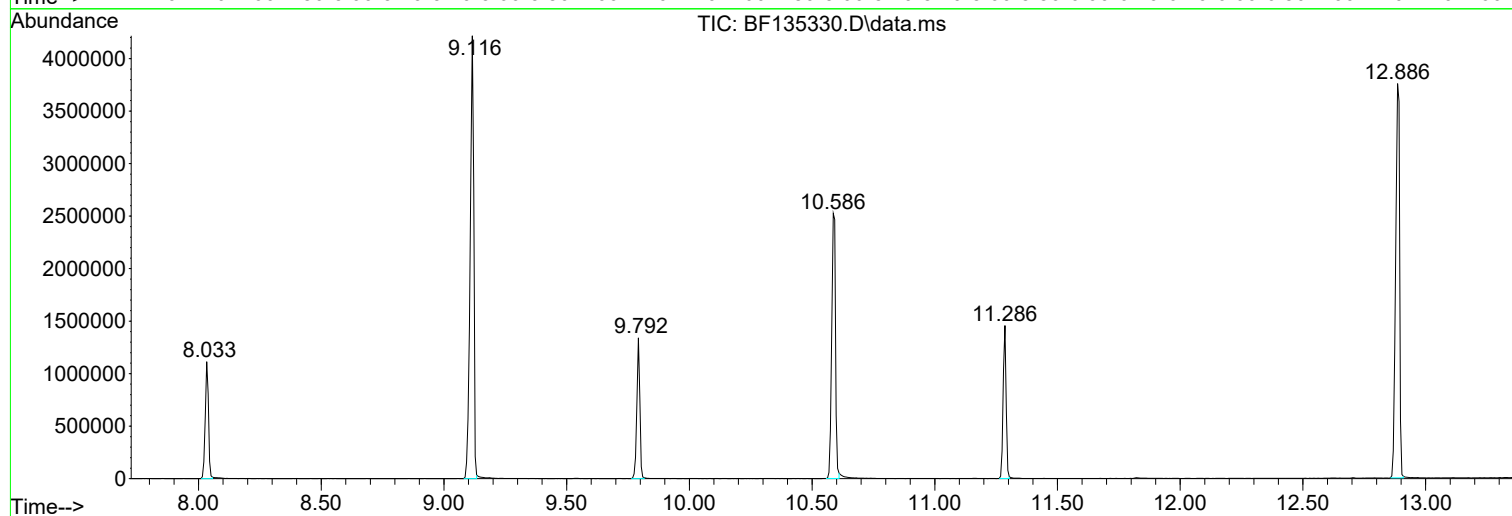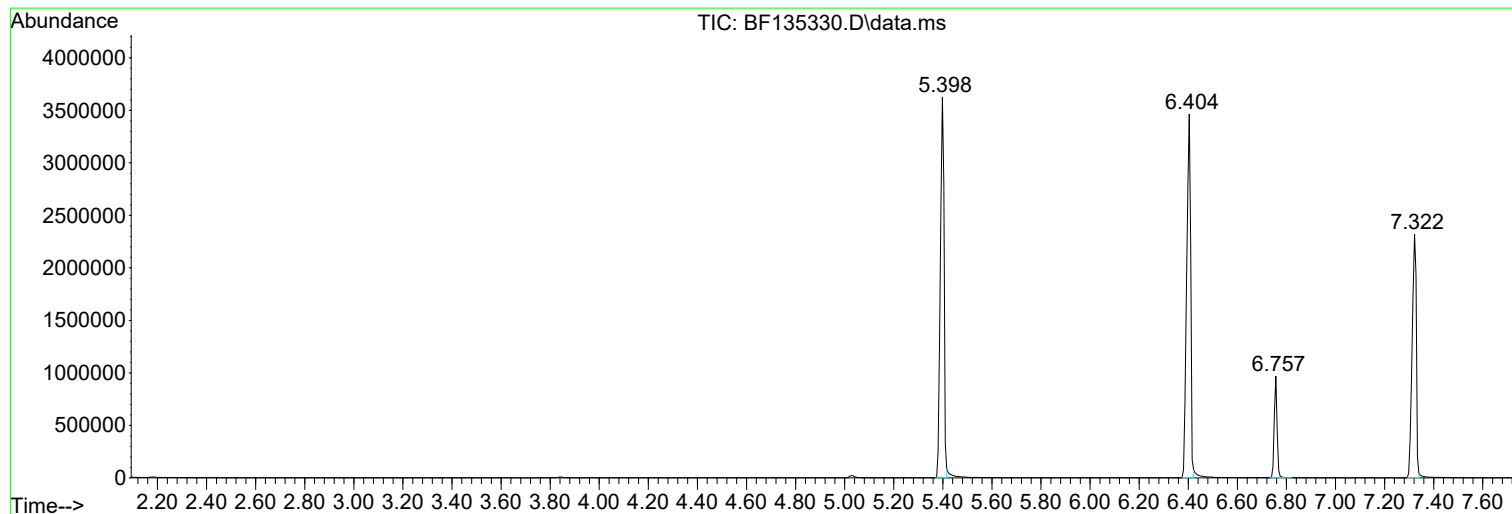

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135330.D
Acq On : 19 Sep 2023 10:45
Operator : CG\JU
Sample : PB155601BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155601BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135330.D
Acq On : 19 Sep 2023 10:45
Operator : CG\JU
Sample : PB155601BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155601BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------