
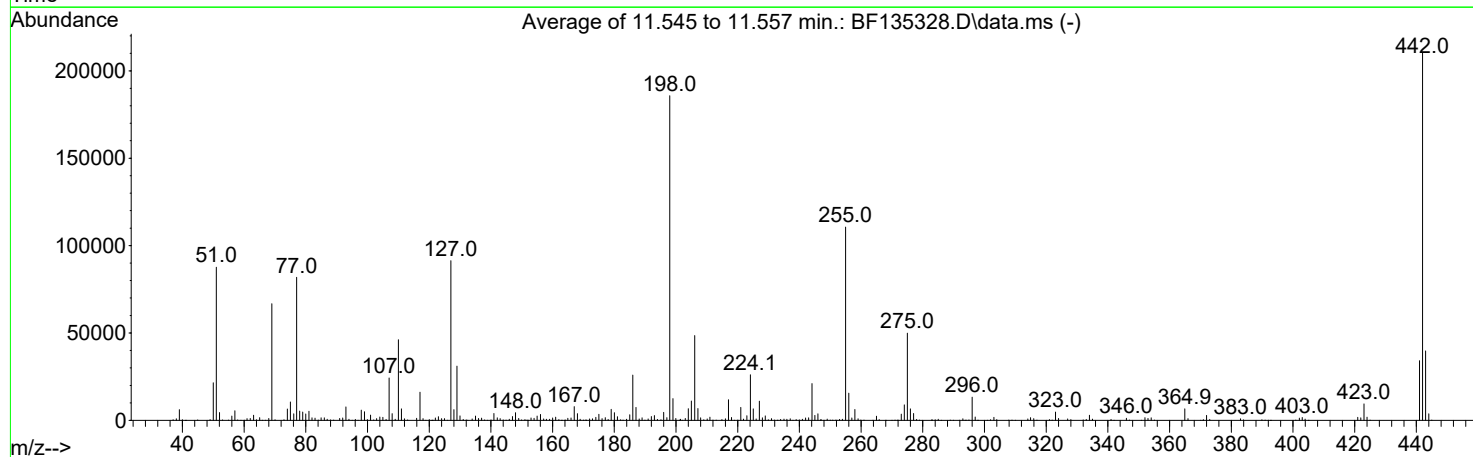


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135328.D
Acq On : 19 Sep 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

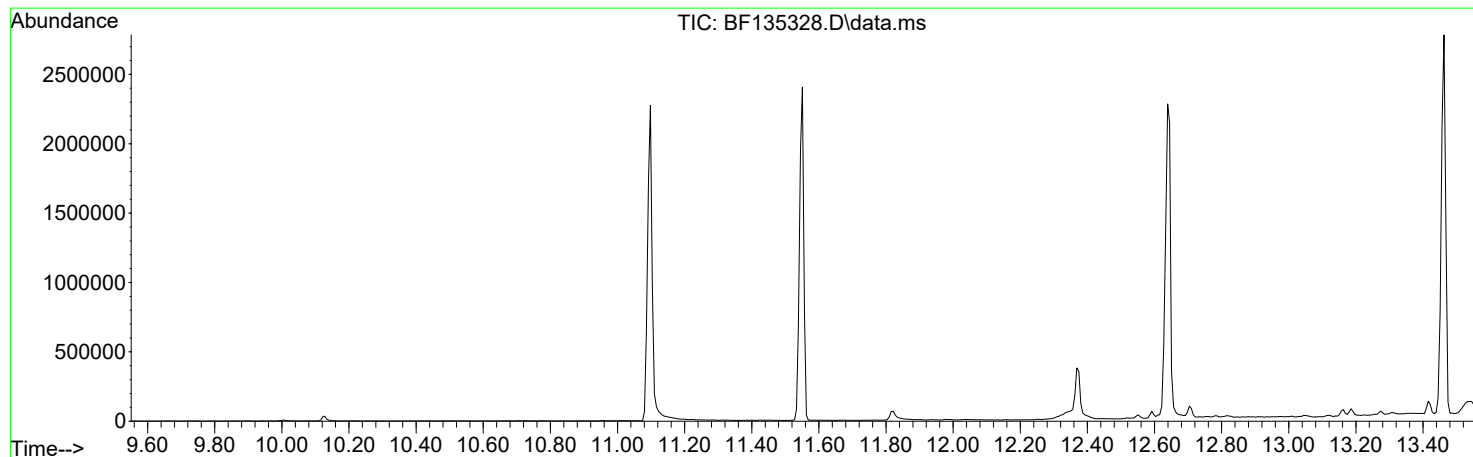

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	87635	PASS
68	69	0.00	2	1.6	1068	PASS
69	198	0.00	100	35.9	66740	PASS
70	69	0.00	2	0.5	333	PASS
127	198	10	80	49.2	91408	PASS
197	198	0.00	2	0.8	1537	PASS
198	198	100	100	100.0	185795	PASS
199	198	5	9	6.7	12443	PASS
275	198	10	60	26.8	49880	PASS
365	198	1	100	3.6	6608	PASS
441	198	0.01	100	18.4	34179	PASS
442	442	50	100	100.0	210496	PASS
443	442	15	24	18.9	39781	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/19/2023	BNA_F	<u>BF135328.D</u>
Compound Name	Response	Retention Time
DDT	496940	13.462
DDD	15298	13.163
DDE	1178	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16476	513416	3.21

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
Data File : BF135328.D
Acq On : 19 Sep 2023 09:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 19 13:01:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

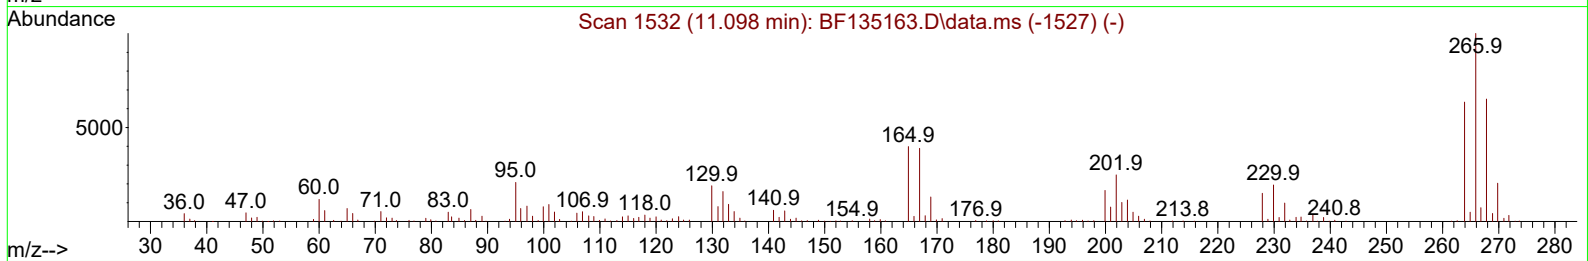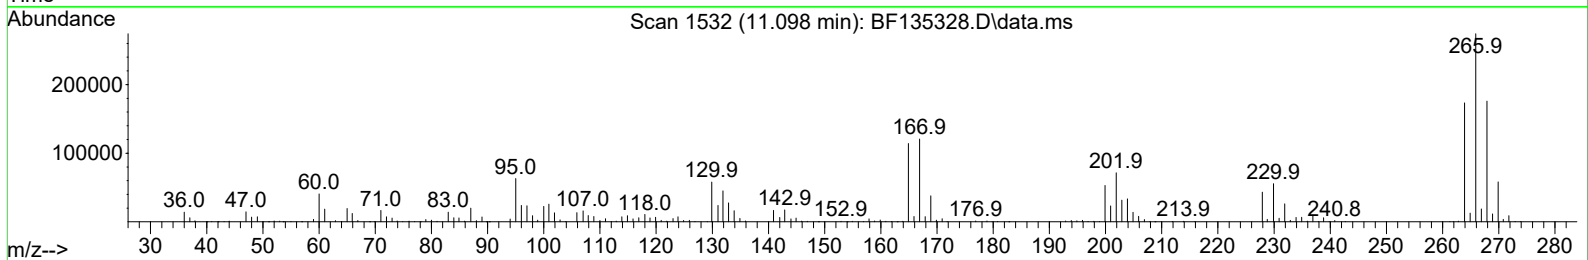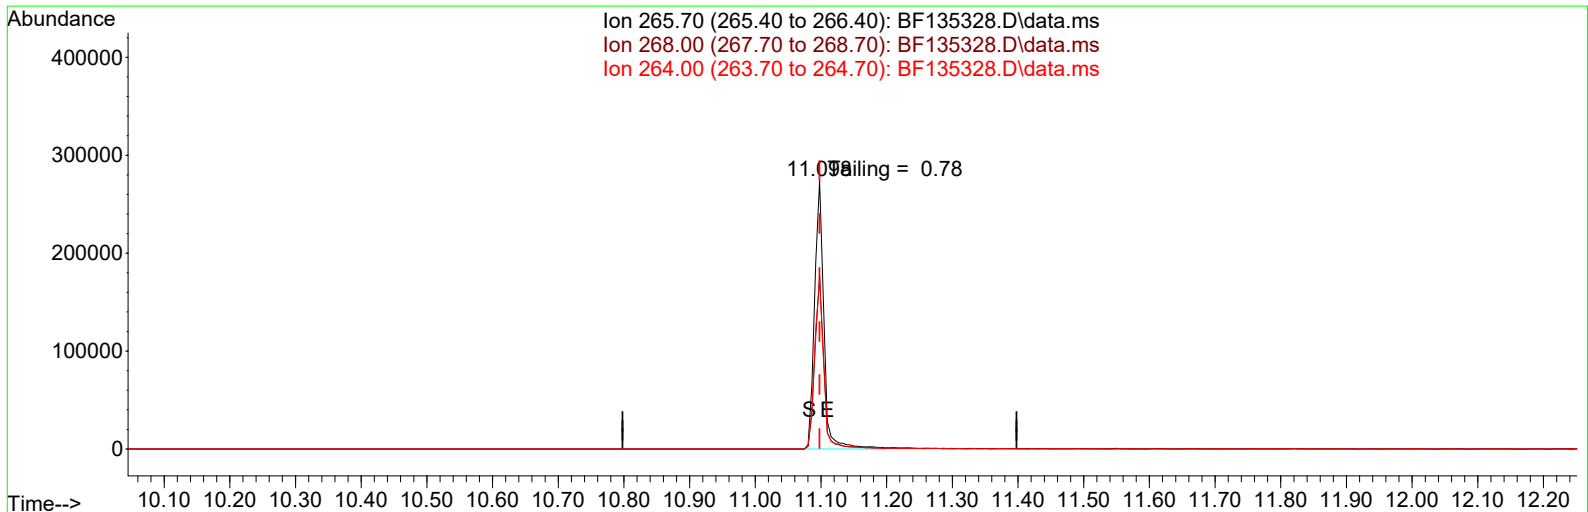

TIC: BF135328.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.000) 150252.26 ng




response 276902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.23
264.00	63.50	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091923\
 Data File : BF135328.D
 Acq On : 19 Sep 2023 09:44
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 19 13:01:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

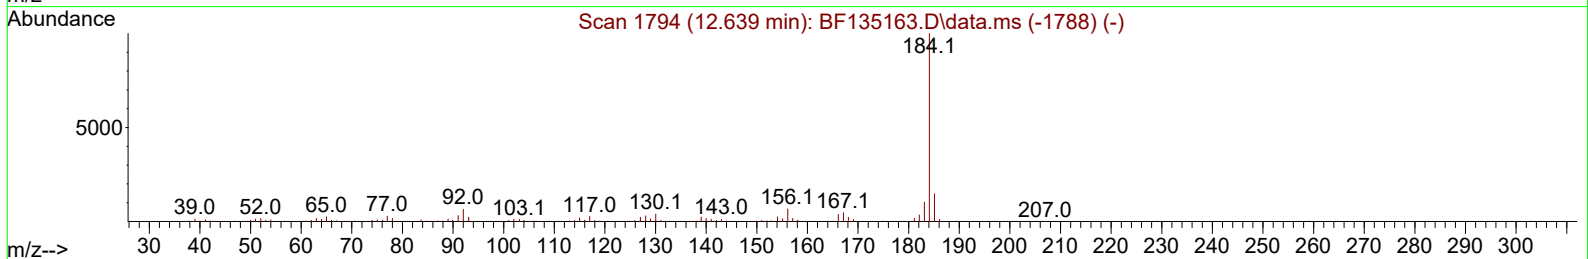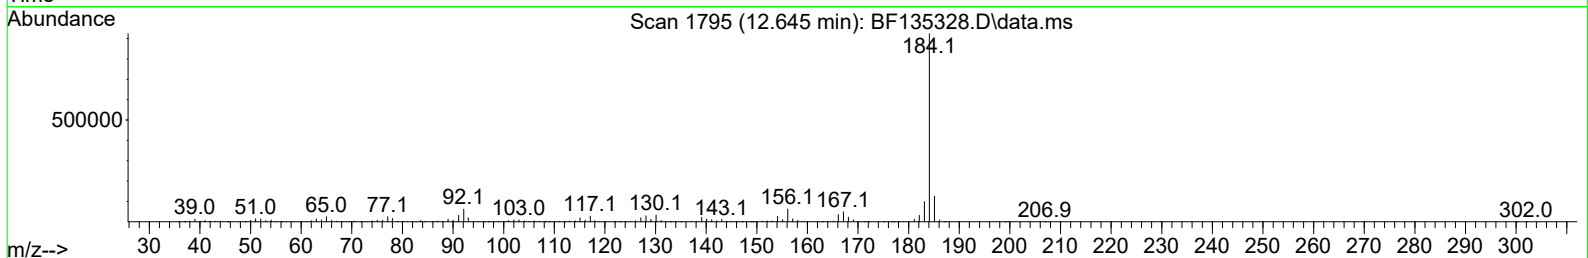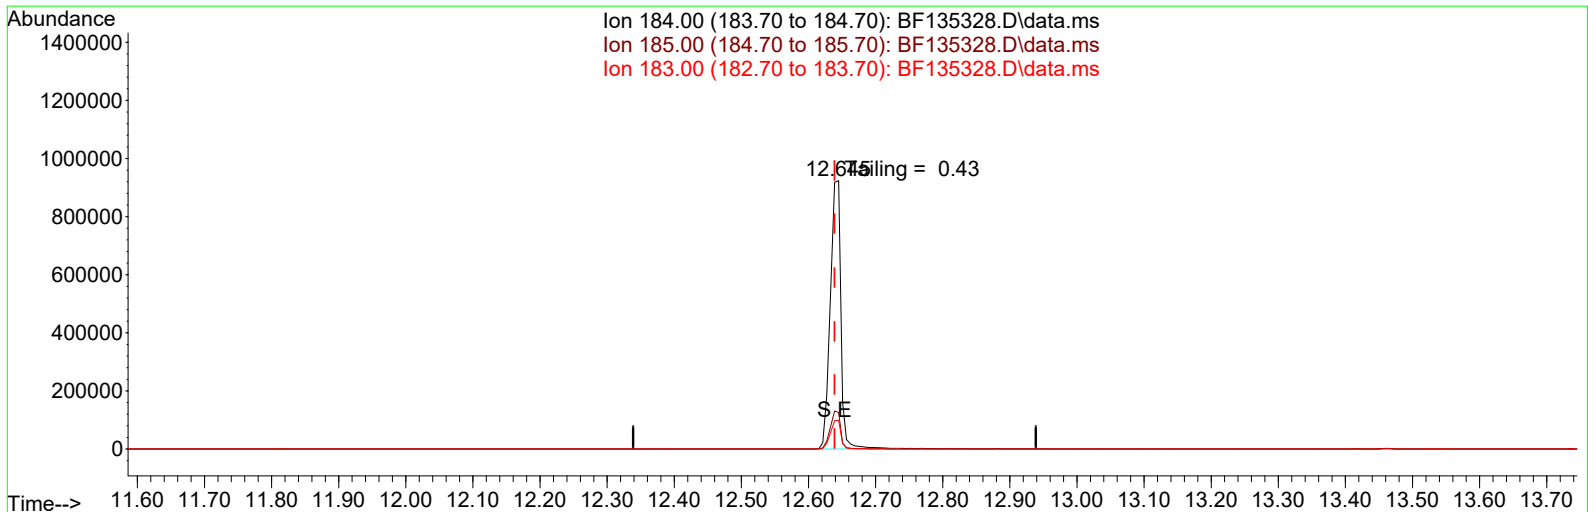

TIC: BF135328.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 79401.29 ng

response 1019929

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.58
183.00	10.30	10.73
0.00	0.00	0.00