

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092018\
 Data File : BF109188.D
 Acq On : 20 Sep 2018 18:12
 Operator : JU/SJ
 Sample : J4993-06 20X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NS-OILY-WATER

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.319	505	507	512	rVB	14291	13273	2.47%	0.423%
2	6.348	677	682	687	rBB	8961	9035	1.68%	0.288%
3	6.484	702	705	711	rVB	41430	33674	6.26%	1.073%
4	6.719	741	745	749	rBV	462586	374032	69.58%	11.916%
5	6.872	768	771	775	rBB	50932	39355	7.32%	1.254%
6	7.272	836	839	847	rVB	33764	30903	5.75%	0.985%
7	7.636	898	901	903	rBV	12234	11682	2.17%	0.372%
8	8.001	959	963	966	rBV	651925	510860	95.03%	16.275%
9	9.072	1142	1145	1150	rBV	73289	59596	11.09%	1.899%
10	9.748	1256	1260	1268	rBV	613582	537588	100.00%	17.127%
11	10.530	1391	1393	1398	rVB	27289	21759	4.05%	0.693%
12	11.224	1507	1511	1515	rBV	547522	499435	92.90%	15.911%
13	11.271	1517	1519	1526	rVB5	4523	7770	1.45%	0.248%
14	11.760	1599	1602	1606	rBV4	11644	13156	2.45%	0.419%
15	12.801	1776	1779	1784	rVB	97741	87851	16.34%	2.799%
16	13.724	1933	1936	1941	rBV4	5333	6927	1.29%	0.221%
17	13.848	1953	1957	1961	rBV	382584	356289	66.28%	11.351%
18	14.336	2038	2040	2044	rVB4	7726	7003	1.30%	0.223%
19	14.636	2087	2091	2099	rVB4	12344	18073	3.36%	0.576%
20	14.948	2141	2144	2148	rVB2	13403	14193	2.64%	0.452%
21	15.189	2182	2185	2191	rBV6	4184	9588	1.78%	0.305%
22	15.254	2191	2196	2202	rVV2	257170	326593	60.75%	10.405%
23	15.306	2202	2205	2211	rVB2	22696	30177	5.61%	0.961%
24	15.706	2264	2273	2282	rVB3	23723	46517	8.65%	1.482%
25	16.171	2346	2352	2362	rBV	16468	30685	5.71%	0.978%
26	16.718	2438	2445	2451	rVB3	8603	19117	3.56%	0.609%
27	17.136	2509	2516	2520	rBV5	4610	12333	2.29%	0.393%
28	17.365	2553	2555	2563	rVB7	6315	11411	2.12%	0.364%


Sum of corrected areas: 3138875

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092018\
Data File : BF109188.D
Acq On : 20 Sep 2018 18:12
Operator : JU/SJ
Sample : J4993-06 20X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NS-OILY-WATER

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

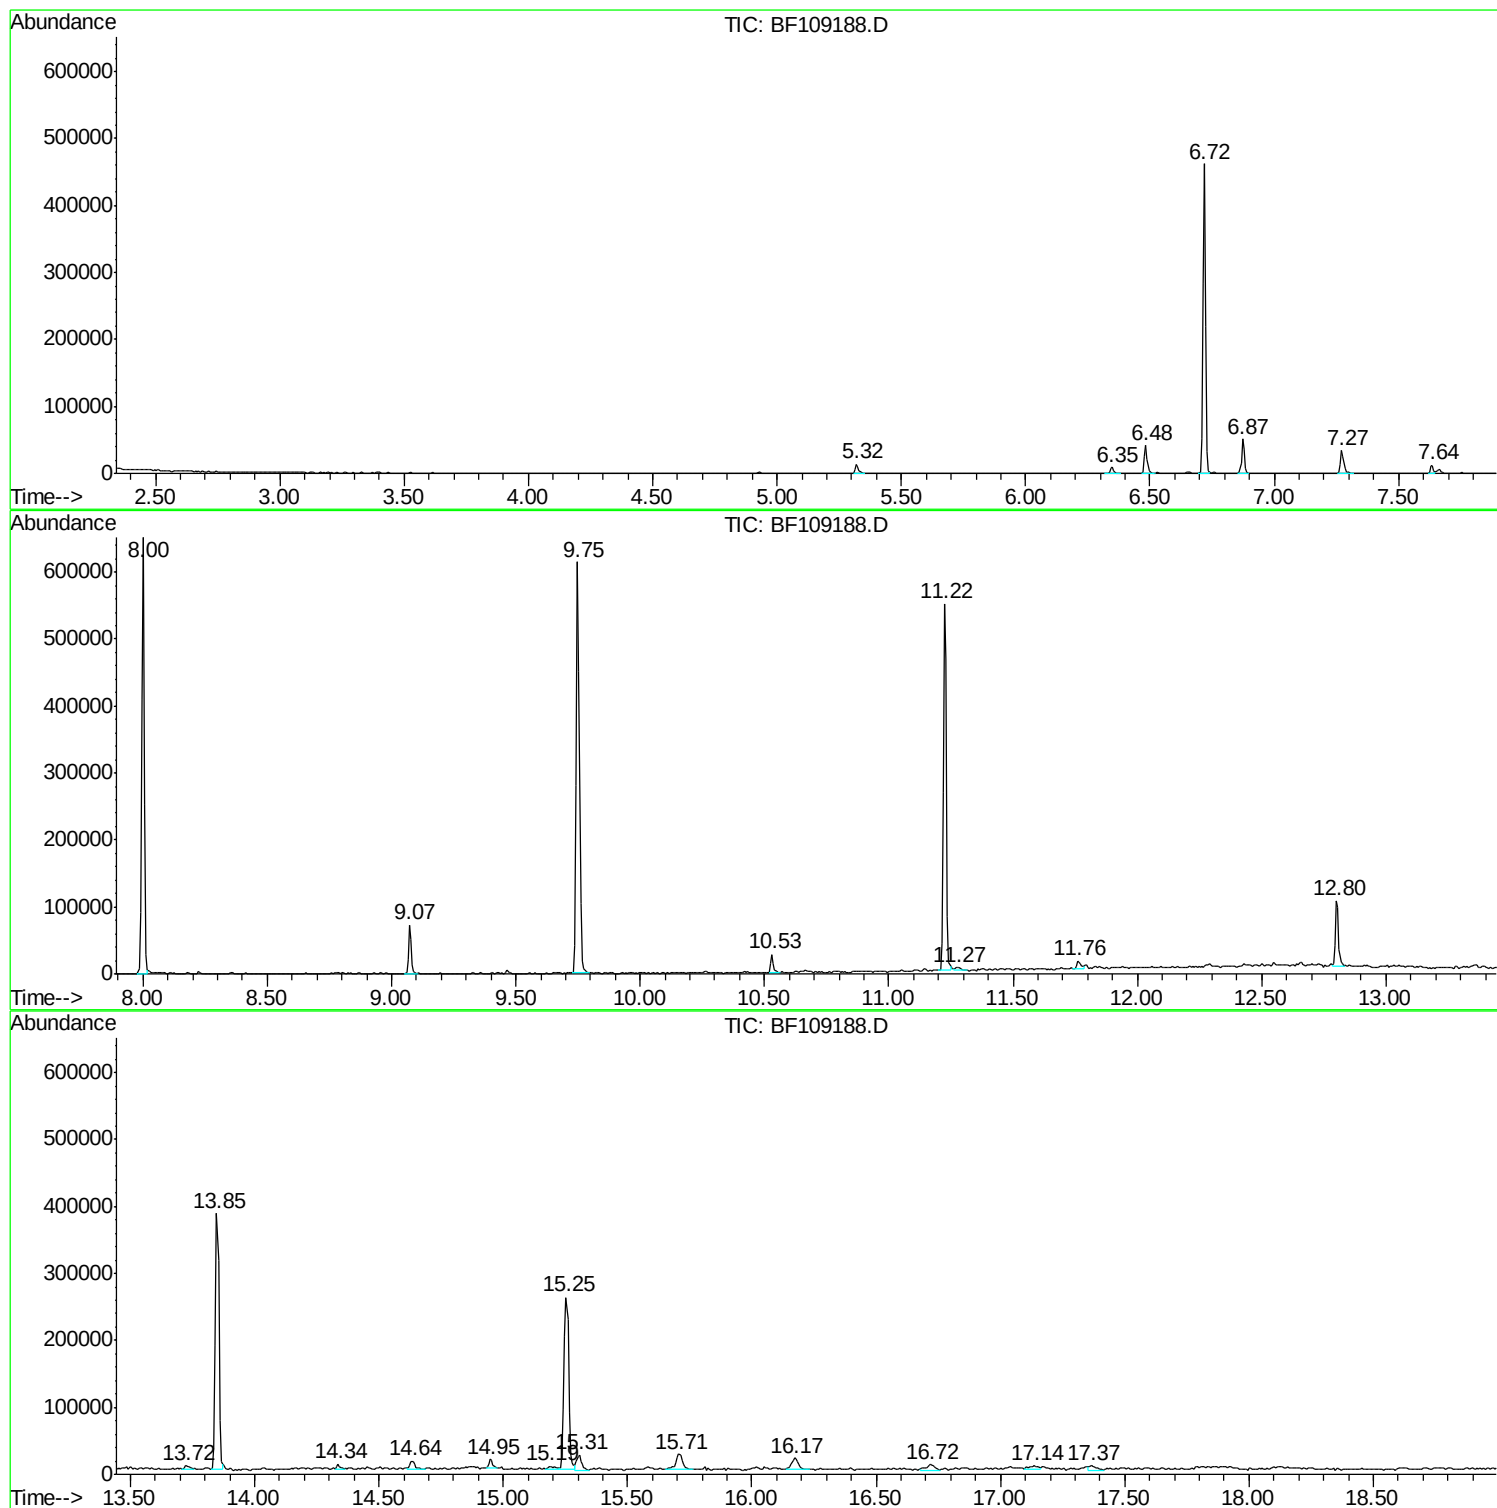

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092018\
Data_File : BF109188.D
Acq_On : 20-Sep-2018 18:122
Operator : JU/SJJ
Sample : J4993-06-20XX
Misc :
ALS_Vial : 10 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
NS-OILY-WATER

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
