


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092018\
 Data File : BF109179.D
 Acq On : 20 Sep 2018 14:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

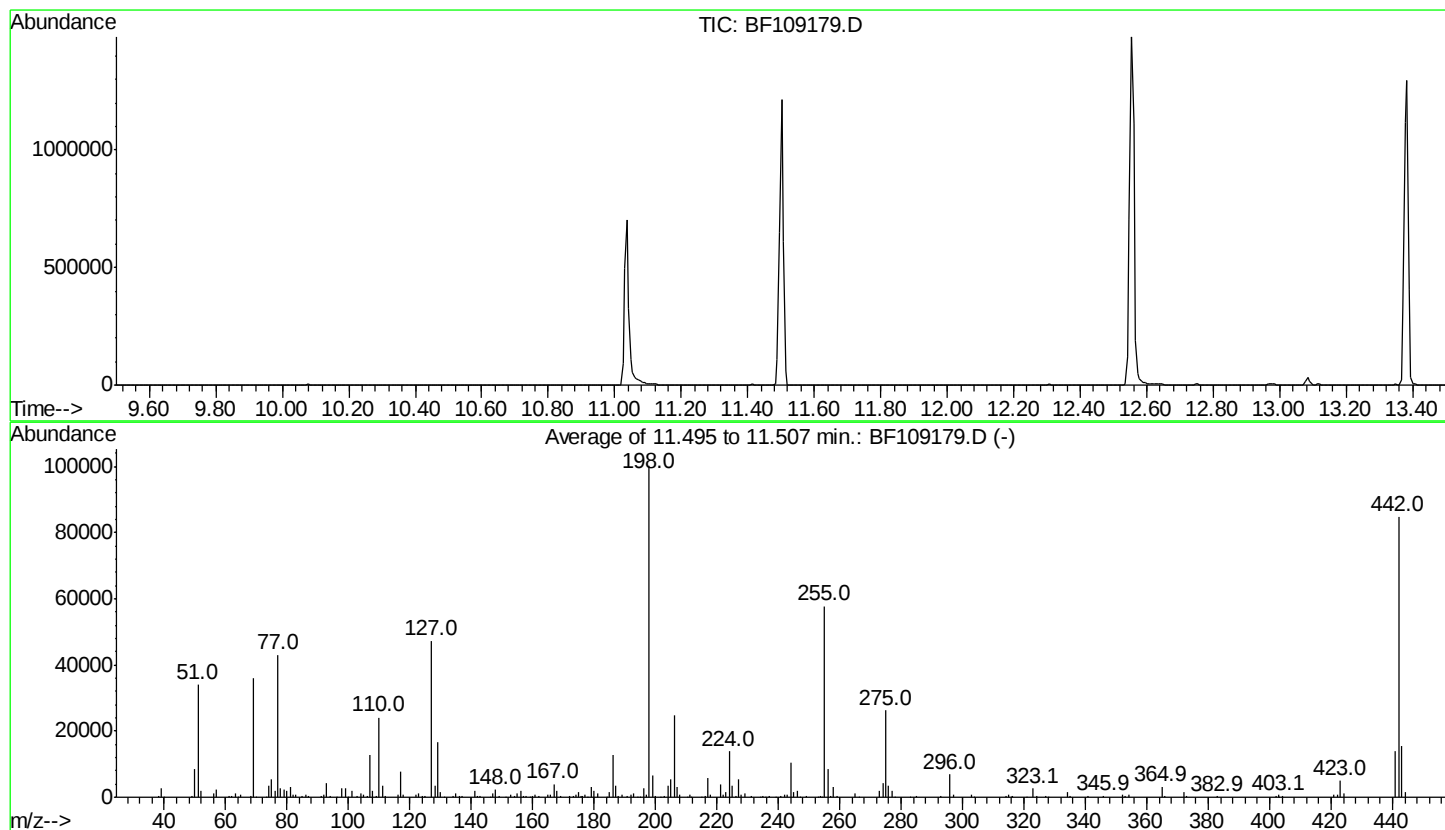

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	33917	PASS
68	69	0.00	2	1.4	506	PASS
69	198	0.00	100	35.8	35904	PASS
70	69	0.00	2	0.3	103	PASS
127	198	10	80	47.2	47322	PASS
197	198	0.00	2	0.8	780	PASS
198	198	100	100	100.0	100285	PASS
199	198	5	9	6.4	6426	PASS
275	198	10	60	26.1	26210	PASS
365	198	1	100	3.3	3292	PASS
441	198	0.01	100	13.9	13892	PASS
442	198	50	100	84.7	84936	PASS
443	442	15	24	18.4	15647	PASS