

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
 Data File : BF117191.D
 Acq On : 20 Sep 2019 17:50
 Operator : HP/JU
 Sample : PB123274BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB123274BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	13	17	22	rVB	18860	26059	1.45%	0.223%
2	5.457	568	573	576	rBV	1165442	1117273	61.99%	9.565%
3	6.463	738	744	747	rBV	1089290	1219330	67.65%	10.438%
4	6.592	761	766	769	rBV	1351656	1344945	74.62%	11.514%
5	6.816	801	804	814	rBV	273263	233921	12.98%	2.003%
6	6.975	827	831	834	rBV	1108134	982602	54.52%	8.412%
7	7.381	895	900	916	rBV	628474	786150	43.62%	6.730%
8	8.098	1018	1022	1037	rBV	252450	296598	16.46%	2.539%
9	9.175	1199	1205	1208	rBV	1686436	1625733	90.20%	13.917%
10	9.851	1315	1320	1330	rBV	332223	368697	20.46%	3.156%
11	10.645	1450	1455	1476	rBV	999723	1013243	56.22%	8.674%
12	11.339	1569	1573	1590	rBV	295831	370025	20.53%	3.168%
13	12.927	1837	1843	1846	rBV	1817334	1802387	100.00%	15.430%
14	13.980	2018	2022	2037	rBV	203382	286925	15.92%	2.456%
15	15.433	2264	2269	2282	rBV	118999	207422	11.51%	1.776%


Sum of corrected areas: 11681310

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
Data File : BF117191.D
Acq On : 20 Sep 2019 17:50
Operator : HP/JU
Sample : PB123274BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB123274BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

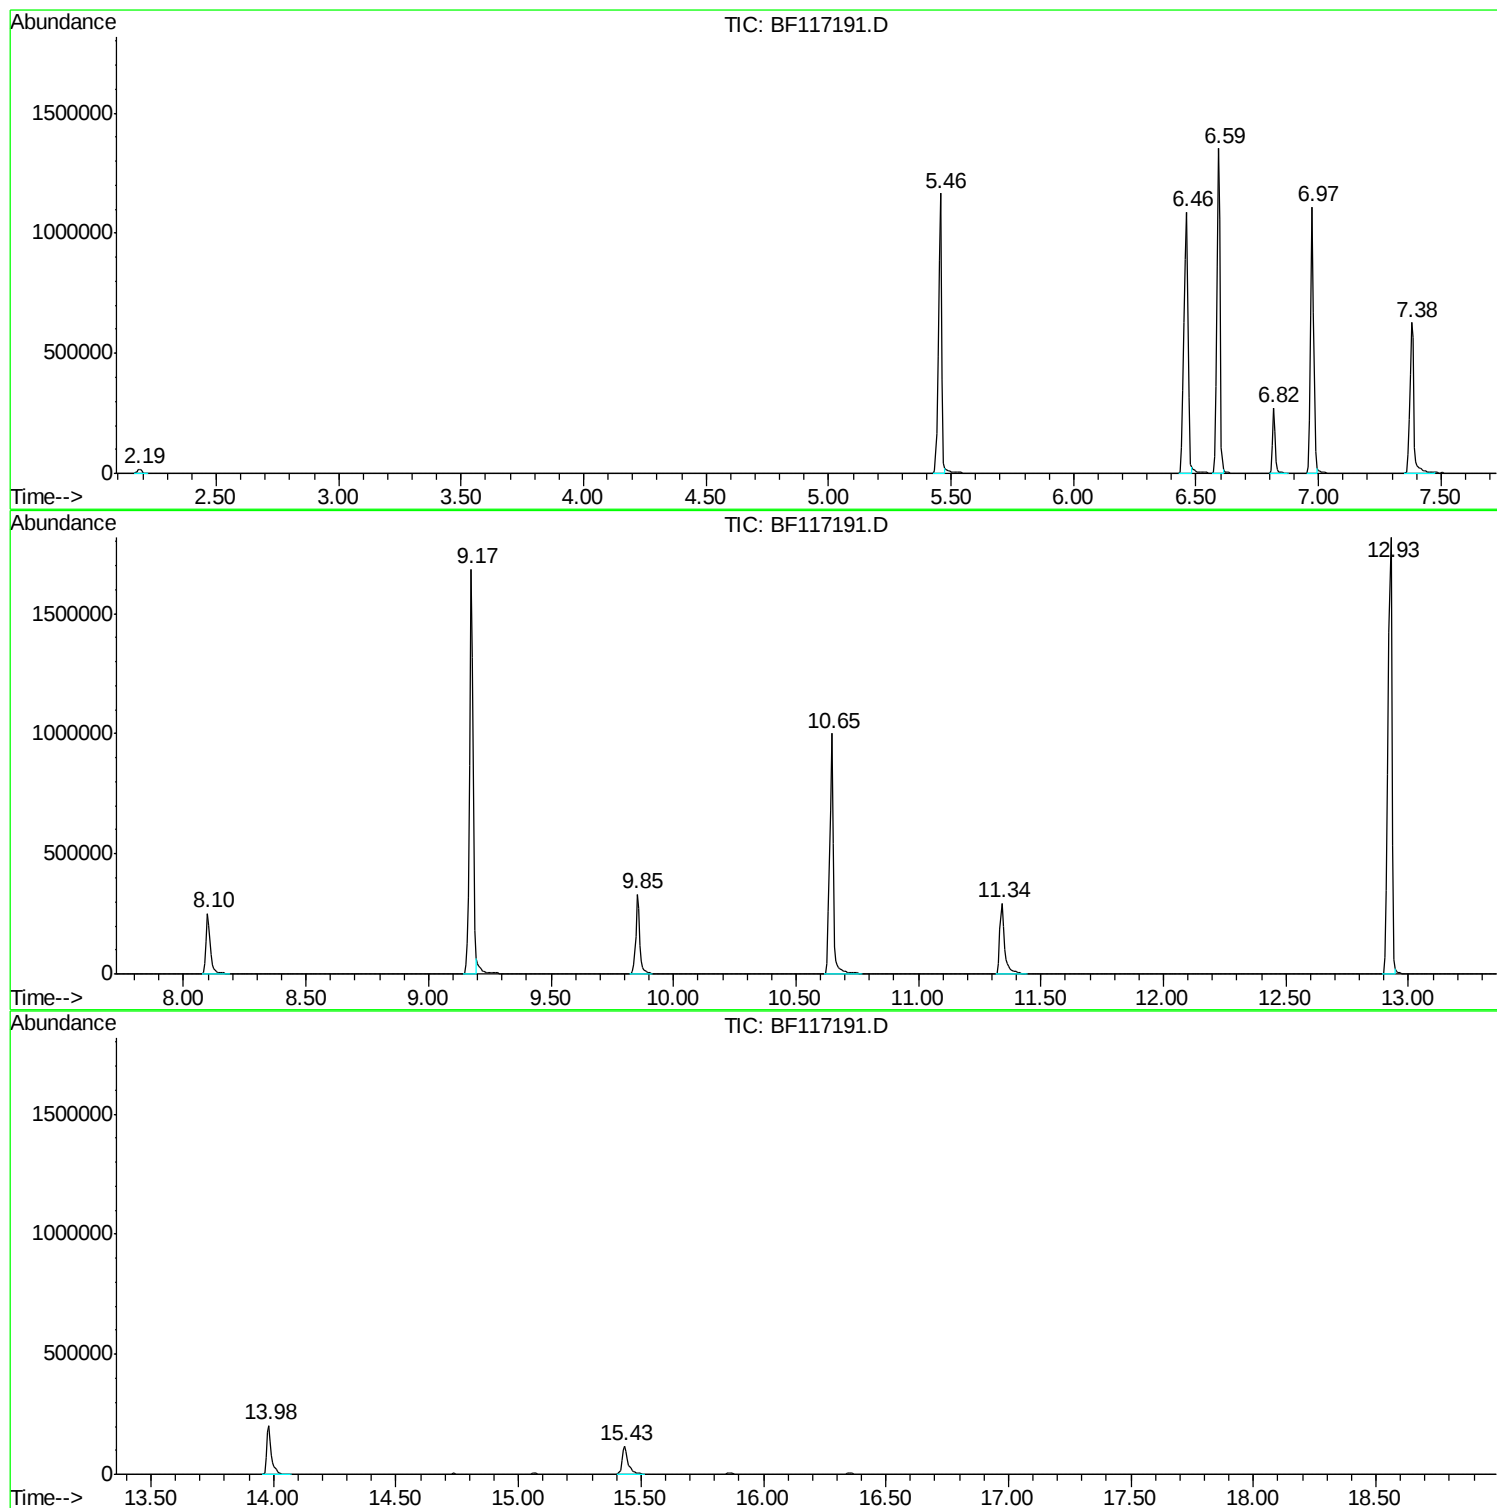

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
Data File : BF117191.D
Acq On : 20 Sep 2019 17:50
Operator : HP/JU
Sample : PB123274BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB123274BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.19 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.19	2.23 ng	26059	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	38
2		N-Ethylformamide	73	C3H7NO	000627-45-2	5
3		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	5
4		Ethyl ether	74	C4H10O	000060-29-7	4
5		Propane, 2-methoxy-2-methyl-	88	C5H12O	001634-04-4	4

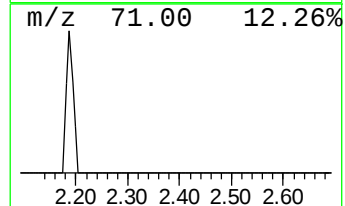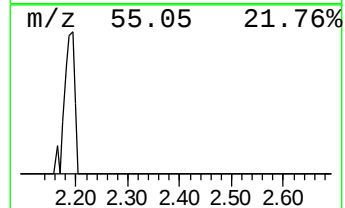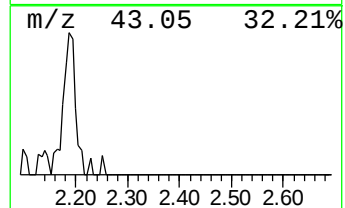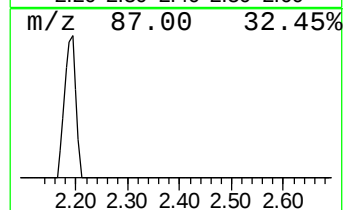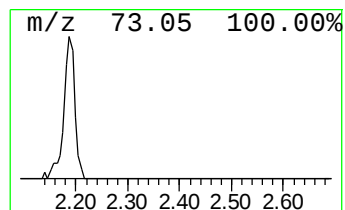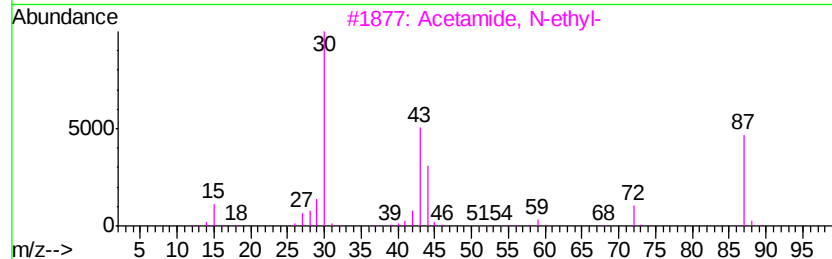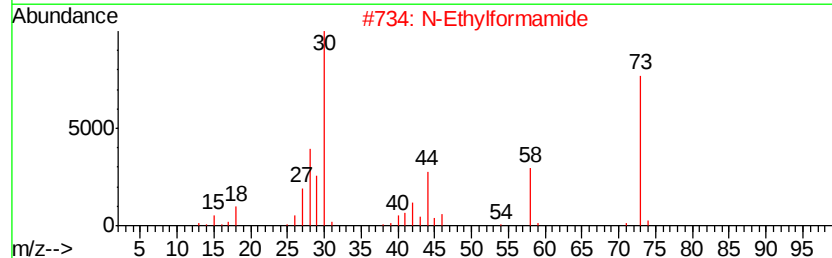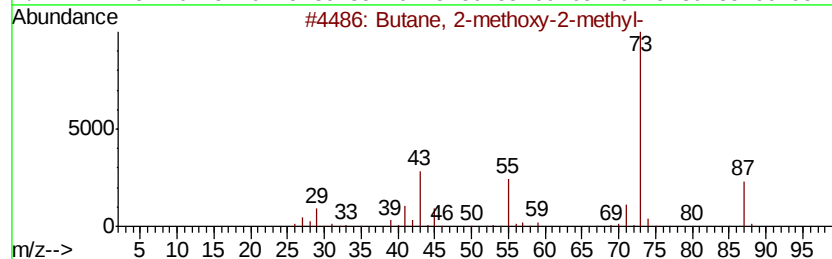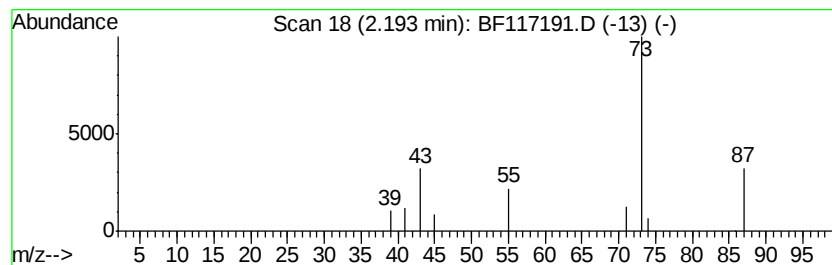

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
Data File : BF117191.D
Acq On : 20 Sep 2019 17:50
Operator : HP/JU
Sample : PB123274BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB123274BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.59 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.59	114.99 ng	1344950	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

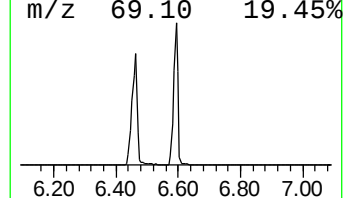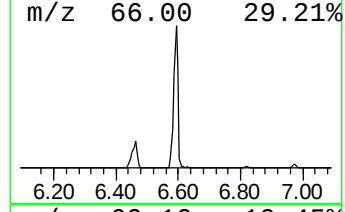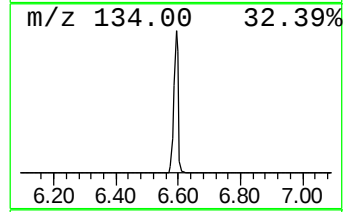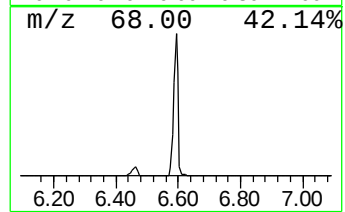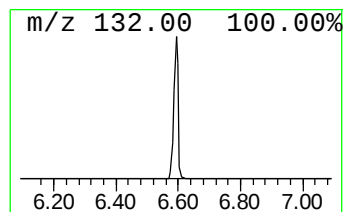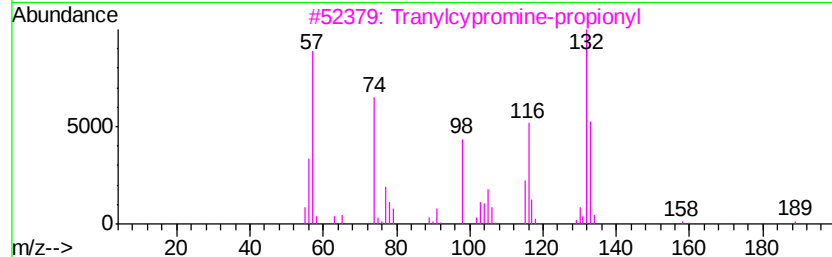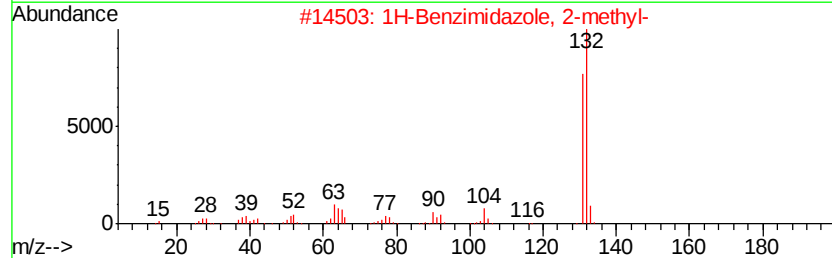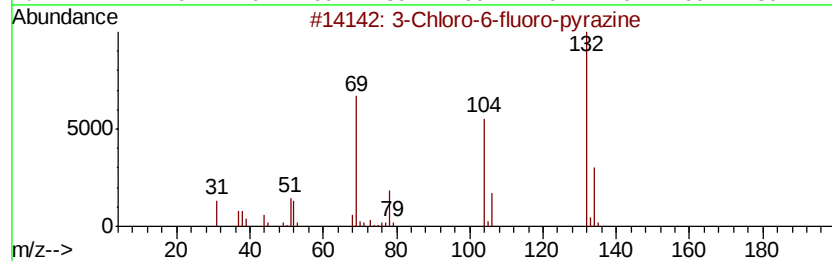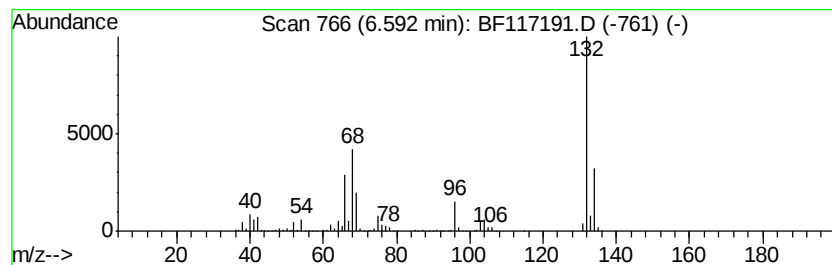

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
Data File : BF117191.D
Acq On : 20 Sep 2019 17:50
Operator : HP/JU
Sample : PB123274BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB123274BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.19	2.19	2.2	ng	26059	1	6.82	233921	20.0
unknown6.59	6.59	115.0	ng	1344950	1	6.82	233921	20.0