

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
 Data File : BF117203.D
 Acq On : 20 Sep 2019 23:09
 Operator : HP/JU
 Sample : K4964-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	6	15	rVB	313987	368629	35.47%	3.521%
2	5.451	568	572	590	rBV	773794	805254	77.49%	7.691%
3	6.469	740	745	761	rBV	834698	900081	86.62%	8.597%
4	6.598	762	767	770	rBV	1053050	950133	91.44%	9.075%
5	6.816	801	804	815	rBV	278234	244212	23.50%	2.332%
6	6.975	827	831	835	rBV	830258	724089	69.68%	6.916%
7	7.381	896	900	912	rBV	501591	554991	53.41%	5.301%
8	8.098	1018	1022	1039	rBV	294329	295272	28.42%	2.820%
9	9.175	1201	1205	1208	rBV	1310101	1039131	100.00%	9.925%
10	9.569	1268	1272	1281	rVB	129033	124322	11.96%	1.187%
11	9.851	1316	1320	1324	rBV	348210	297520	28.63%	2.842%
12	10.069	1351	1357	1368	rBV	71810	101920	9.81%	0.973%
13	10.645	1449	1455	1467	rBV	413708	456569	43.94%	4.361%
14	10.769	1471	1476	1481	rVB3	9705	15628	1.50%	0.149%
15	10.916	1494	1501	1504	rBV4	7349	15557	1.50%	0.149%
16	11.004	1513	1516	1526	rVB3	30159	36249	3.49%	0.346%
17	11.280	1560	1563	1567	rBV	16903	16626	1.60%	0.159%
18	11.339	1569	1573	1575	rBV	235630	218590	21.04%	2.088%
19	11.363	1575	1577	1580	rVB	84882	72735	7.00%	0.695%
20	11.416	1583	1586	1589	rBV	27061	26286	2.53%	0.251%
21	11.574	1610	1613	1620	rBV4	25103	49237	4.74%	0.470%
22	11.680	1627	1631	1635	rVB4	25692	31246	3.01%	0.298%
23	11.868	1655	1663	1669	rBV3	171982	215057	20.70%	2.054%
24	11.951	1674	1677	1680	rBV	42418	39854	3.84%	0.381%
25	12.116	1701	1705	1707	rBV4	16302	19150	1.84%	0.183%
26	12.292	1731	1735	1737	rBV3	13977	17932	1.73%	0.171%
27	12.392	1748	1752	1755	rBV3	40108	64386	6.20%	0.615%
28	12.474	1764	1766	1772	rVB5	25197	30822	2.97%	0.294%
29	12.551	1776	1779	1781	rBV	220064	190266	18.31%	1.817%
30	12.645	1792	1795	1799	rBV4	42954	42844	4.12%	0.409%
31	12.780	1812	1818	1824	rBV	183942	210511	20.26%	2.011%
32	12.921	1837	1842	1849	rVB	685235	662647	63.77%	6.329%
33	12.998	1852	1855	1860	rBV5	18188	31561	3.04%	0.301%
34	13.104	1871	1873	1877	rVB	25755	29254	2.82%	0.279%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
Data File : BF117203.D
Acq On : 20 Sep 2019 23:09
Operator : HP/JU
Sample : K4964-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.174	1882	1885	1888	rBV	17946	18277	1.76%	0.175%
36	13.215	1890	1892	1896	rVB2	22389	19940	1.92%	0.190%
37	13.339	1910	1913	1915	rBV3	16710	15163	1.46%	0.145%
38	13.486	1936	1938	1940	rBV3	14599	14146	1.36%	0.135%
39	13.727	1977	1979	1982	rBV	20813	21661	2.08%	0.207%
40	13.827	1992	1996	2004	rVB5	78172	141400	13.61%	1.350%
41	13.974	2017	2021	2024	rBV2	193691	254270	24.47%	2.429%
42	14.004	2024	2026	2029	rVB	93341	78870	7.59%	0.753%
43	14.133	2046	2048	2049	rBV2	20105	15868	1.53%	0.152%
44	14.809	2160	2163	2169	rVB	79801	95343	9.18%	0.911%
45	15.015	2194	2198	2204	rBV	82495	133302	12.83%	1.273%
46	15.315	2245	2249	2255	rVB	51733	65961	6.35%	0.630%
47	15.374	2255	2259	2264	rBV	71772	99344	9.56%	0.949%
48	15.433	2265	2269	2274	rBV	122548	186860	17.98%	1.785%
49	15.768	2317	2326	2337	rBV10	70830	343486	33.06%	3.281%
50	16.886	2512	2516	2522	rVB4	20054	32875	3.16%	0.314%
51	17.321	2587	2590	2599	rVB3	18050	34918	3.36%	0.333%


Sum of corrected areas: 10470245

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
Data File : BF117203.D
Acq On : 20 Sep 2019 23:09
Operator : HP/JU
Sample : K4964-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
SB-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

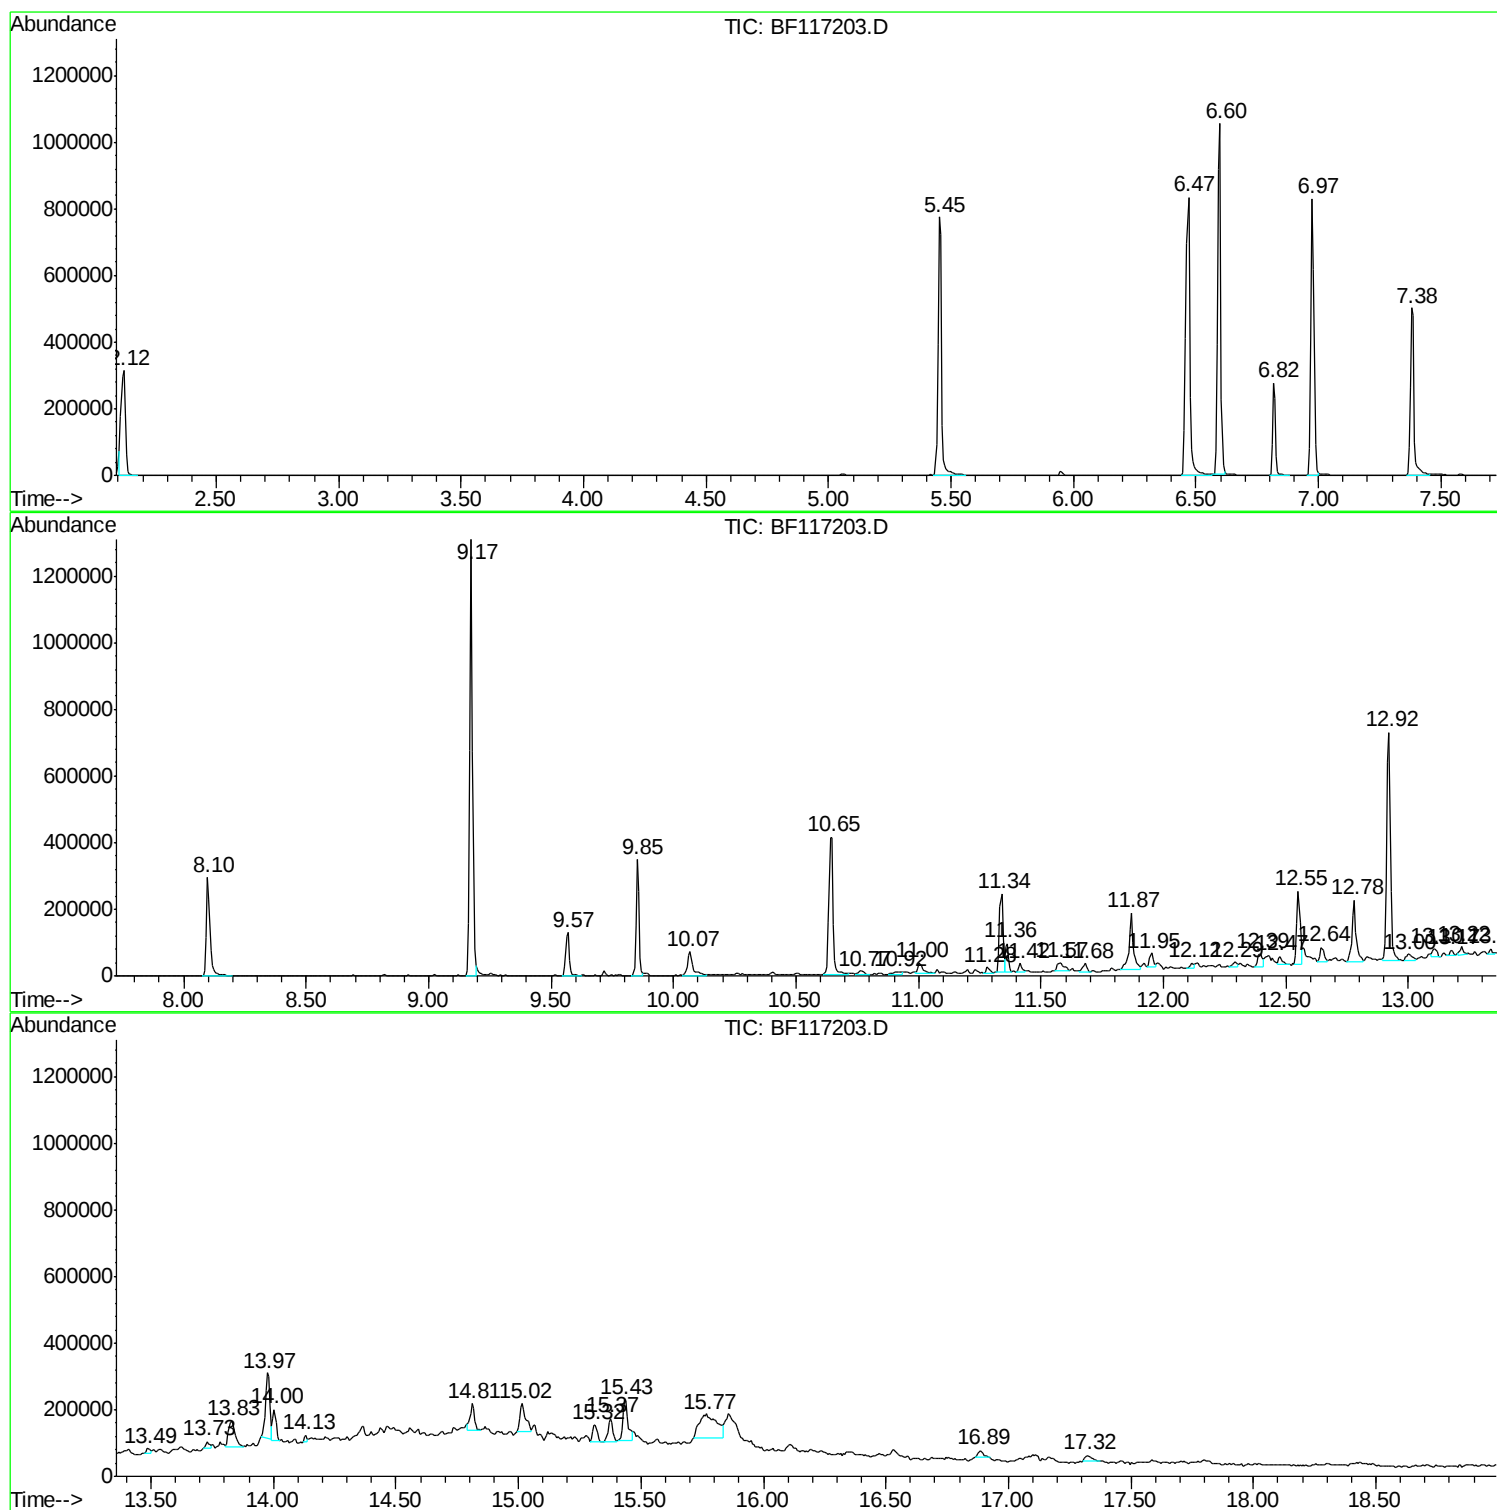

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
Data_File : BF117203.D
Acq_On : 20-Sep-2019 23:099
Operator : HP/JUU
Sample : K4964-022
Misc :
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-2

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
