

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
 Data File : BF117204.D
 Acq On : 20 Sep 2019 23:36
 Operator : HP/JU
 Sample : K4964-02DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-2DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	568	571	582	rBV	103496	128725	41.55%	4.665%
2	6.463	741	744	759	rBV	101787	150834	48.68%	5.466%
3	6.592	763	766	773	rBV	187802	169685	54.77%	6.150%
4	6.816	801	804	814	rBV	252859	227865	73.55%	8.258%
5	6.975	827	831	841	rBV	143301	133531	43.10%	4.839%
6	7.381	897	900	912	rBV	62519	84646	27.32%	3.068%
7	8.098	1018	1022	1039	rBV	262356	291861	94.20%	10.577%
8	9.175	1201	1205	1216	rBV	180073	183745	59.31%	6.659%
9	9.569	1269	1272	1280	rBV	16840	19003	6.13%	0.689%
10	9.851	1317	1320	1332	rVB	344001	309825	100.00%	11.228%
11	10.645	1452	1455	1463	rBV	66470	69568	22.45%	2.521%
12	11.339	1569	1573	1581	rBV	249604	241841	78.06%	8.764%
13	11.422	1584	1587	1592	rVB2	3450	4493	1.45%	0.163%
14	11.586	1610	1615	1619	rBV5	3402	6838	2.21%	0.248%
15	11.686	1629	1632	1633	rBV2	3638	3666	1.18%	0.133%
16	11.863	1657	1662	1671	rBV4	11488	21096	6.81%	0.765%
17	11.951	1674	1677	1681	rBV4	5058	6733	2.17%	0.244%
18	12.398	1749	1753	1755	rBV3	5540	7104	2.29%	0.257%
19	12.551	1777	1779	1783	rBV	33503	32837	10.60%	1.190%
20	12.645	1791	1795	1800	rVB7	4466	7659	2.47%	0.278%
21	12.780	1813	1818	1823	rBV	32675	33461	10.80%	1.213%
22	12.916	1838	1841	1848	rBV	137656	122085	39.40%	4.424%
23	13.004	1854	1856	1858	rBV3	3544	3840	1.24%	0.139%
24	13.092	1867	1871	1872	rBV3	4894	6011	1.94%	0.218%
25	13.186	1883	1887	1888	rBV3	2926	3691	1.19%	0.134%
26	13.210	1888	1891	1892	rBV3	3645	3529	1.14%	0.128%
27	13.274	1900	1902	1905	rBV3	4550	5583	1.80%	0.202%
28	13.333	1910	1912	1916	rVV4	4505	4634	1.50%	0.168%
29	13.639	1958	1964	1965	rBV5	10888	17271	5.57%	0.626%
30	13.827	1993	1996	2003	rVB9	10934	19690	6.36%	0.714%
31	13.974	2017	2021	2025	rBV	153127	183169	59.12%	6.638%
32	14.086	2038	2040	2042	rBV3	5636	5203	1.68%	0.189%
33	14.433	2097	2099	2102	rBV3	9344	9696	3.13%	0.351%
34	14.810	2160	2163	2165	rVB3	15258	14386	4.64%	0.521%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
Data File : BF117204.D
Acq On : 20 Sep 2019 23:36
Operator : HP/JU
Sample : K4964-02DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-2DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.010	2195	2197	2201	rVB3	10930	14744	4.76%	0.534%
36	15.368	2255	2258	2263	rBV2	14602	17832	5.76%	0.646%
37	15.433	2264	2269	2277	rVB	109456	148085	47.80%	5.367%
38	15.545	2286	2288	2289	rBV2	8080	7136	2.30%	0.259%
39	16.798	2499	2501	2503	rBV2	4290	4788	1.55%	0.174%
40	16.886	2514	2516	2519	rBV3	4714	5104	1.65%	0.185%
41	17.086	2547	2550	2551	rBV3	4373	4094	1.32%	0.148%
42	17.315	2588	2589	2598	rVB8	7105	10679	3.45%	0.387%
43	18.009	2704	2707	2709	rBV4	4041	5197	1.68%	0.188%
44	18.092	2719	2721	2726	rVB5	2889	4277	1.38%	0.155%
45	18.339	2762	2763	2768	rBV5	3901	3588	1.16%	0.130%


Sum of corrected areas: 2759328

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092019\
Data File : BF117204.D
Acq On : 20 Sep 2019 23:36
Operator : HP/JU
Sample : K4964-02DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-2DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

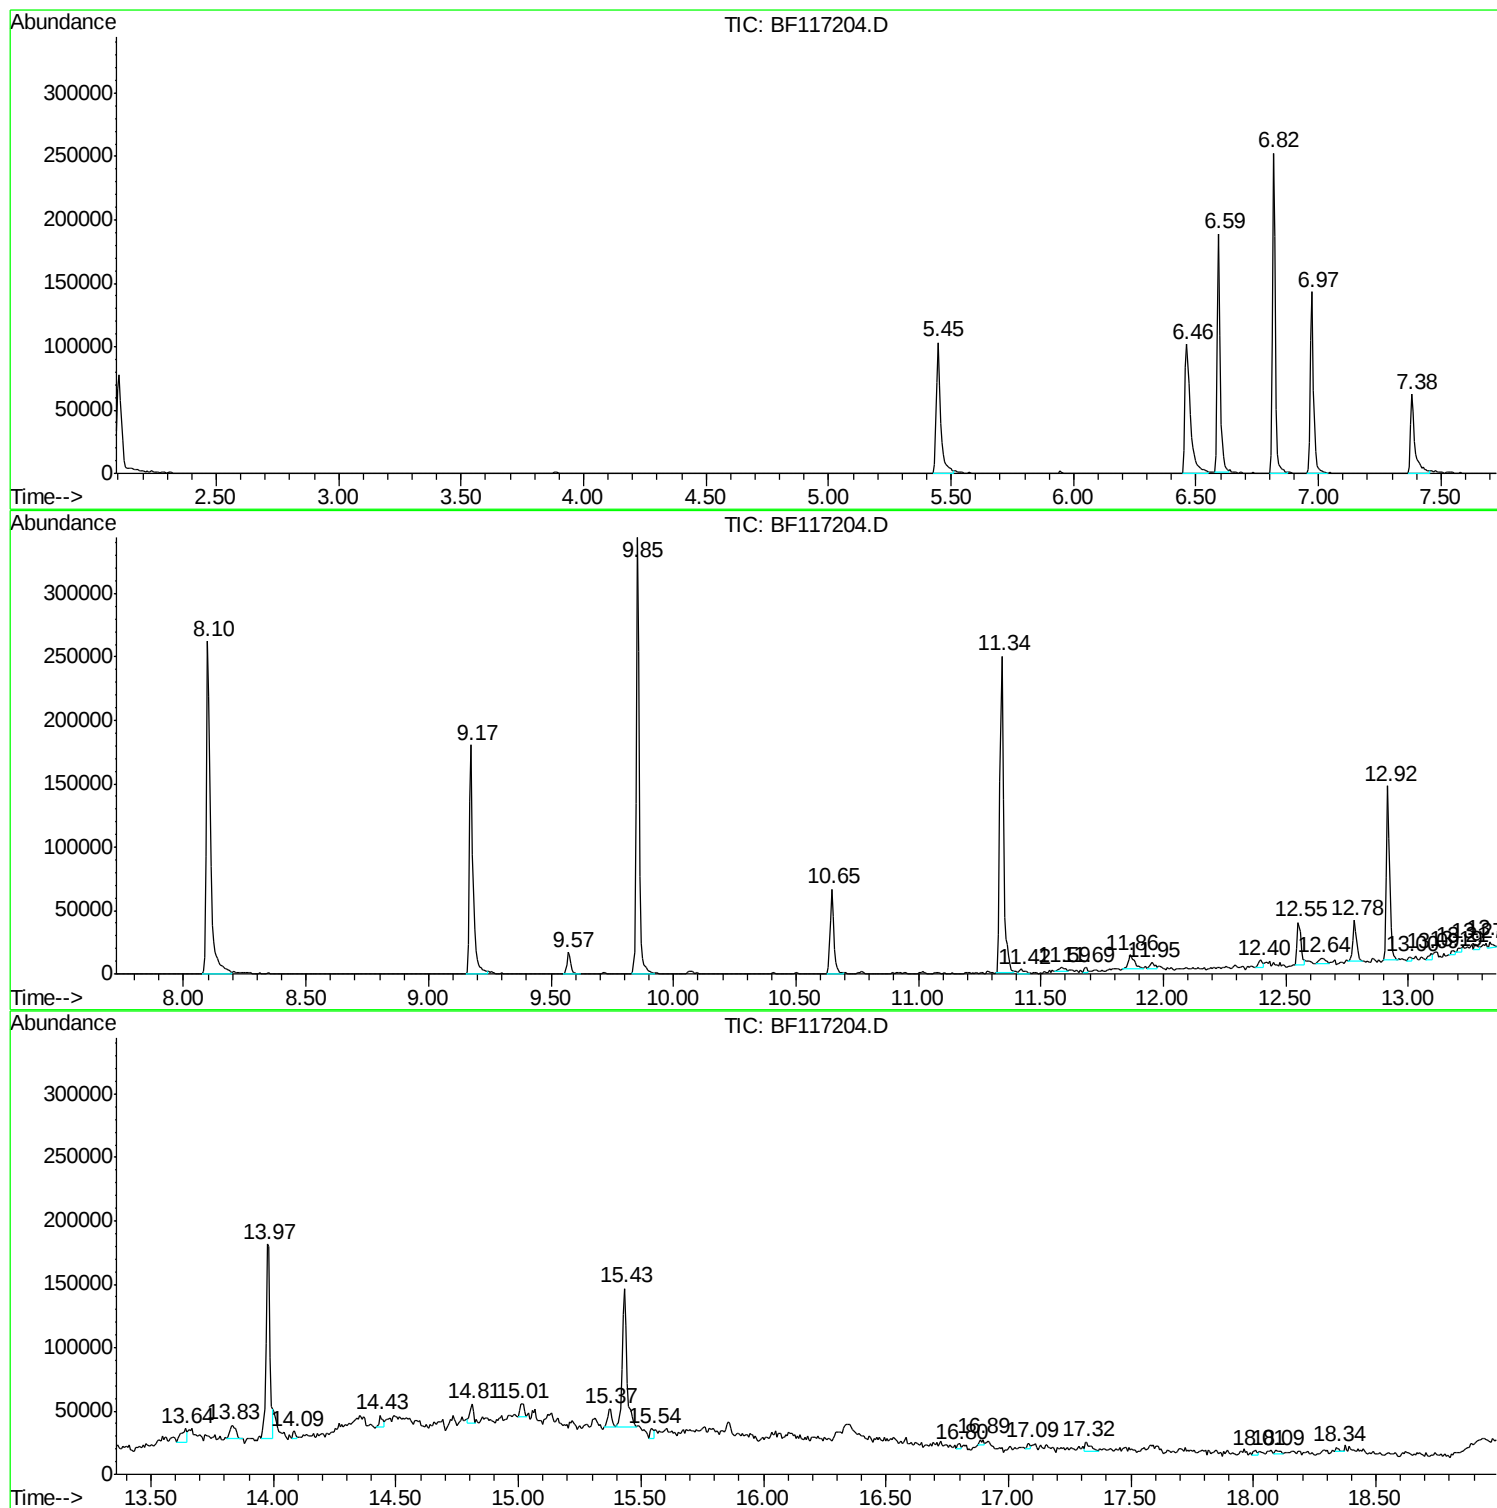

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
Data_File : BF117204.D
Acq_On : 20-Sep-2019 23:366
Operator : HP/JUU
Sample : K4964-02DL_5XX
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SB-2DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
