


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092019\
 Data File : BF117184.D
 Acq On : 20 Sep 2019 13:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

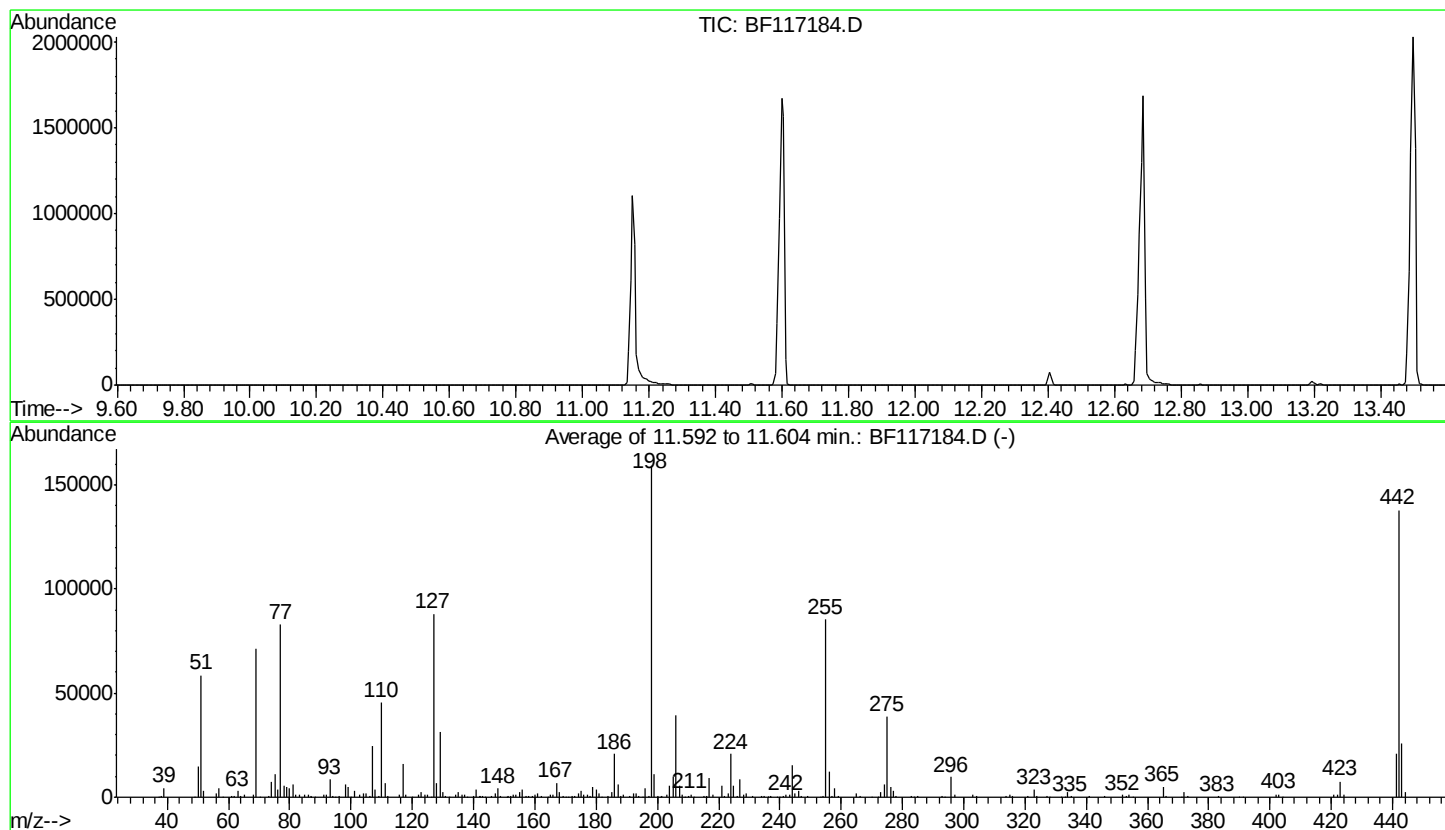

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	58368	PASS
68	69	0.00	2	1.4	1020	PASS
69	198	0.00	100	44.7	71192	PASS
70	69	0.00	2	0.4	275	PASS
127	198	10	80	55.3	87989	PASS
197	198	0.00	2	0.6	889	PASS
198	198	100	100	100.0	159117	PASS
199	198	5	9	6.8	10802	PASS
275	198	10	60	24.3	38701	PASS
365	198	1	100	3.2	5064	PASS
441	198	0.01	100	13.2	20977	PASS
442	198	50	100	86.6	137773	PASS
443	442	15	24	18.9	26030	PASS