

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
 Data File : BF135350.D
 Acq On : 20 Sep 2023 11:21
 Operator : CG\JU
 Sample : PB155675BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155675BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	492	498	512	rBV	83809	127166	3.11%	0.485%
2	5.398	558	563	583	rBV	3528233	3851002	94.15%	14.687%
3	6.404	729	734	737	rBV	3390044	3727618	91.13%	14.217%
4	6.757	790	794	802	rBV	945731	803048	19.63%	3.063%
5	7.322	885	890	893	rBV	2395741	2547721	62.29%	9.717%
6	8.034	1006	1011	1028	rBV	1102941	1077678	26.35%	4.110%
7	9.116	1189	1195	1198	rBV	3952212	4090300	100.00%	15.600%
8	9.792	1304	1310	1326	rBV	1316689	1156255	28.27%	4.410%
9	10.586	1441	1445	1472	rVB	2265320	2502710	61.19%	9.545%
10	11.286	1560	1564	1575	rBV	1443048	1199001	29.31%	4.573%
11	12.886	1831	1836	1839	rBV	3603750	3649677	89.23%	13.919%
12	13.939	2011	2015	2026	rBV	722827	769397	18.81%	2.934%
13	15.410	2260	2265	2277	rBV	499868	718724	17.57%	2.741%




Sum of corrected areas: 26220297

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
Data File : BF135350.D
Acq On : 20 Sep 2023 11:21
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

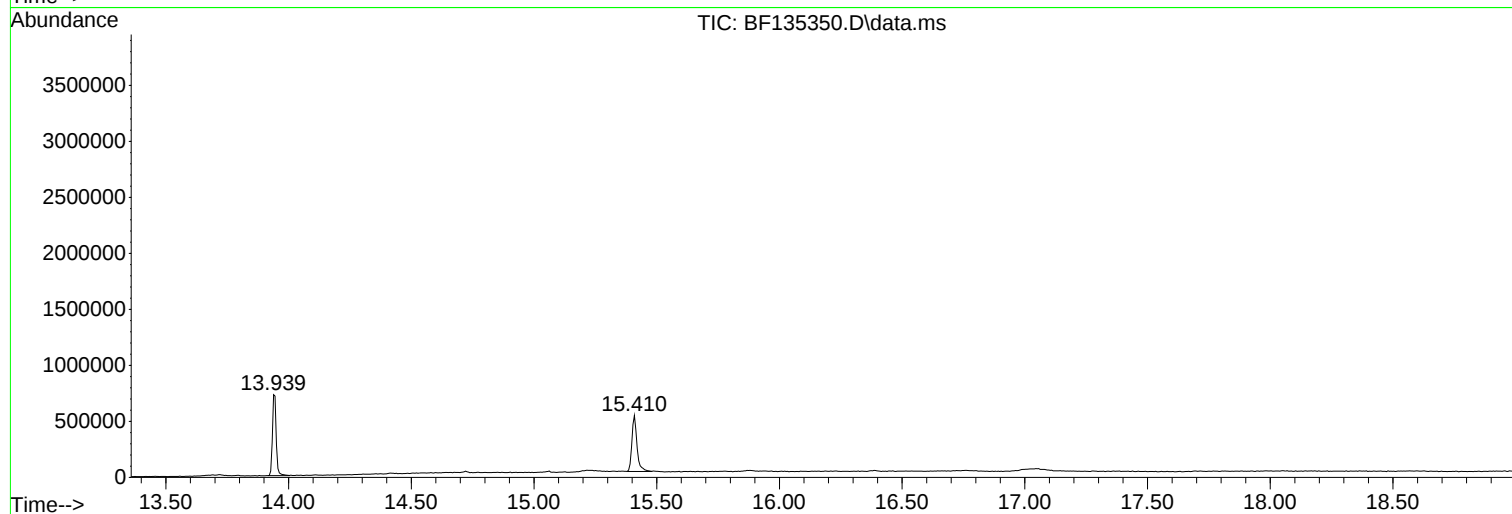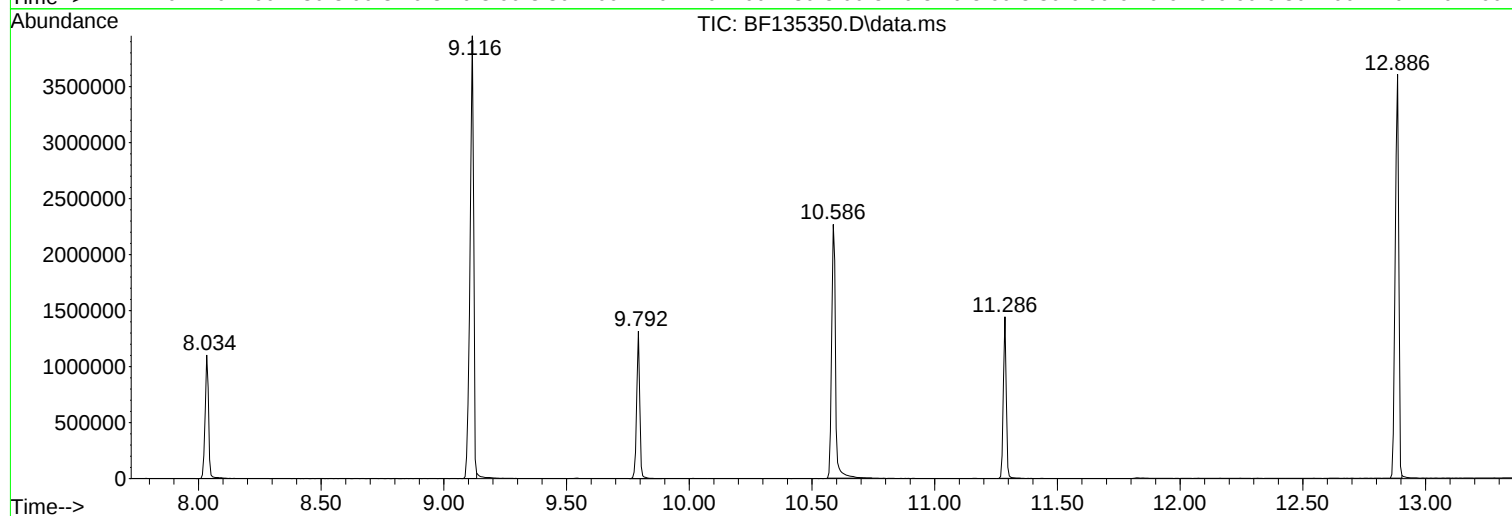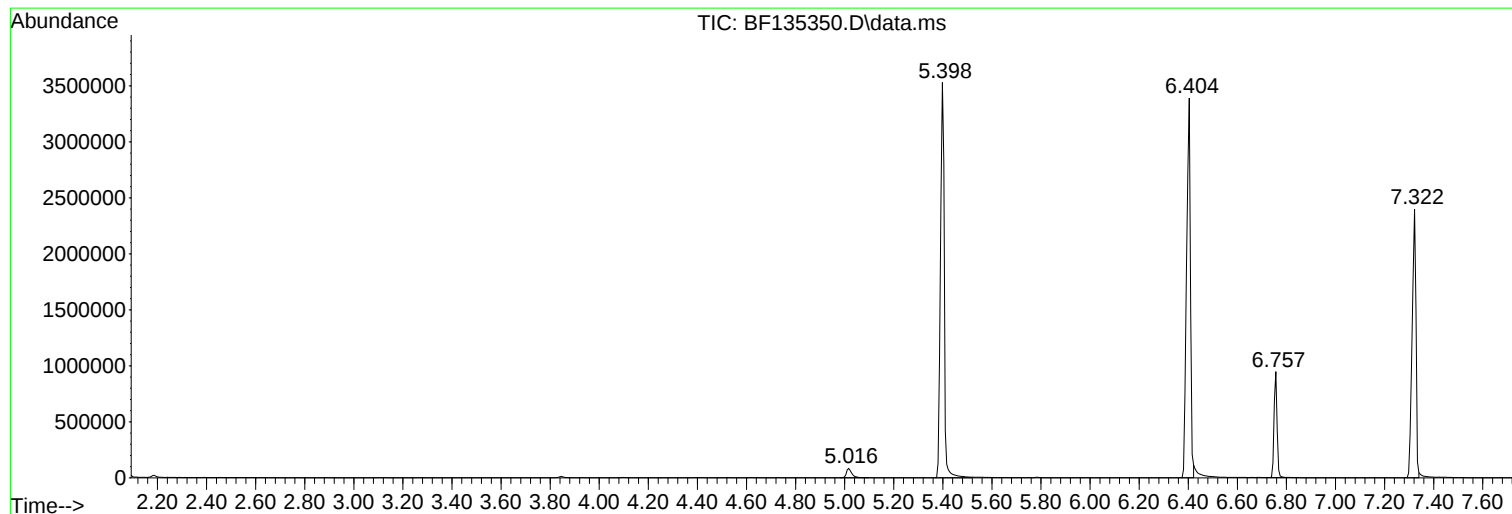

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
Data File : BF135350.D
Acq On : 20 Sep 2023 11:21
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	3.17 ng	127166	1,4-Dichlorobenzene-d4	6.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16		
4	1,3,4-Oxadiazole, 2-(acetyloxy)-...	172	C7H12N2O3	066398-57-0	12		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

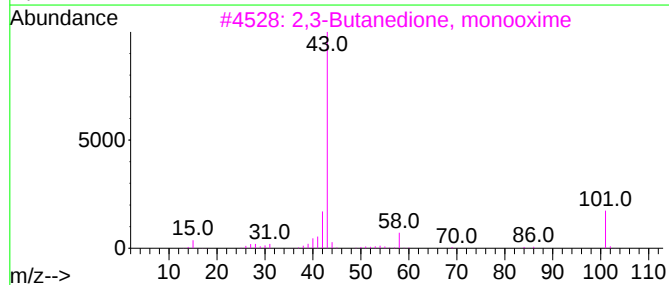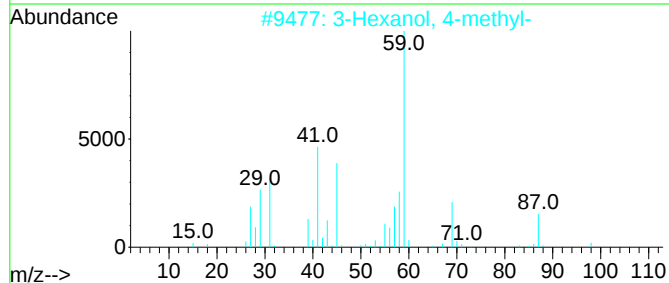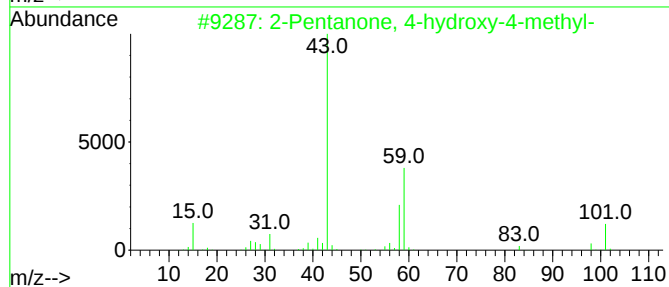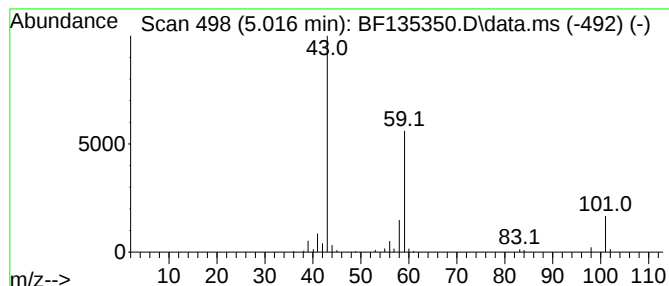

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
Data File : BF135350.D
Acq On : 20 Sep 2023 11:21
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	3.2	ng	127166	1	6.757	803048	20.0