


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
Data File : BF135348.D
Acq On : 20 Sep 2023 09:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

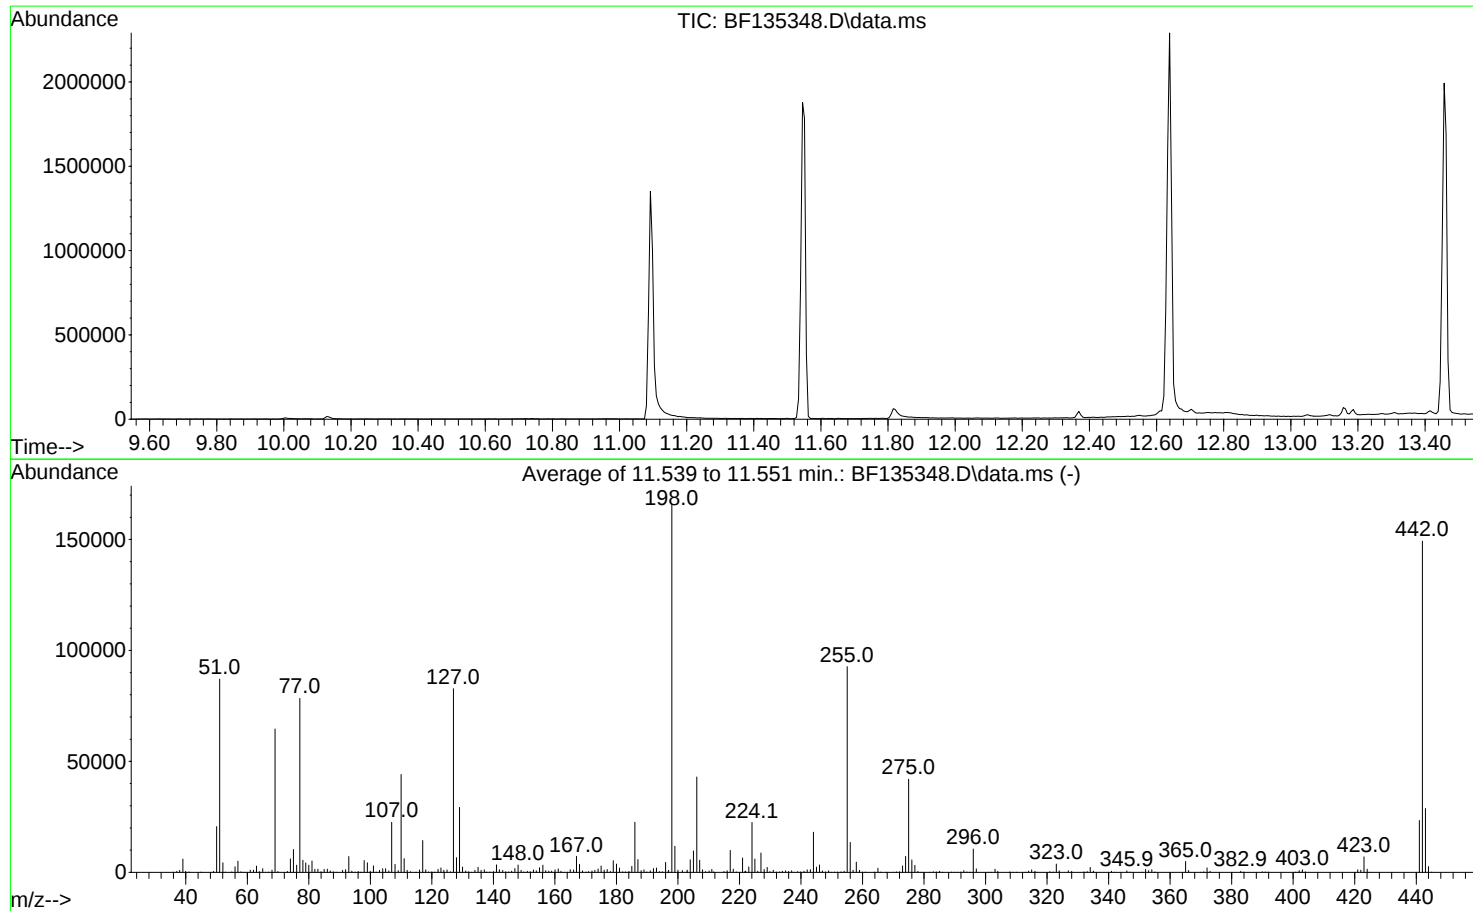




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.5	87064	PASS
68	69	0.00	2	1.6	1035	PASS
69	198	0.00	100	39.0	64592	PASS
70	69	0.00	2	0.5	329	PASS
127	198	10	80	50.0	82795	PASS
197	198	0.00	2	0.6	972	PASS
198	198	100	100	100.0	165749	PASS
199	198	5	9	7.1	11720	PASS
275	198	10	60	25.3	41992	PASS
365	198	1	100	3.0	4941	PASS
441	198	0.01	100	14.1	23357	PASS
442	442	50	100	100.0	149264	PASS
443	442	15	24	19.3	28765	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
Data File : BF135348.D
Acq On : 20 Sep 2023 09:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 21 02:28:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

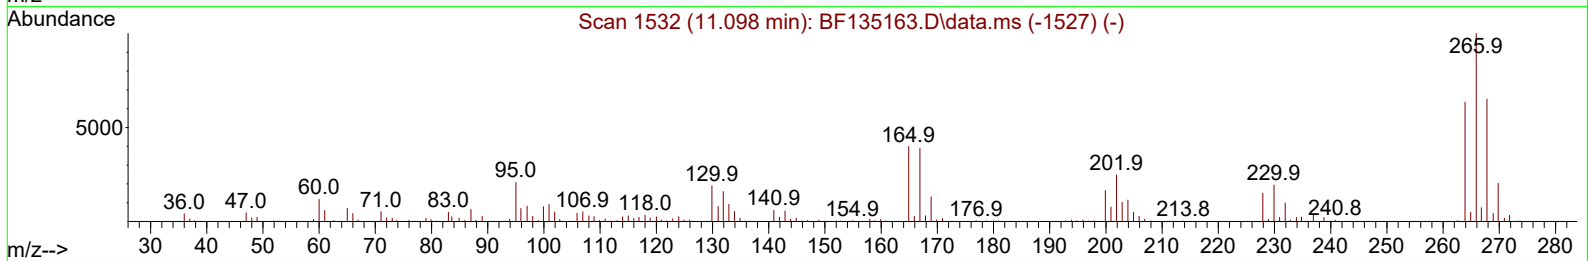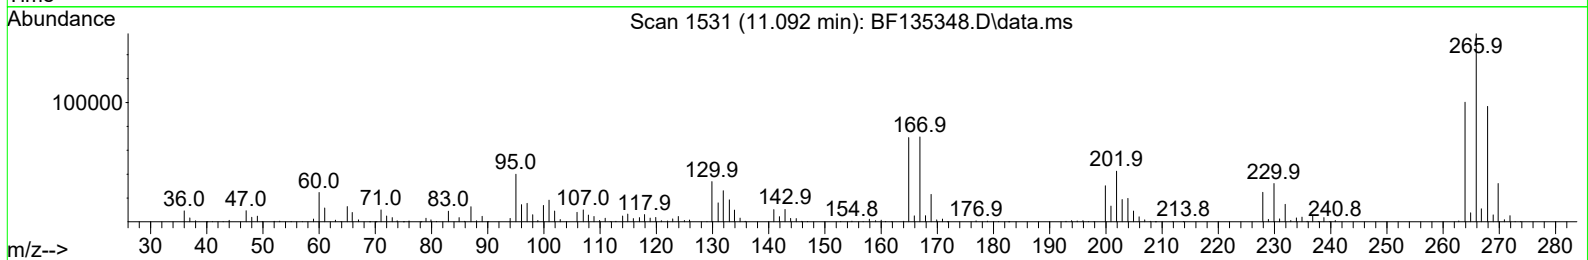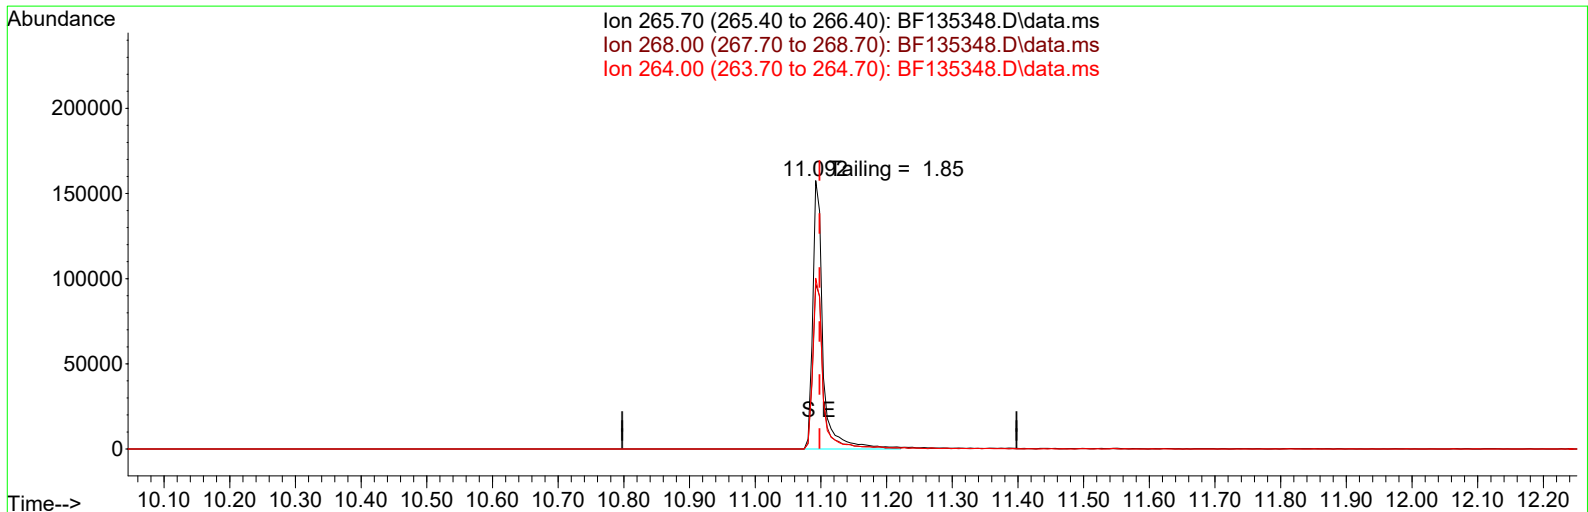

TIC: BF135348.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 35183.48 ng




response 173618

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.37
264.00	63.50	63.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092023\
 Data File : BF135348.D
 Acq On : 20 Sep 2023 09:50
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 21 02:28:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

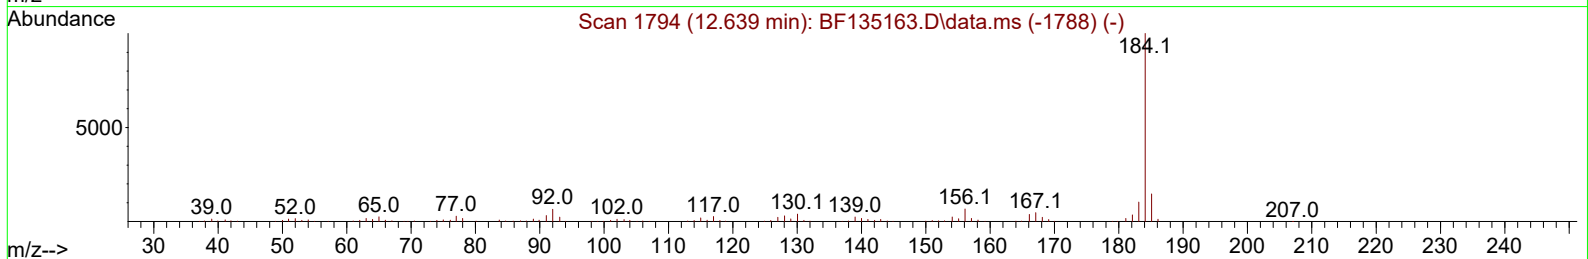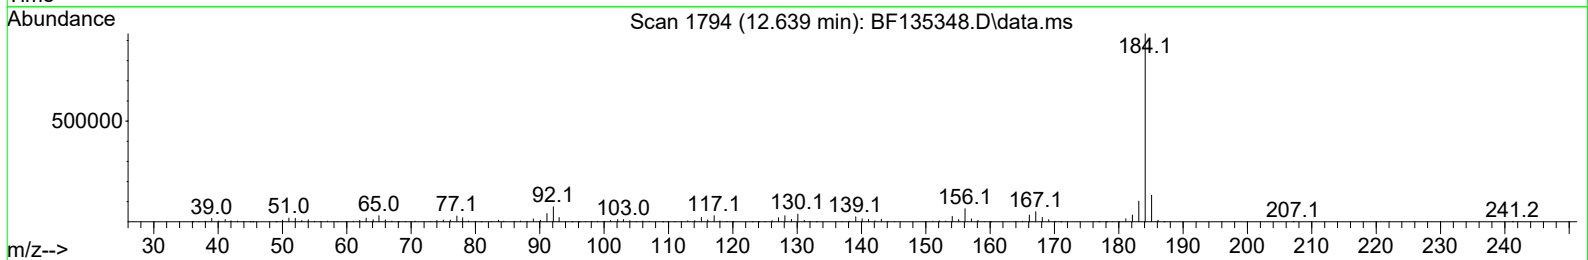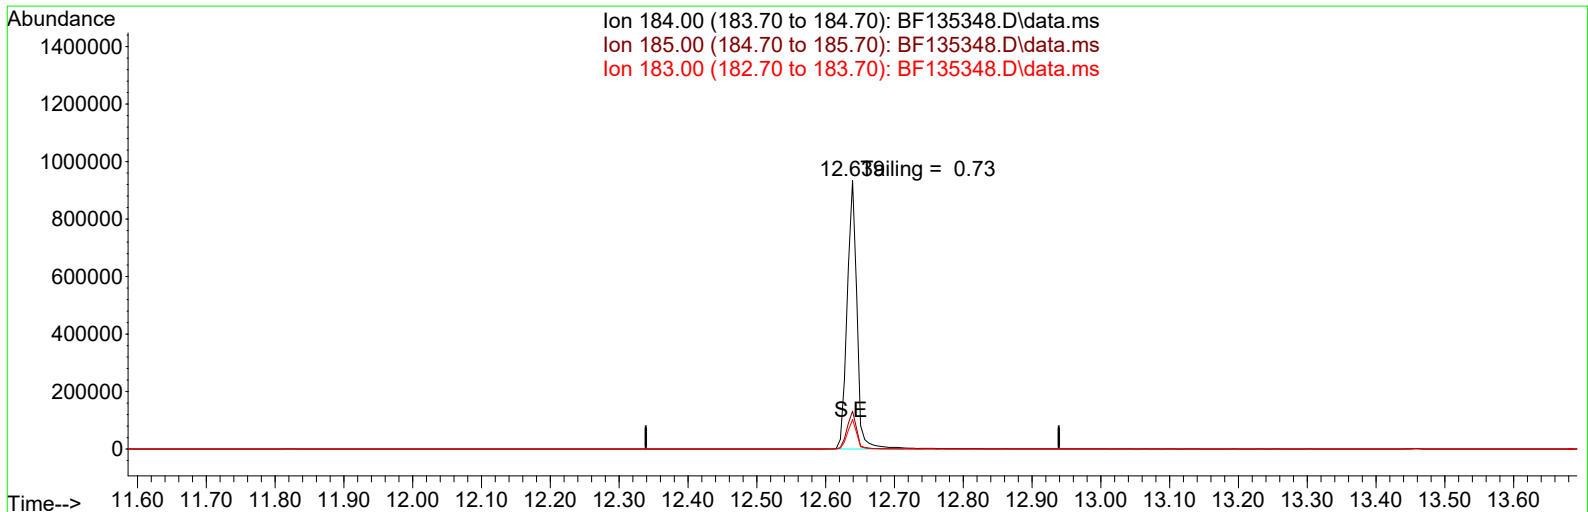

TIC: BF135348.D\data.ms

(77) Benzidine

12.639min (-12.639) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.60	0.00#
183.00	10.30	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2023	BNA_F	<u>BF135348.D</u>
Compound Name	Response	Retention Time
DDT	364279	13.457
DDD	13695	13.157
DDE	587	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14282	378561	3.77

Instrument :
BNA_F
ClientSampleId :
DFTPP