
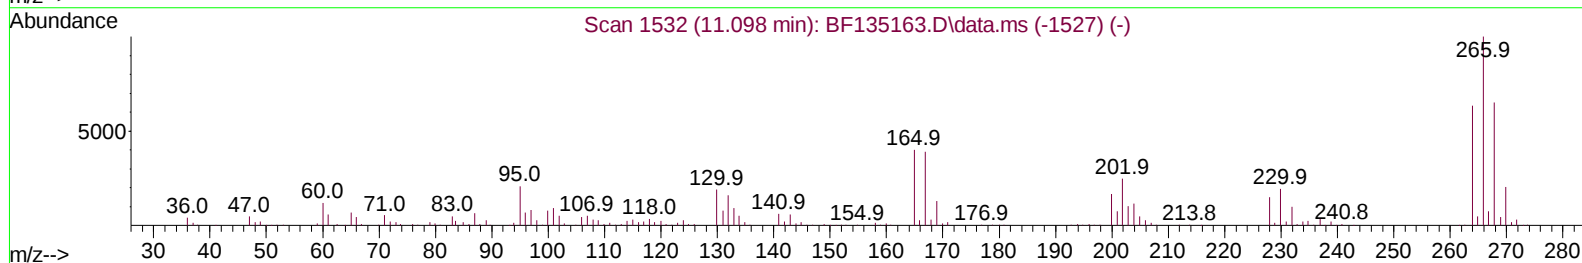
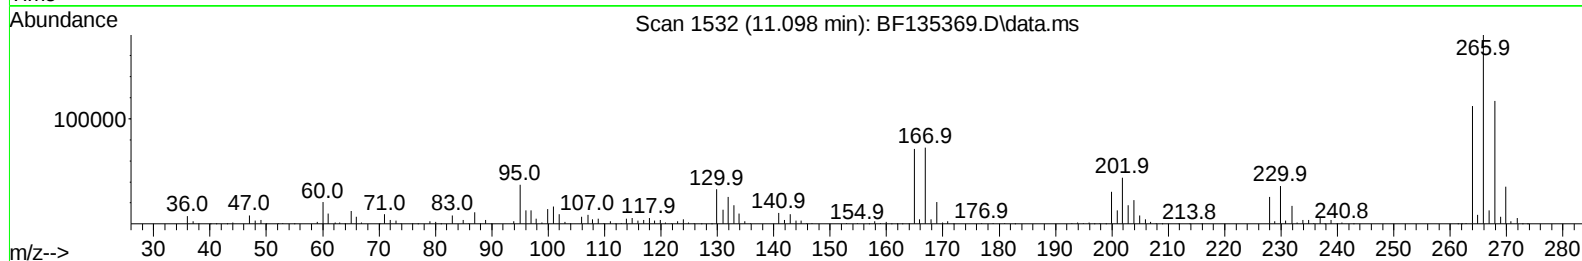


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092123\
Data File : BF135369.D
Acq On : 21 Sep 2023 09:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 06:52:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

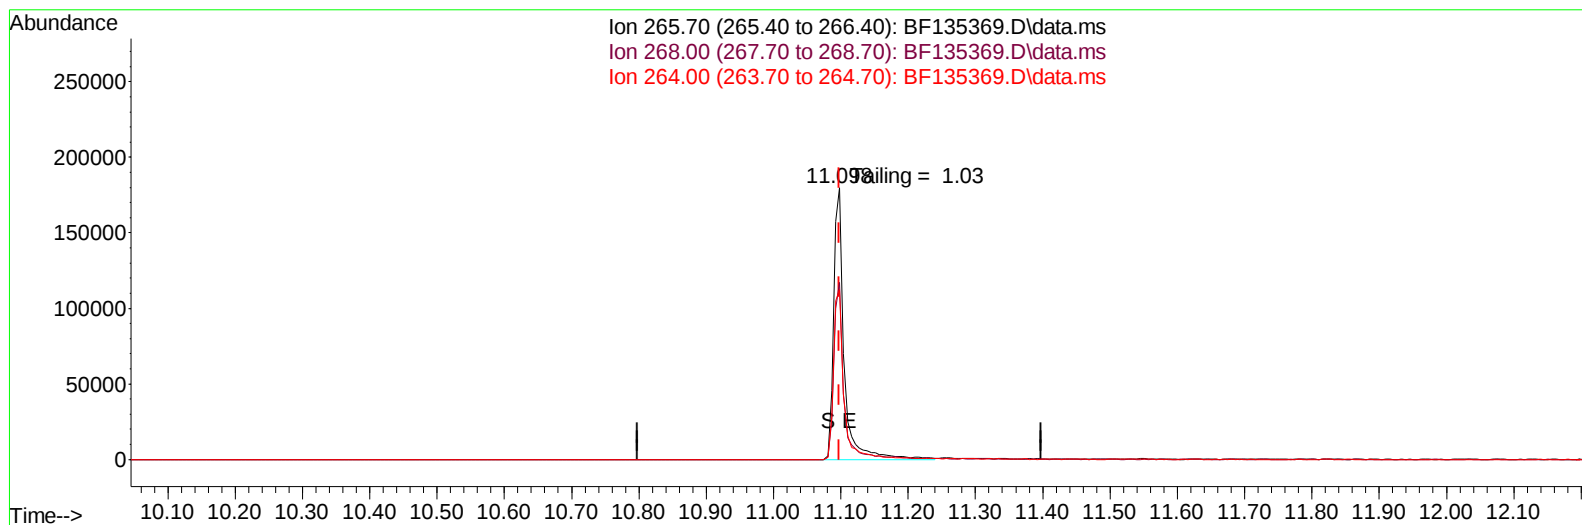

TIC: BF135369.D\data.ms

(70) Pentachlorophenol (C)




11.098min (+ 0.000) 215033.53 ng

response 195537

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	65.16
264.00	63.50	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092123\
Data File : BF135369.D
Acq On : 21 Sep 2023 09:21
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 06:52:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

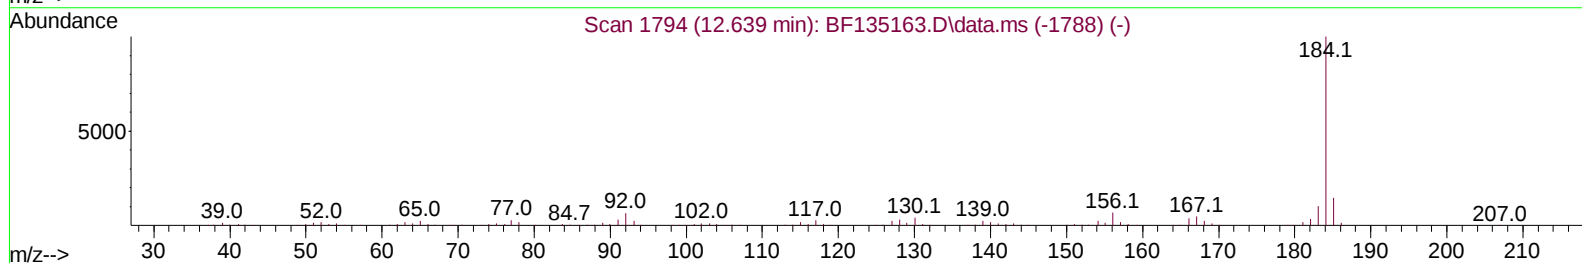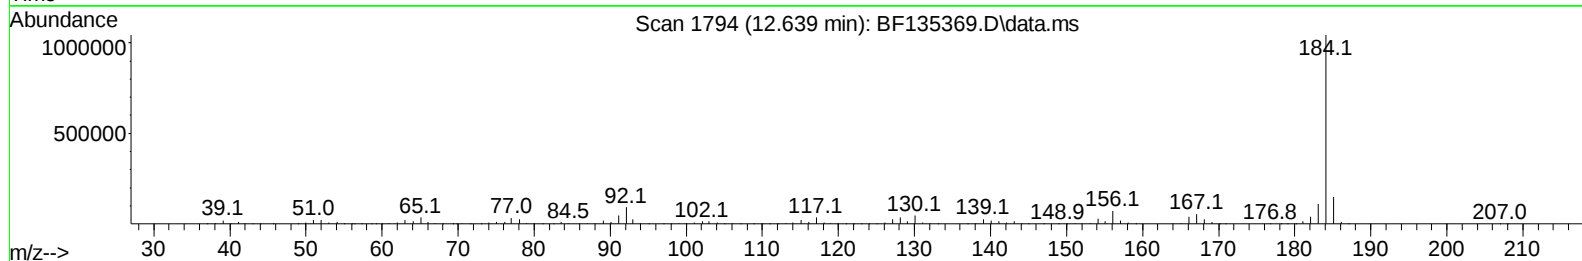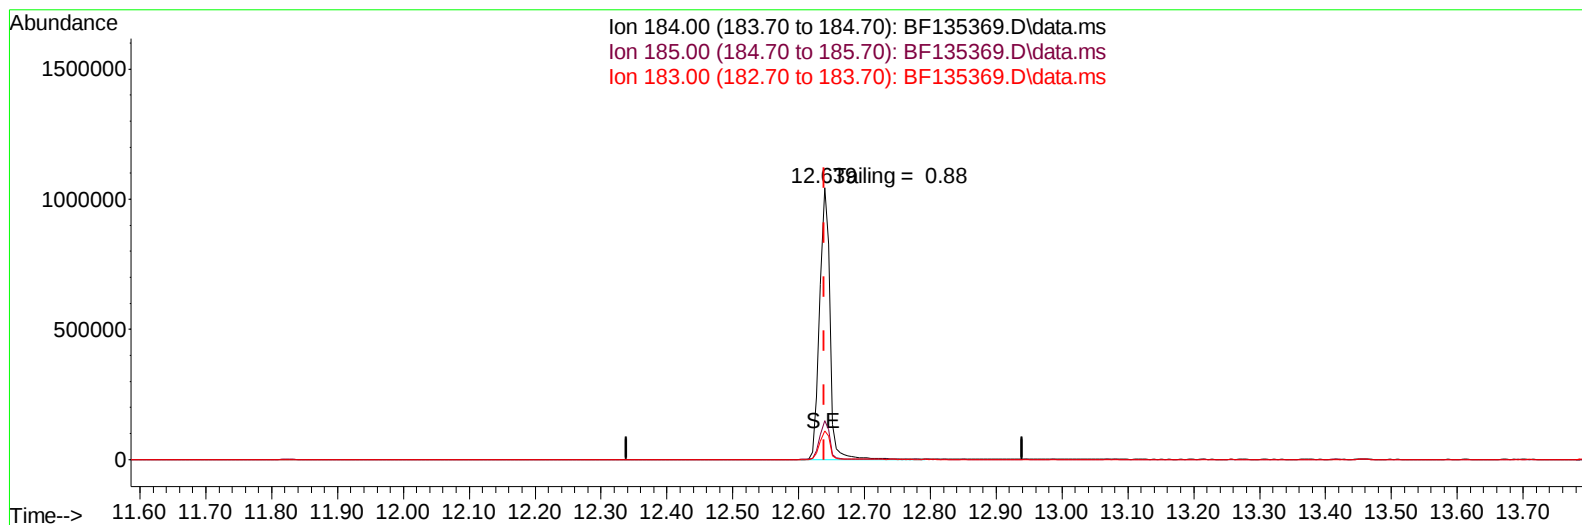

TIC: BF135369.D\data.ms

(77) Benzidine

12.639min (+ 0.000) 117946.85 ng

response 1101859

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.39
183.00	10.30	10.56
0.00	0.00	0.00