

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092123\
 Data File : BF135371.D
 Acq On : 21 Sep 2023 10:21
 Operator : CG\JU
 Sample : PB155710BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155710BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	559	563	582	rBV	3787781	4405702	96.53%	15.298%
2	6.410	729	735	737	rBV	3479845	4323263	94.72%	15.012%
3	6.757	790	794	805	rVB	1049660	846321	18.54%	2.939%
4	7.322	885	890	893	rBV	2508178	2968927	65.05%	10.309%
5	8.034	1007	1011	1015	rBV	1202805	1109477	24.31%	3.853%
6	9.116	1189	1195	1198	rBV	4239409	4564209	100.00%	15.849%
7	9.792	1305	1310	1323	rBV	1395268	1198754	26.26%	4.163%
8	10.592	1441	1446	1449	rBV	2476739	2607236	57.12%	9.053%
9	11.286	1560	1564	1573	rBV	1426600	1211367	26.54%	4.206%
10	12.886	1831	1836	1839	rBV	3732772	4008987	87.84%	13.921%
11	13.945	2012	2016	2028	rBV	797312	813638	17.83%	2.825%
12	15.409	2260	2265	2277	rBV	510183	740705	16.23%	2.572%




Sum of corrected areas: 28798586

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092123\
Data File : BF135371.D
Acq On : 21 Sep 2023 10:21
Operator : CG\JU
Sample : PB155710BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155710BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

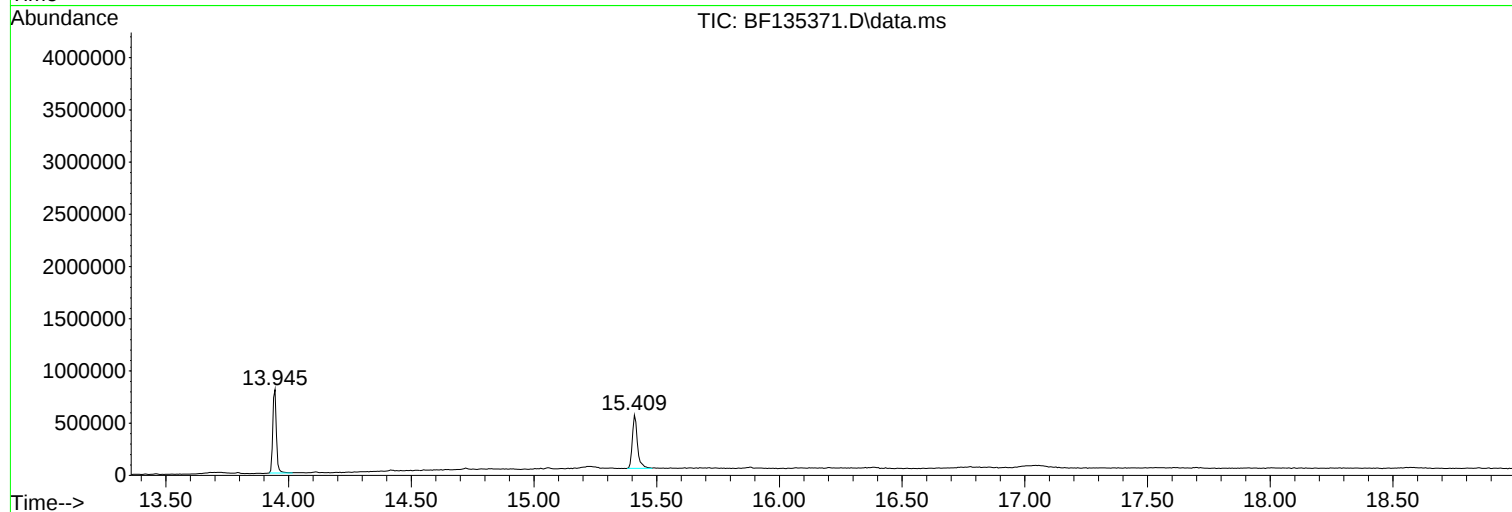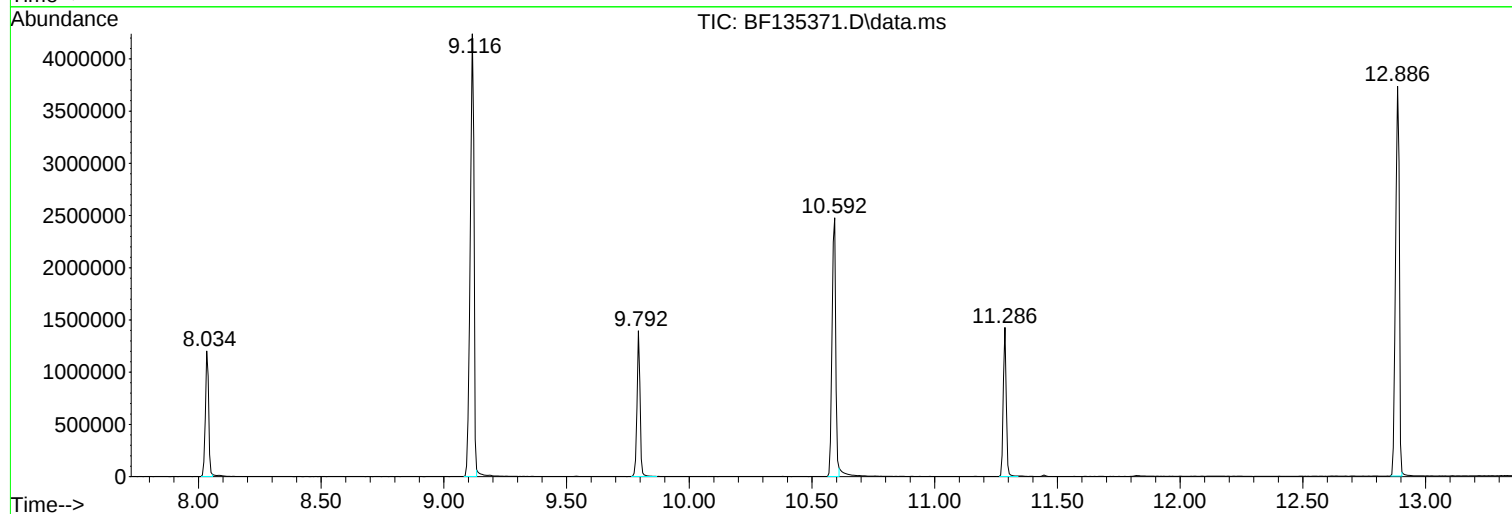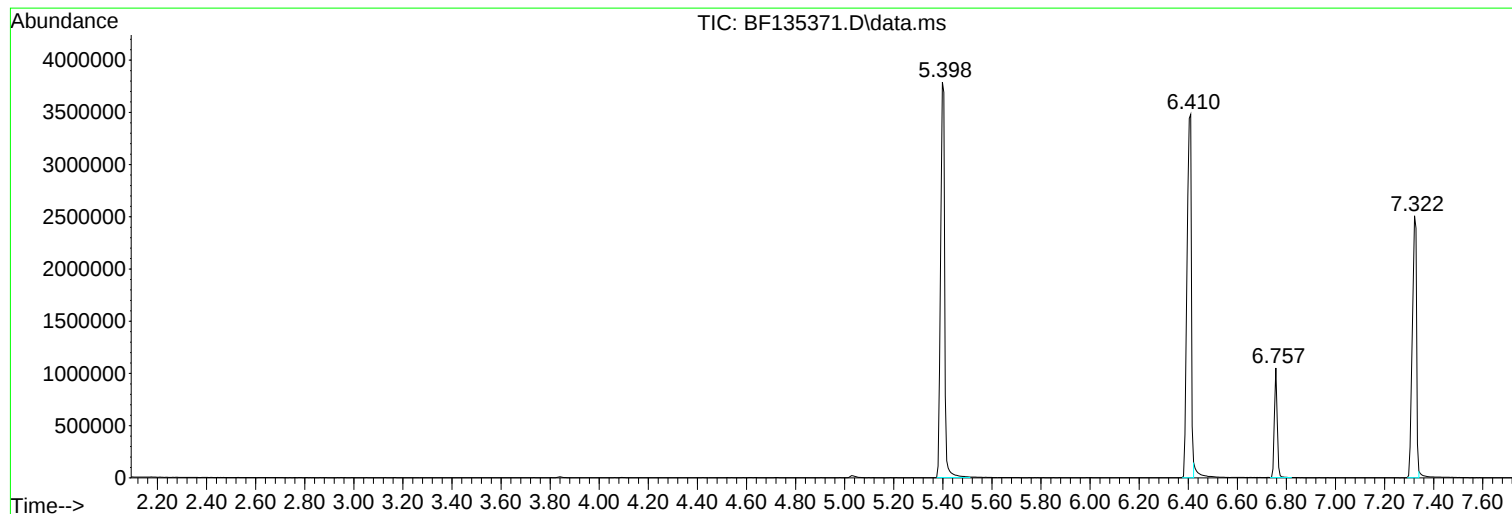

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092123\
Data File : BF135371.D
Acq On : 21 Sep 2023 10:21
Operator : CG\JU
Sample : PB155710BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155710BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092123\
Data File : BF135371.D
Acq On : 21 Sep 2023 10:21
Operator : CG\JU
Sample : PB155710BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155710BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------