


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092123\  
 Data File : BF135369.D  
 Acq On : 21 Sep 2023 09:21  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Sep 12 00:19:07 2023

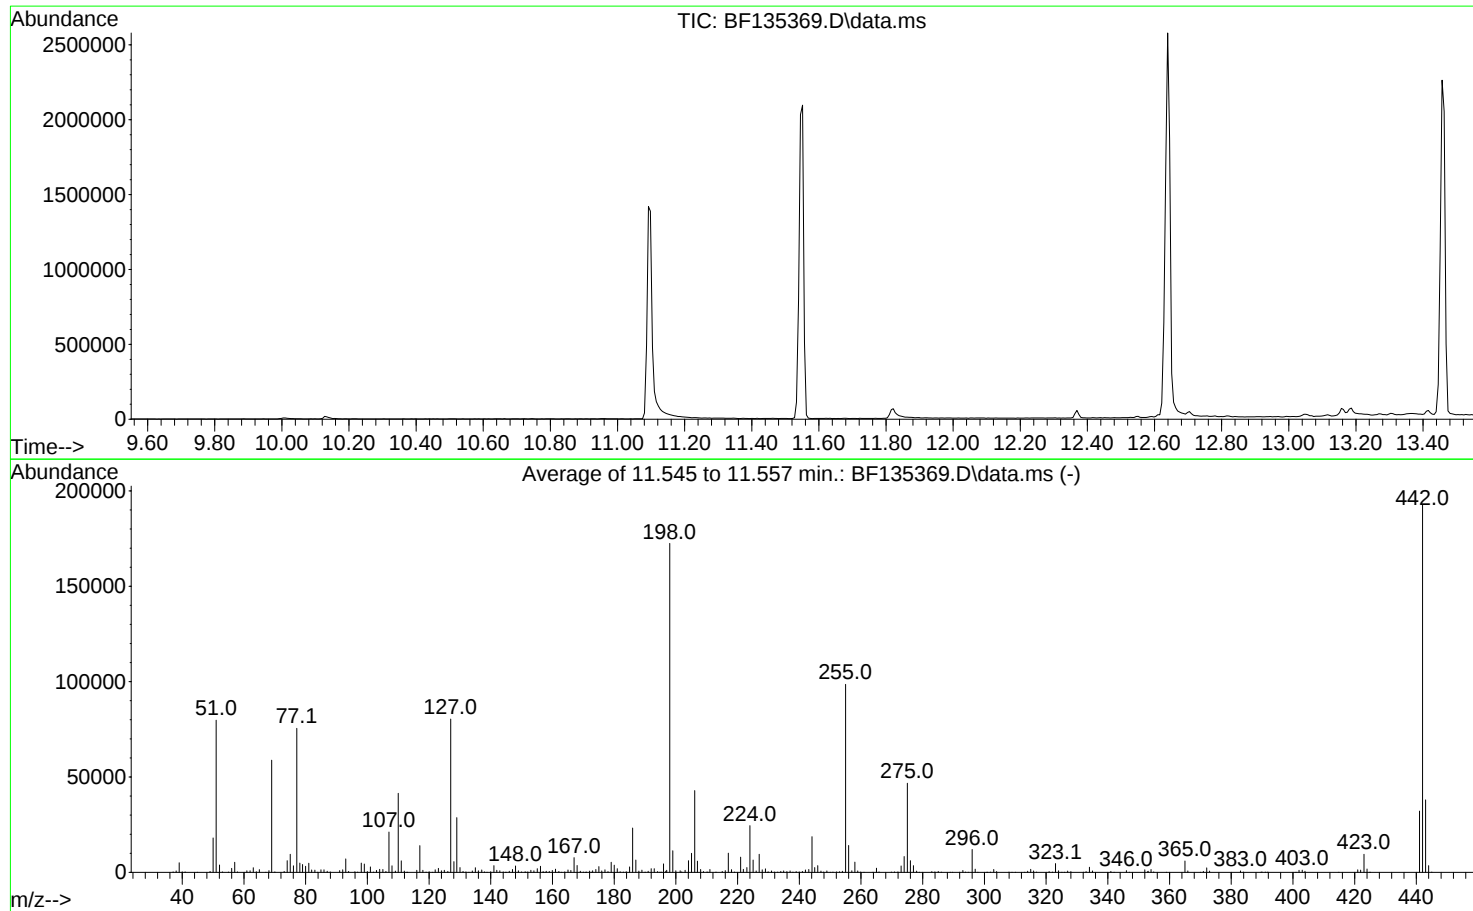




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 46.2         | 79753      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 961        | PASS                |
| 69             | 198             | 0.00            | 100             | 34.1         | 58838      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 227        | PASS                |
| 127            | 198             | 10              | 80              | 46.6         | 80339      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1067       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 172459     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 11323      | PASS                |
| 275            | 198             | 10              | 60              | 27.1         | 46755      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 5983       | PASS                |
| 441            | 198             | 0.01            | 100             | 18.7         | 32168      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 192883     | PASS                |
| 443            | 442             | 15              | 24              | 19.7         | 38048      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092123\  
Data File : BF135369.D  
Acq On : 21 Sep 2023 09:21  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 22 06:52:52 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 00:19:07 2023  
Response via : Initial Calibration

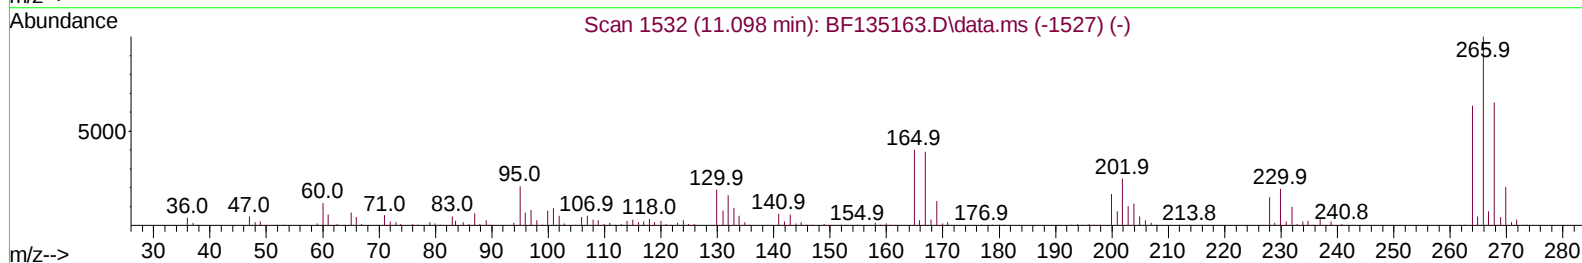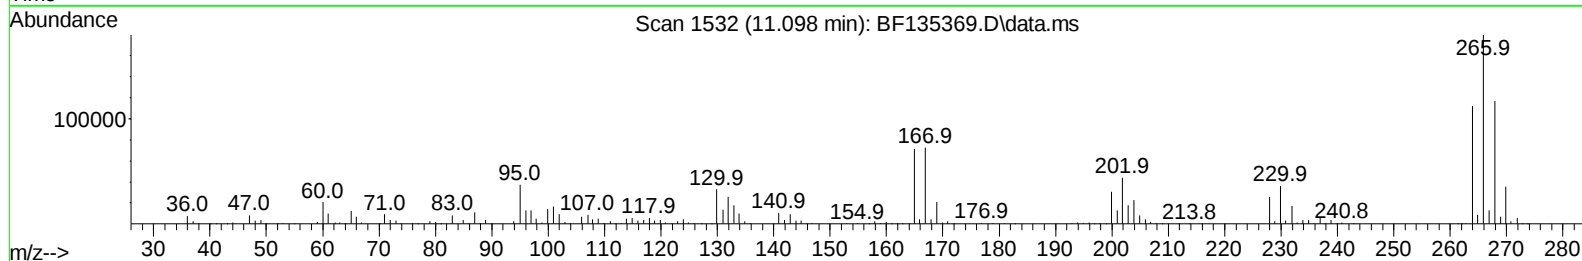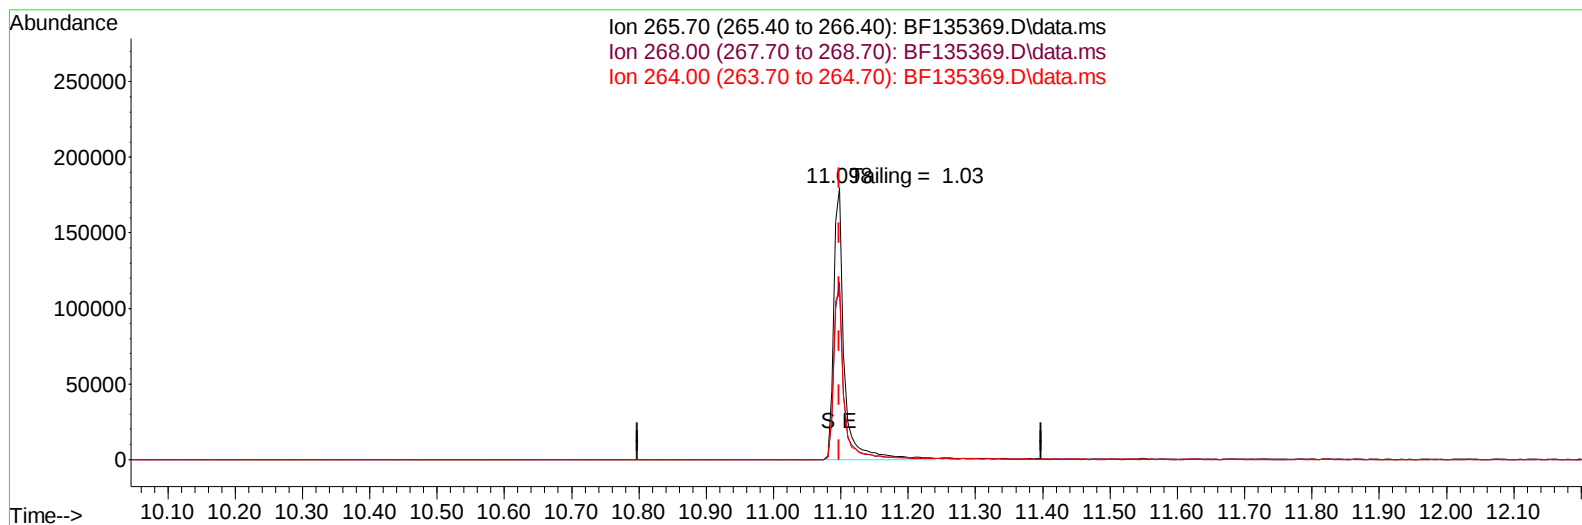

TIC: BF135369.D\data.ms

**(70) Pentachlorophenol (C)**

**11.098min (+ 0.000) 215033.53 ng**




**response 195537**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.10  | 65.16  |
| 264.00 | 63.50  | 62.58  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092123\  
Data File : BF135369.D  
Acq On : 21 Sep 2023 09:21  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 22 06:52:52 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 00:19:07 2023  
Response via : Initial Calibration

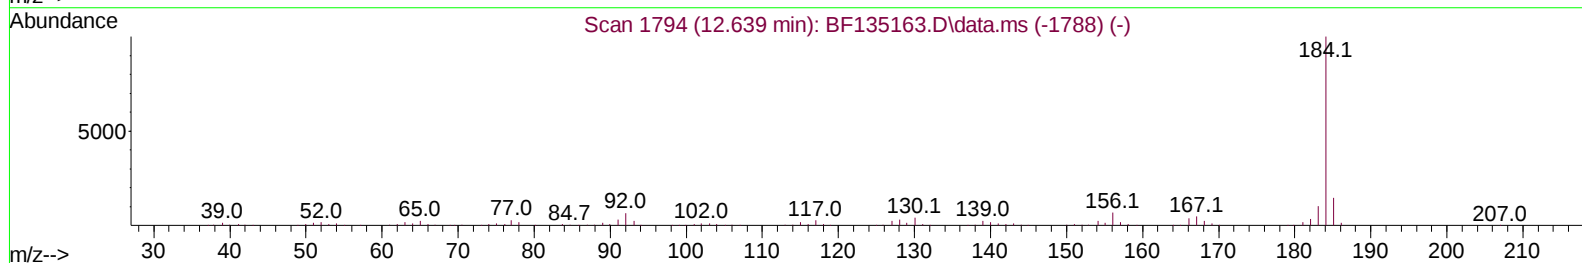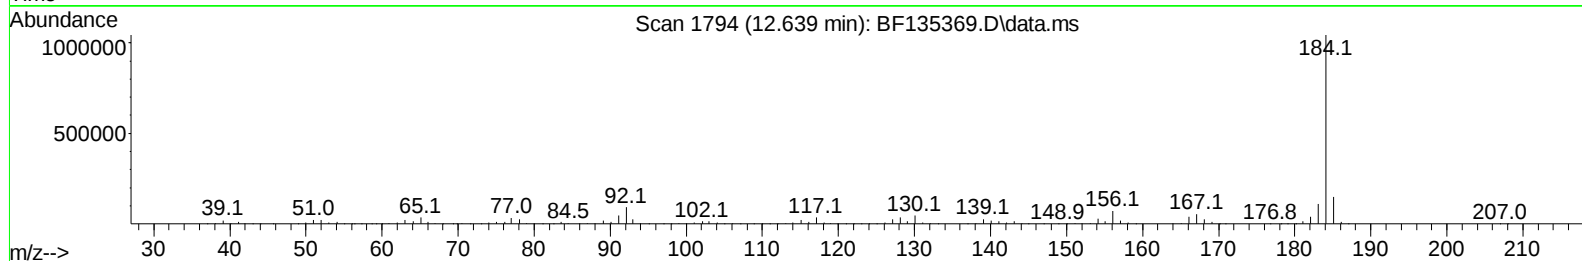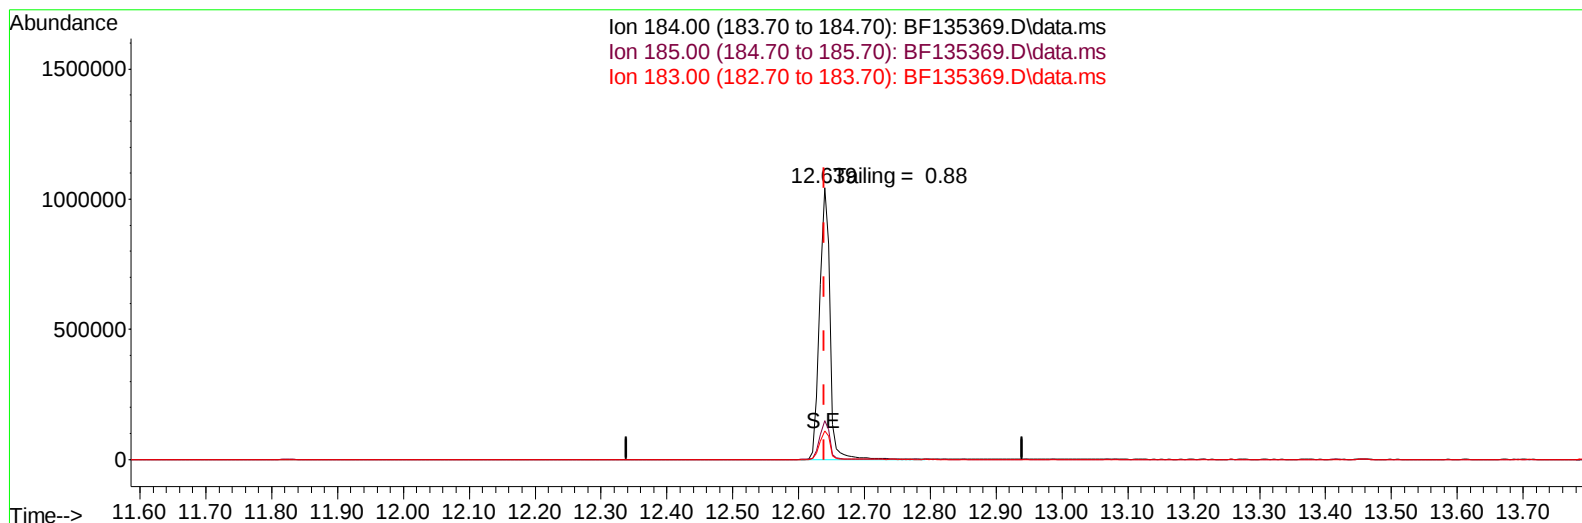

TIC: BF135369.D\data.ms

**(77) Benzidine**

**12.639min (+ 0.000) 117946.85 ng**

**response 1101859**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.39  |
| 183.00 | 10.30  | 10.56  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/21/2023     | BNA_F            | <u>BF135369.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 431884           | 13.457             |
| DDD           | 13956            | 13.157             |
| DDE           | 938              | 12.816             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 14894         | 446778           | 3.33               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP