

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092218\
 Data File : BF109219.D
 Acq On : 22 Sep 2018 14:22
 Operator : JU/SJ
 Sample : PB113087BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB113087BL

Quant Time: Sep 24 07:06:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	106931	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	412023	20.00	ng	0.00
38) Acenaphthene-d10	9.73	164	200268	20.00	ng	0.00
63) Phenanthrene-d10	11.21	188	392486	20.00	ng	0.00
75) Chrysene-d12	13.83	240	328720	20.00	ng	-0.01
86) Perylene-d12	15.23	264	246869	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	672565	103.60	ng	0.00
7) Phenol-d6	6.35	99	860243	103.84	ng	-0.01
23) Nitrobenzene-d5	7.26	82	555765	79.63	ng	-0.02
41) 2,4,6-Tribromophenol	10.52	330	189734	96.11	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	1021386	76.92	ng	-0.01
78) Terphenyl-d14	12.80	244	1069368	79.84	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092218\
Data File : BF109219.D
Acq On : 22 Sep 2018 14:22
Operator : JU/SJ
Sample : PB113087BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB113087BL

Quant Time: Sep 24 07:06:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

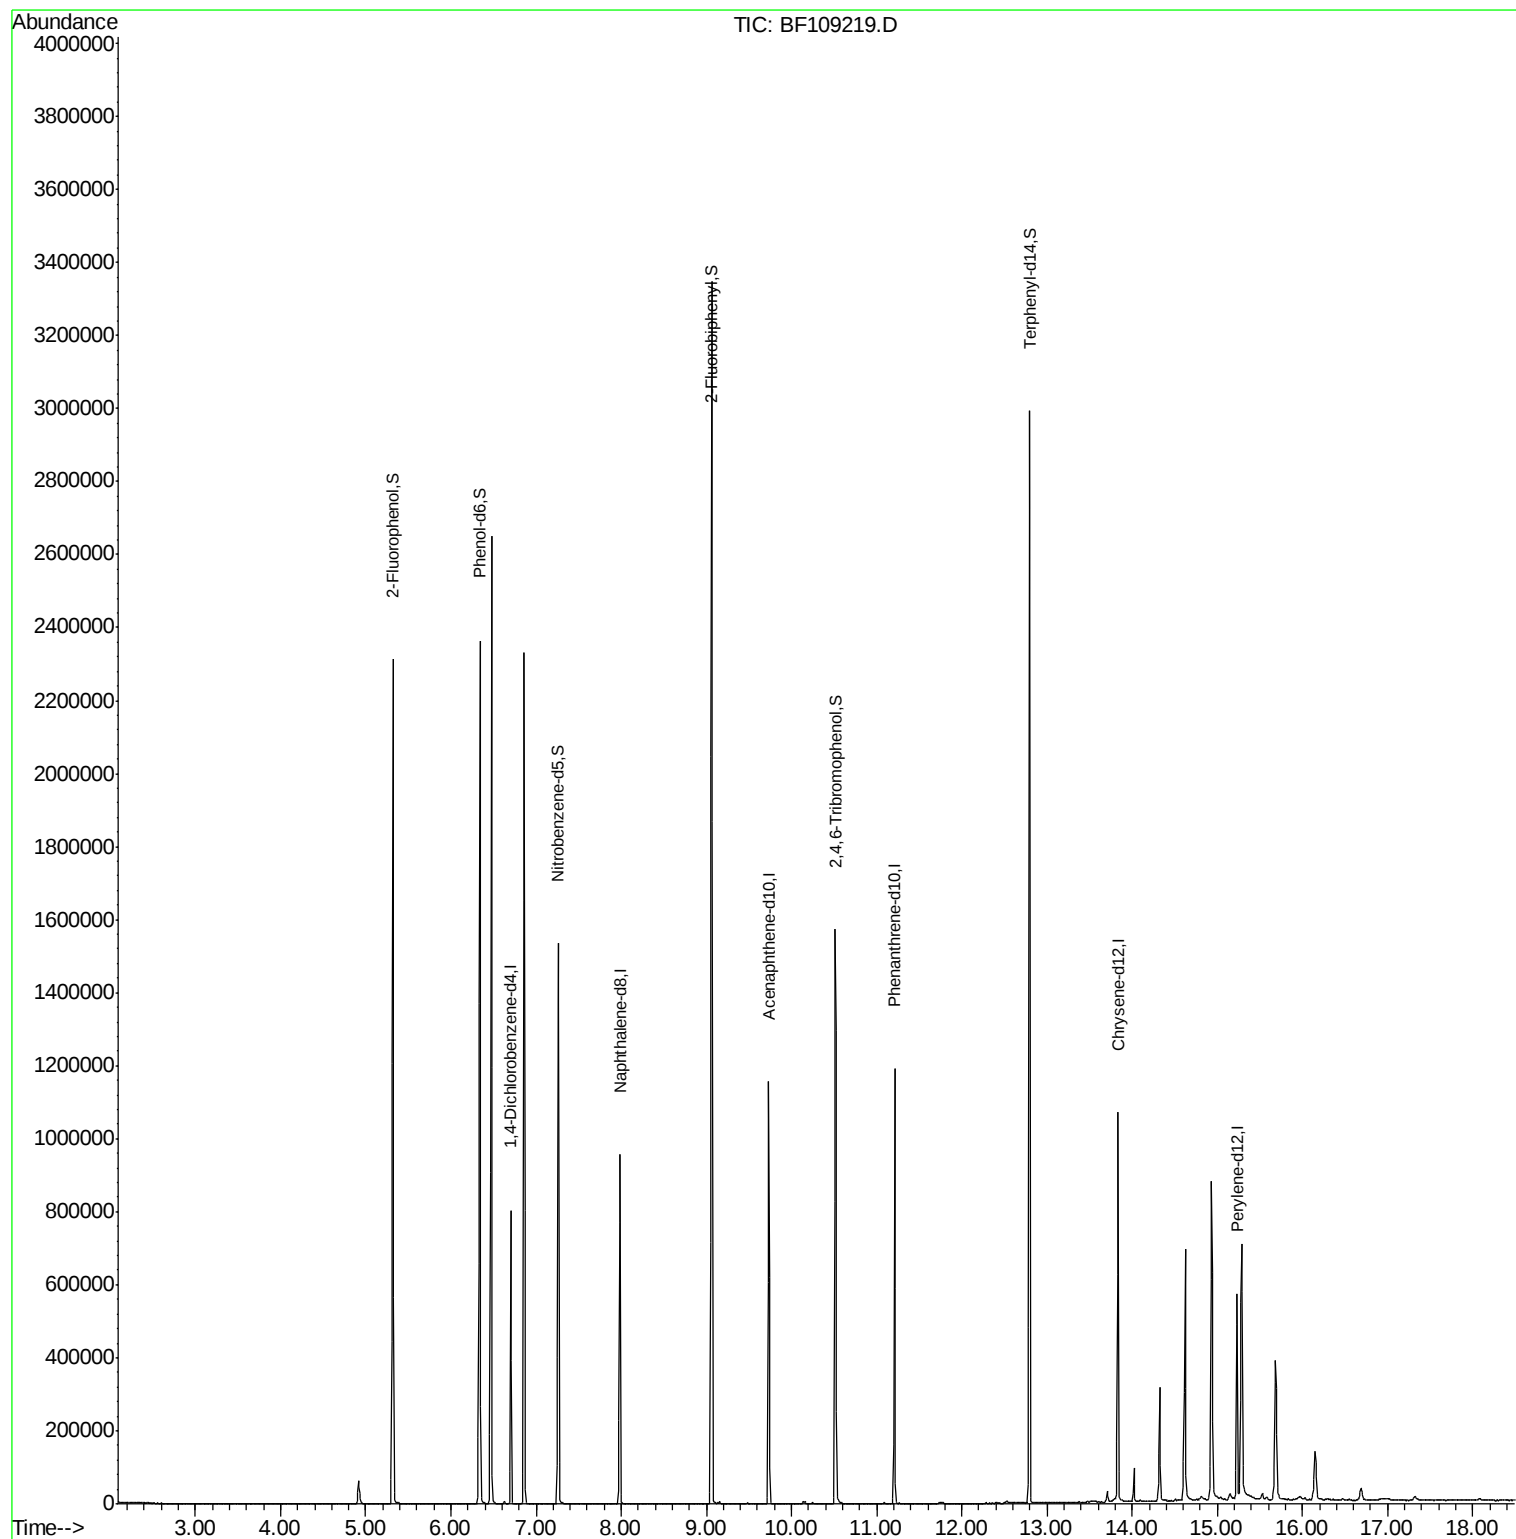

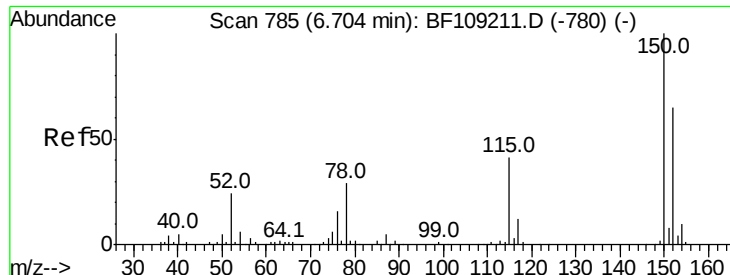


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF109219.D
Acq: 22 Sep 2018 14:22

Instrument :
BNA_F
ClientSampleId :
PB113087BL

Tot Ion:152 Resp: 106931
Ion Ratio Lower Upper
152 100
150 158.6 124.6 186.8
115 62.7 50.1 75.1

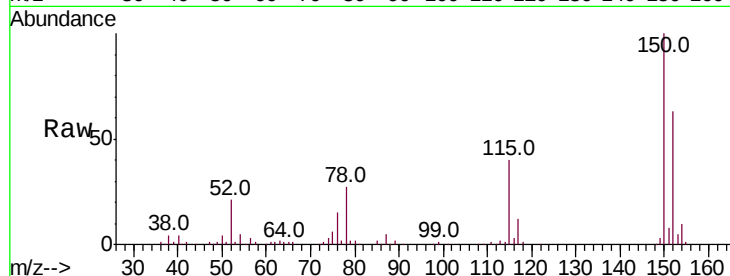


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

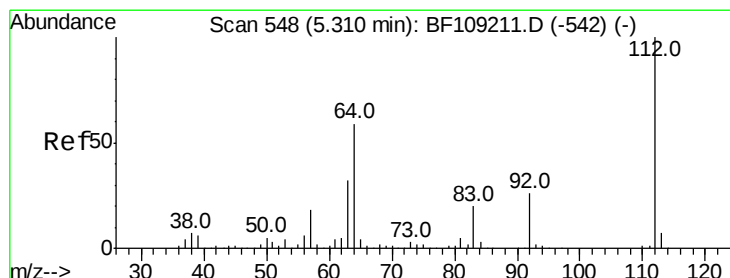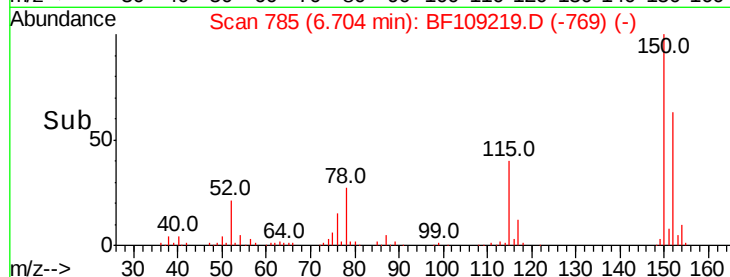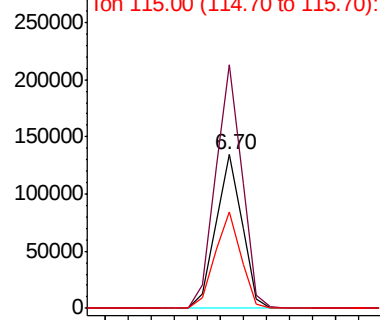



#5


2-Fluorophenol
Concen: 103.596 ng
RT: 5.32 min Scan# 550
Delta R.T. 0.01 min
Lab File: BF109219.D
Acq: 22 Sep 2018 14:22

Tgt Ion:112 Resp: 672565
Ion Ratio Lower Upper
112 100
64 58.0 47.9 71.9
63 31.3 23.7 35.5

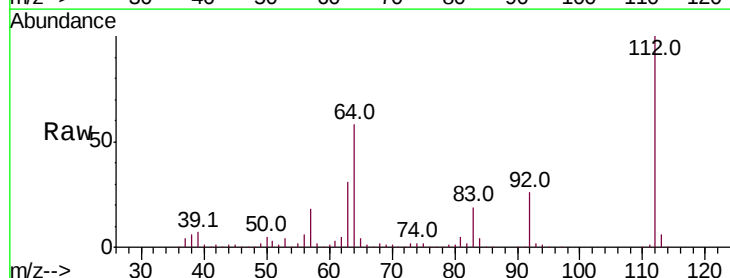

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

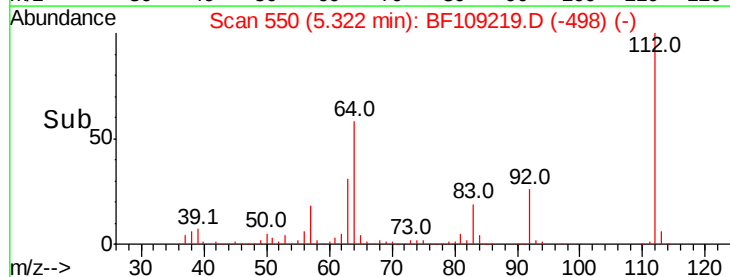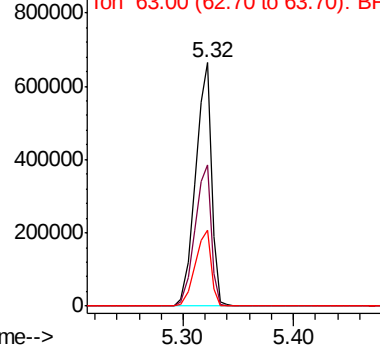

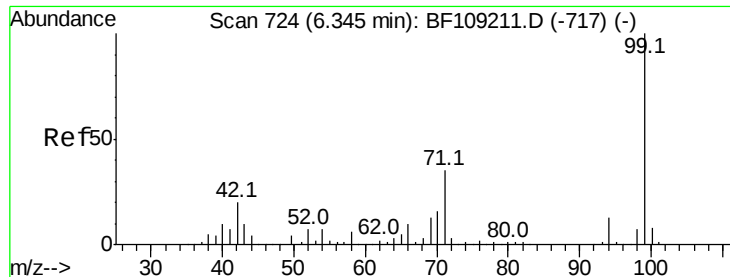

#7

Phenol-d6

Concen: 103.841 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.01 min

Lab File: BF109219.D

Acq: 22 Sep 2018 14:22

Instrument :

BNA_F

ClientSampleId :

PB113087BL


Tot Ion: 99 Resp: 860243

Ion Ratio Lower Upper




99 100

42 19.6 14.5 21.7

71 35.9 25.4 38.0

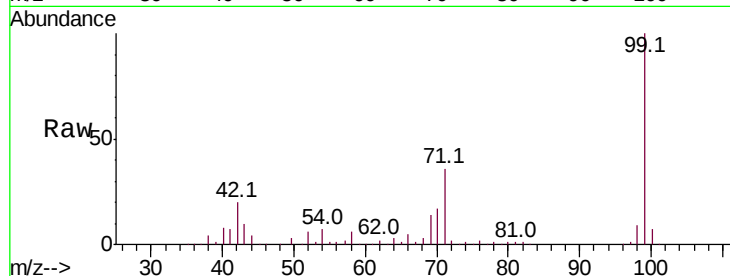

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

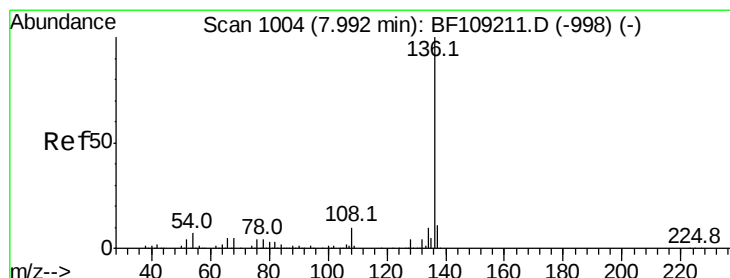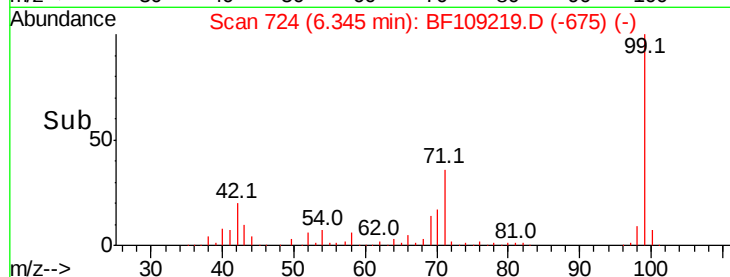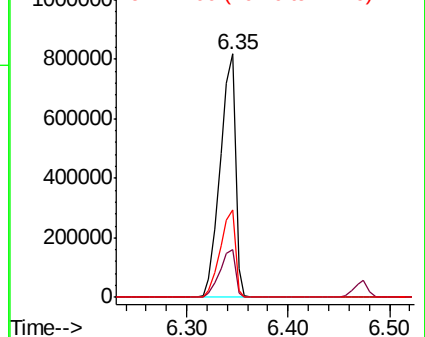

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.99 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF109219.D

Acq: 22 Sep 2018 14:22

Tgt Ion: 136 Resp: 412023


Ion Ratio Lower Upper

136 100



137 10.9 8.9 13.3


54 6.8 6.6 9.8

68 5.4 5.0 7.4

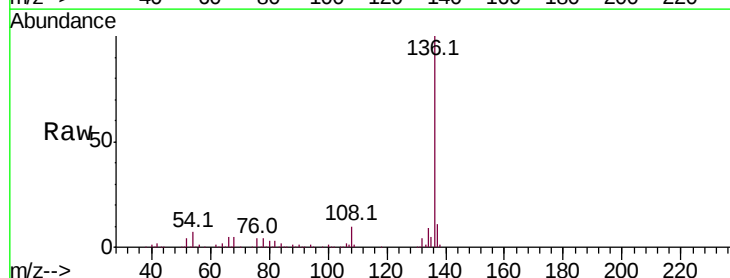

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

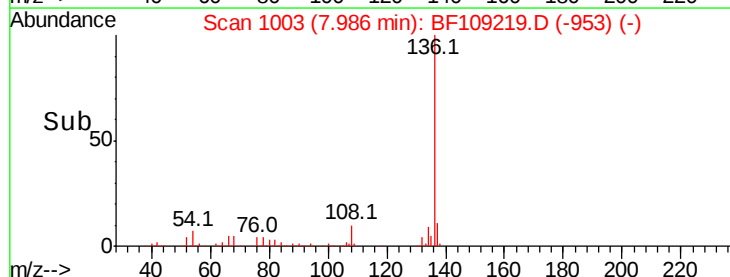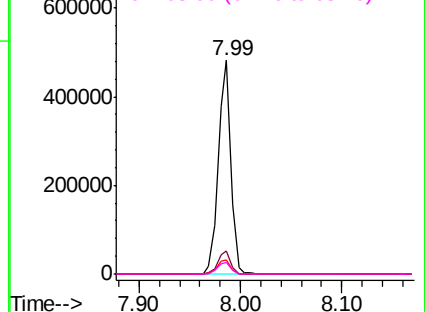


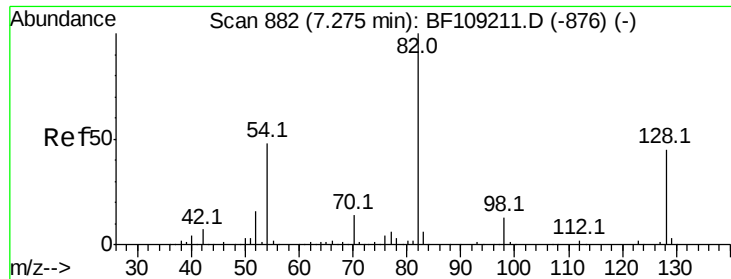




#23
 Nitrobenzene-d5
 Concen: 79.626 ng
 RT: 7.26 min Scan# 880
 Delta R.T. -0.02 min
 Lab File: BF109219.D
 Acq: 22 Sep 2018 14:22

Instrument :
 BNA_F
 ClientSampleId :
 PB113087BL

Tot Ion	82	Resp	555765
Ion Ratio	Lower	Upper	
82	100		
128	41.7	36.1	54.1
54	49.3	41.4	62.2

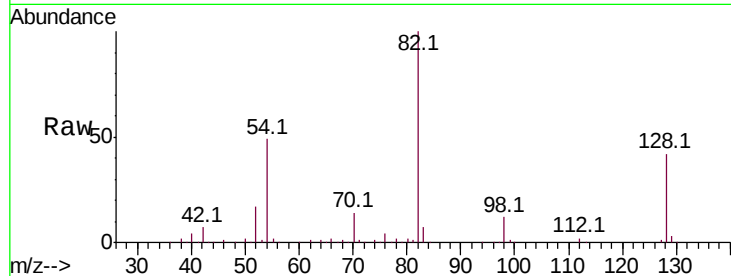


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

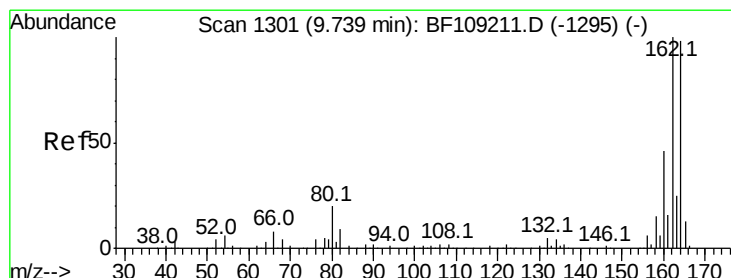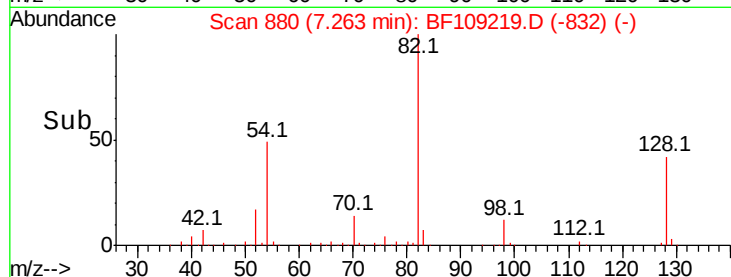
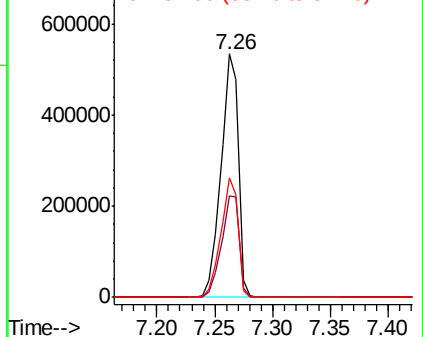



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF109219.D
 Acq: 22 Sep 2018 14:22

Tgt Ion	164	Resp	200268
Ion Ratio	Lower	Upper	
164	100		
162	102.0	86.1	129.1
160	46.9	38.3	57.5

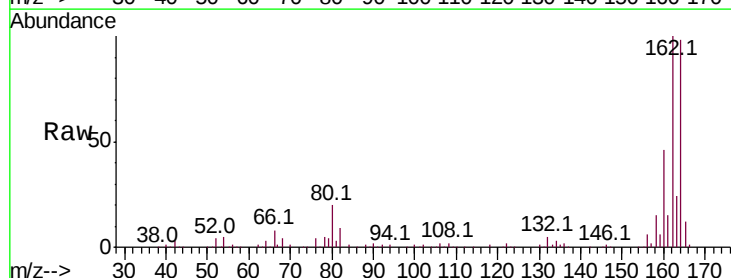

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

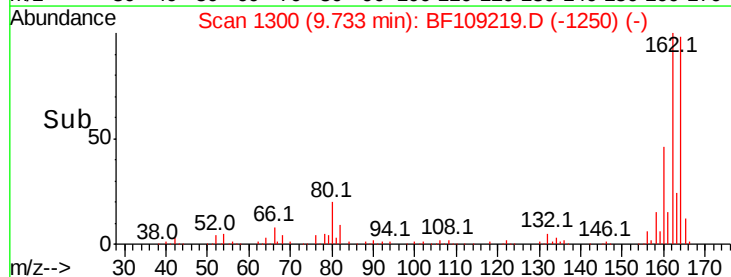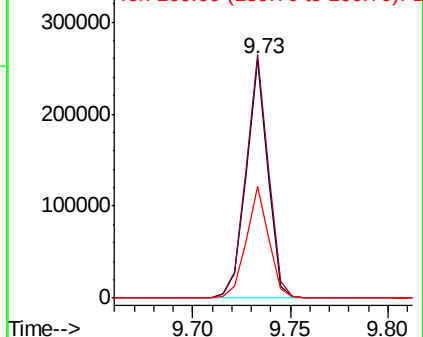


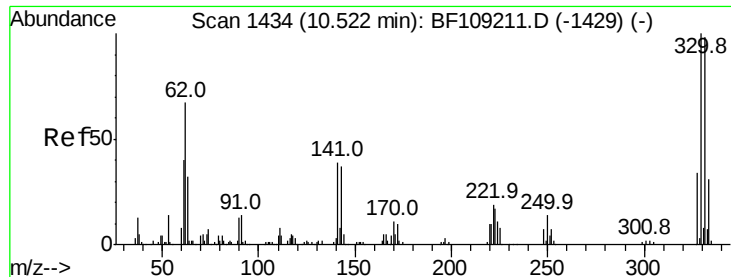




#41
 2,4,6-Tribromophenol
 Concen: 96.106 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF109219.D
 Acq: 22 Sep 2018 14:22

Instrument :
 BNA_F
 ClientSampleId :
 PB113087BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.2	77.0	115.6
141	35.3	29.9	44.9

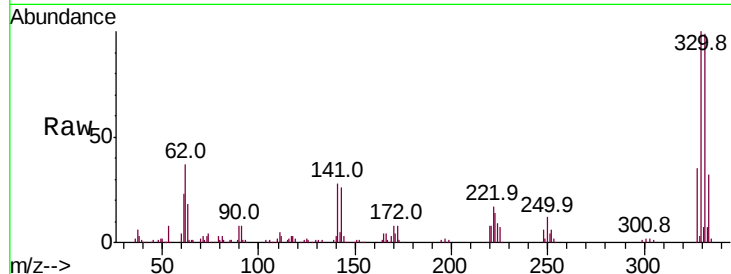


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

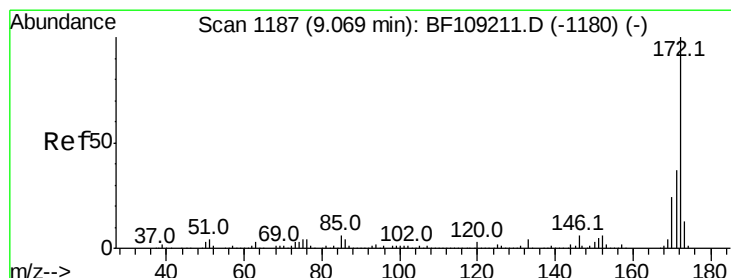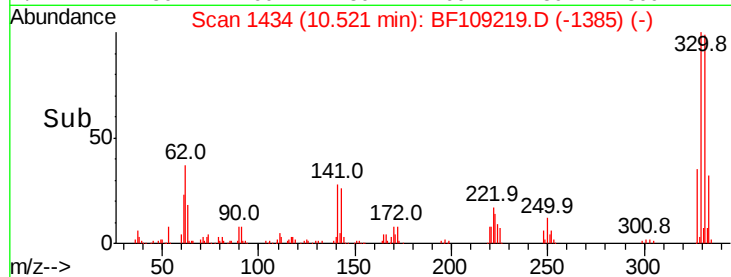
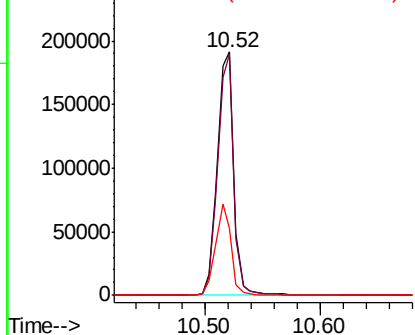



#44
 2-Fluorobiphenyl
 Concen: 76.919 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF109219.D
 Acq: 22 Sep 2018 14:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	29.7	44.5
170	24.1	19.6	29.4

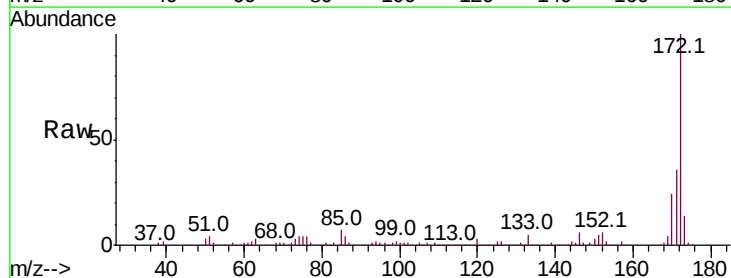

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



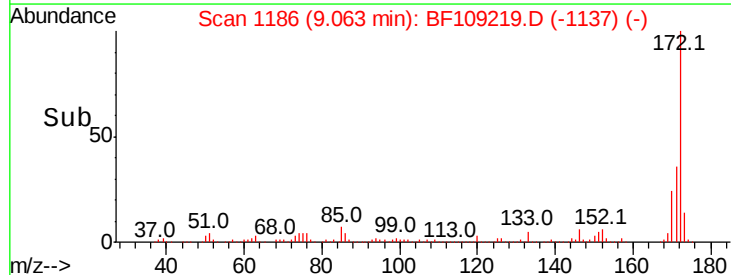
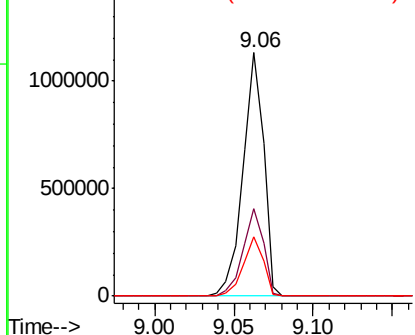


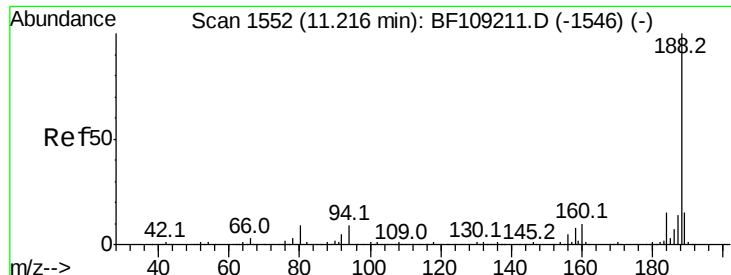

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF109219.D
Acq: 22 Sep 2018 14:22




Instrument :
BNA_F
ClientSampleId :
PB113087BL


Tot Ion	Ratio	Lower	Upper
188	100		
94	9.8	8.5	12.7
80	10.1	9.2	13.8

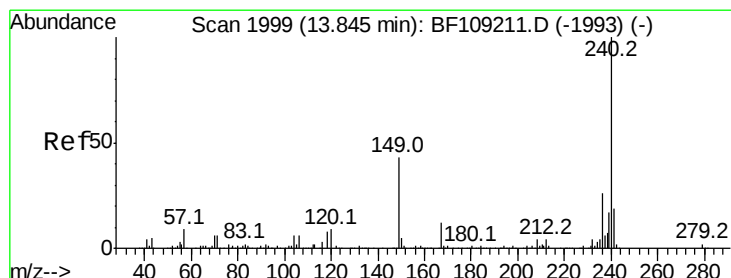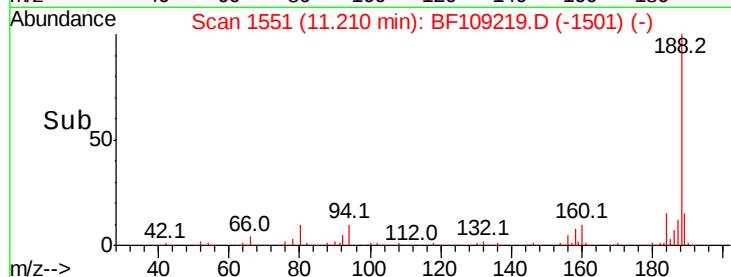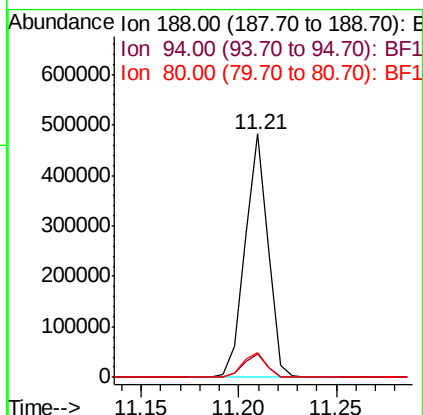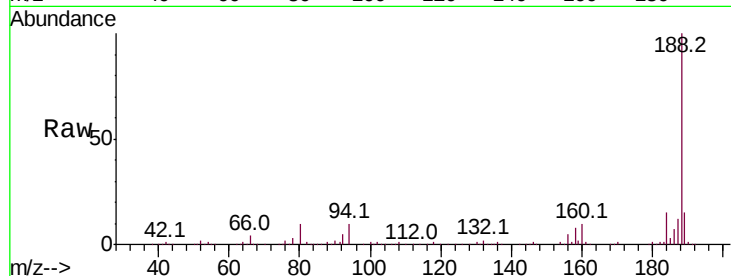

#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.83 min Scan# 1997
Delta R.T. -0.01 min
Lab File: BF109219.D
Acq: 22 Sep 2018 14:22

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.5	9.5	14.3
236	26.1	20.7	31.1

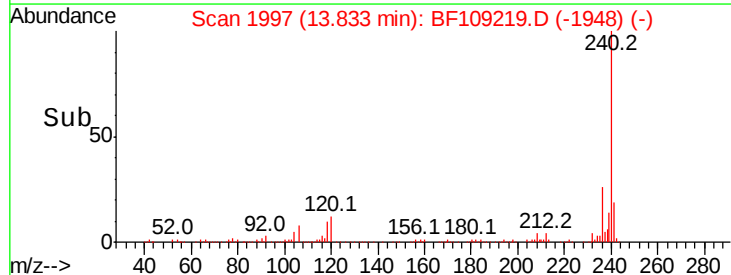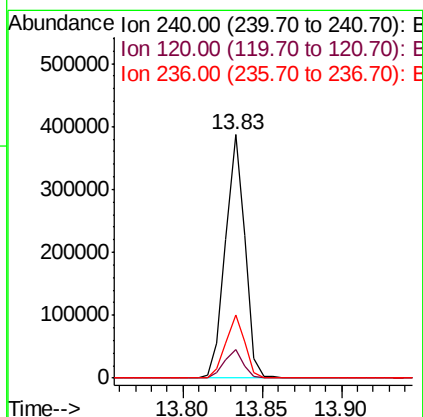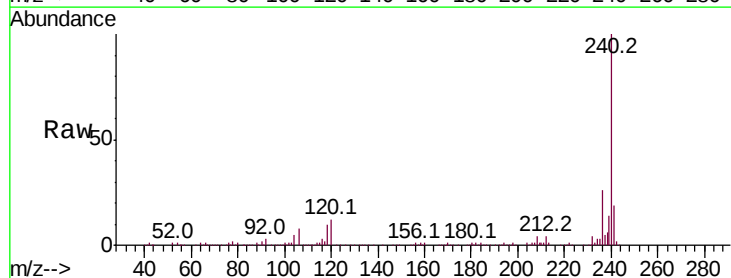

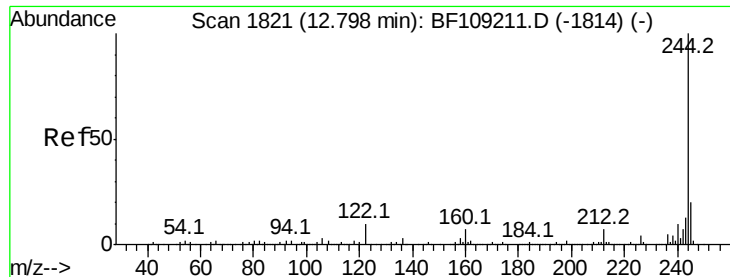

#78

Terphenyl-d14

Concen: 79.837 ng

RT: 12.80 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BF109219.D

Acq: 22 Sep 2018 14:22

Instrument :

BNA_F

ClientSampleId :

PB113087BL


Tot Ion:244 Resp: 1069368

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0




122 10.8 11.0 16.4#

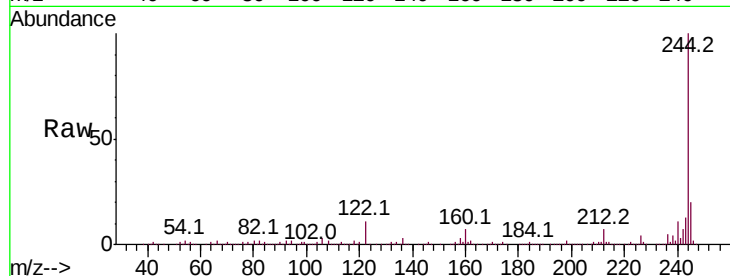

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

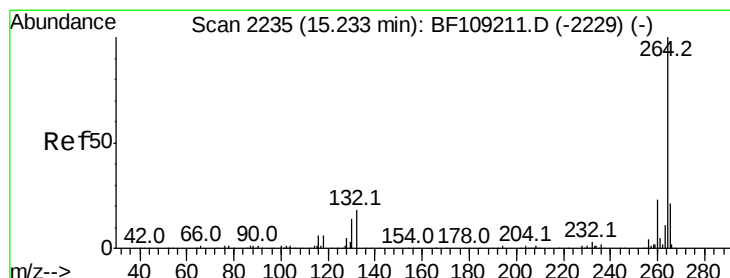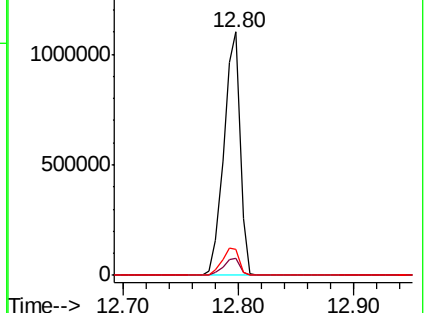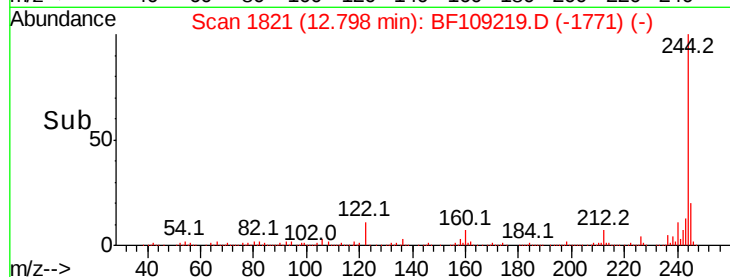

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.23 min Scan# 2235

Delta R.T. -0.01 min

Lab File: BF109219.D

Acq: 22 Sep 2018 14:22


Tgt Ion:264 Resp: 246869

Ion Ratio Lower Upper

264 100

260 22.8 19.2 28.8

265 21.0 17.5 26.3

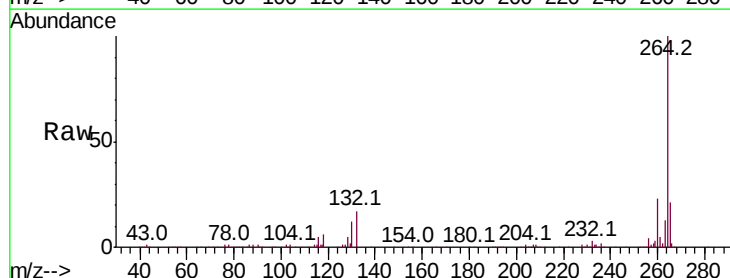

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

