


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092218\
 Data File : BF109206.D
 Acq On : 22 Sep 2018 7:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 22 13:32:18 2018

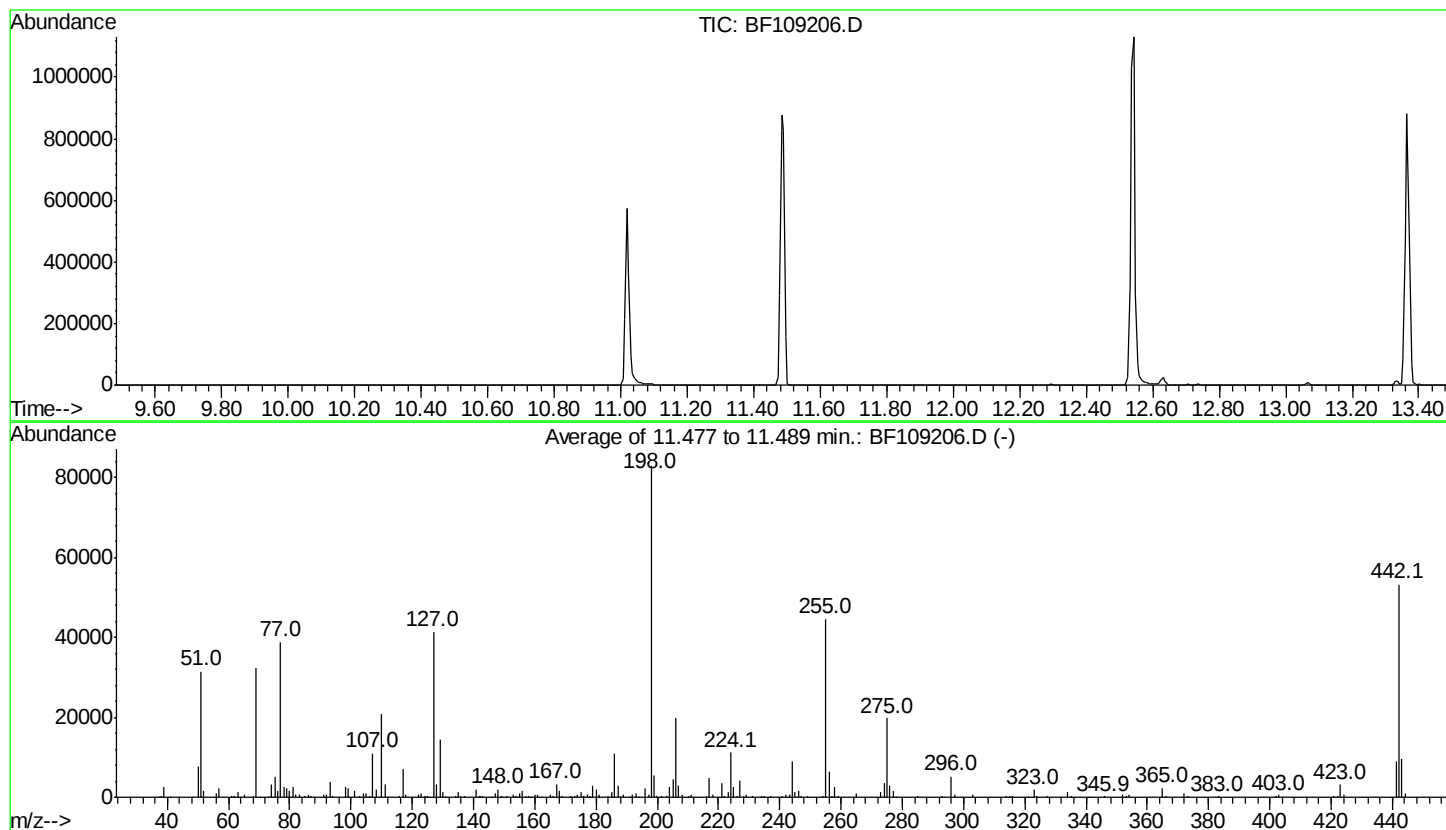

AutoFind: Scans 1554, 1555, 1556; Background Corrected with Scan 1550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	31469	PASS
68	69	0.00	2	1.3	412	PASS
69	198	0.00	100	39.0	32320	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	49.8	41312	PASS
197	198	0.00	2	0.6	524	PASS
198	198	100	100	100.0	82928	PASS
199	198	5	9	6.6	5499	PASS
275	198	10	60	23.8	19748	PASS
365	198	1	100	2.9	2380	PASS
441	198	0.01	100	11.0	9082	PASS
442	198	50	100	64.1	53170	PASS
443	442	15	24	18.2	9655	PASS