


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092220\
 Data File : BF121643.D
 Acq On : 22 Sep 2020 16:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 22 17:53:26 2020

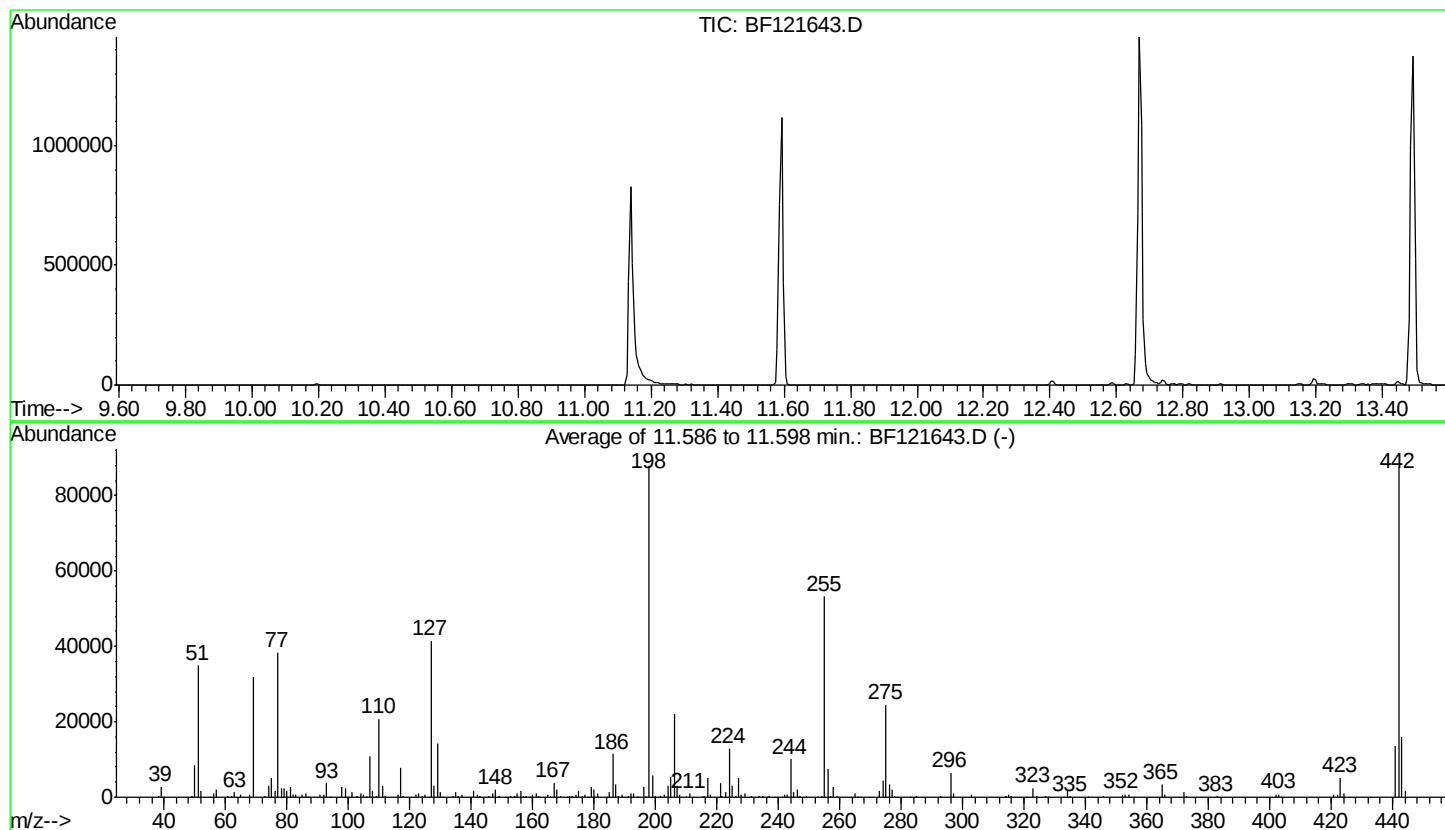

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	34876	PASS
68	69	0.00	2	1.7	532	PASS
69	198	0.00	100	36.1	31759	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.1	41418	PASS
197	198	0.00	2	0.2	170	PASS
198	198	100	100	100.0	87941	PASS
199	198	5	9	6.6	5827	PASS
275	198	10	60	28.0	24618	PASS
365	198	1	100	3.8	3314	PASS
441	198	0.01	100	15.3	13489	PASS
442	198	50	100	99.8	87741	PASS
443	442	15	24	18.2	15945	PASS