
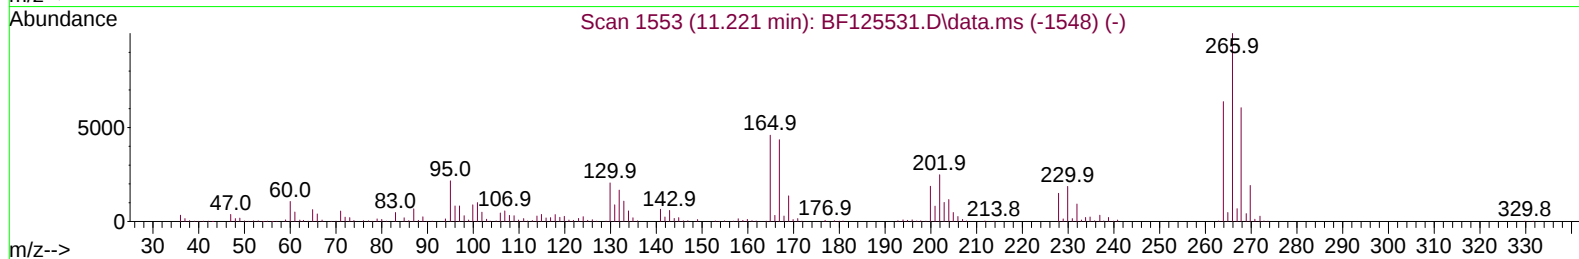
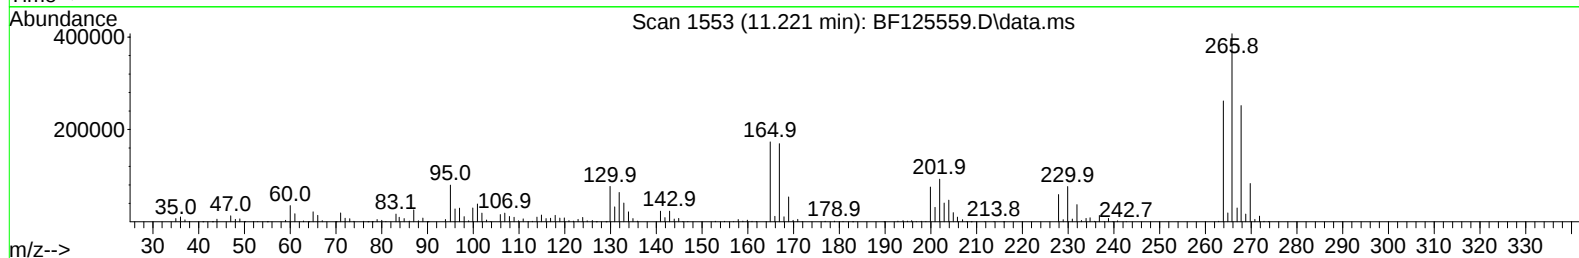


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
Data File : BF125559.D
Acq On : 22 Sep 2021 15:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 15:37:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

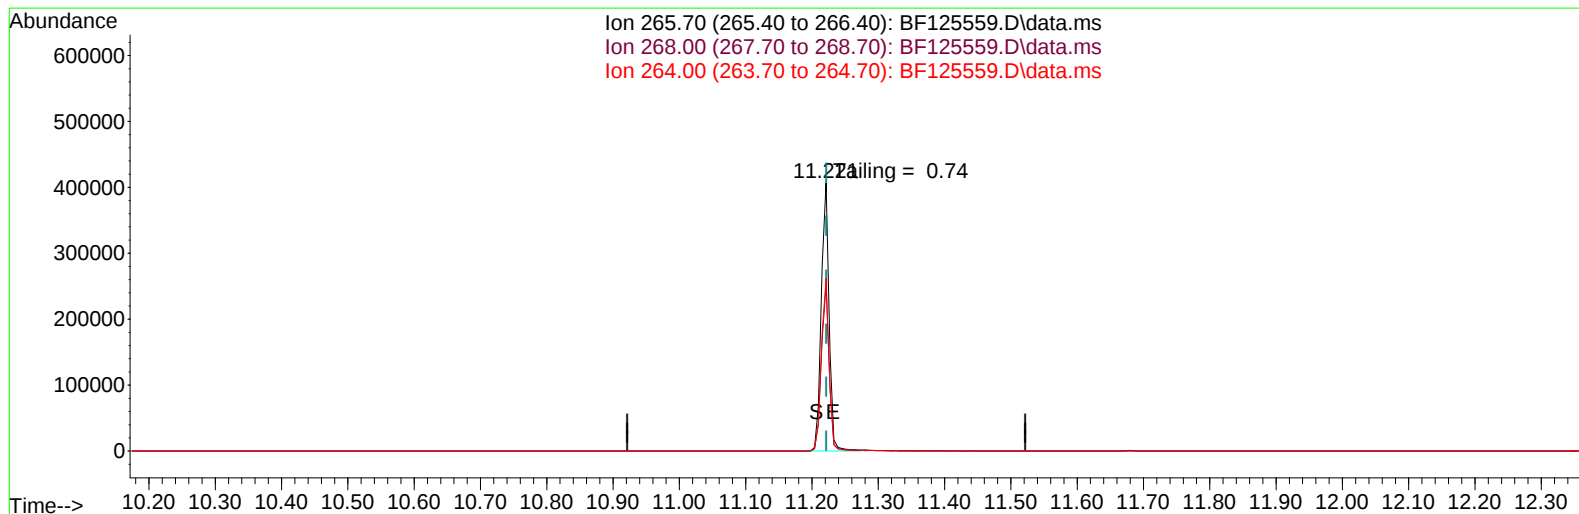

TIC: BF125559.D\data.ms

(70) Pentachlorophenol (C)




11.221min (-0.000) 35072.45 ng

response 337880

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.80
264.00	69.90	64.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
Data File : BF125559.D
Acq On : 22 Sep 2021 15:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 15:37:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

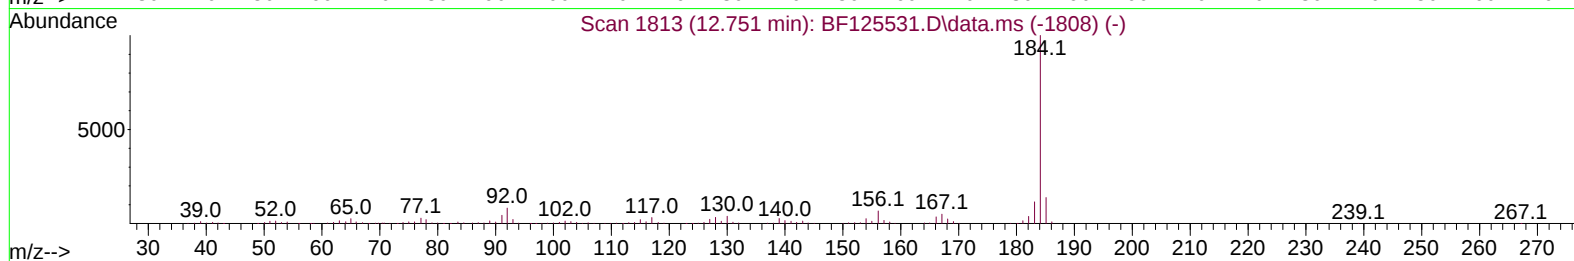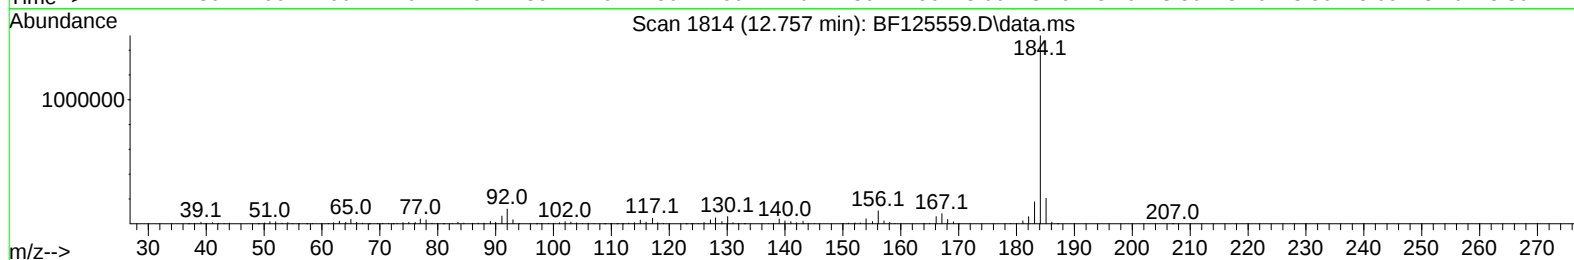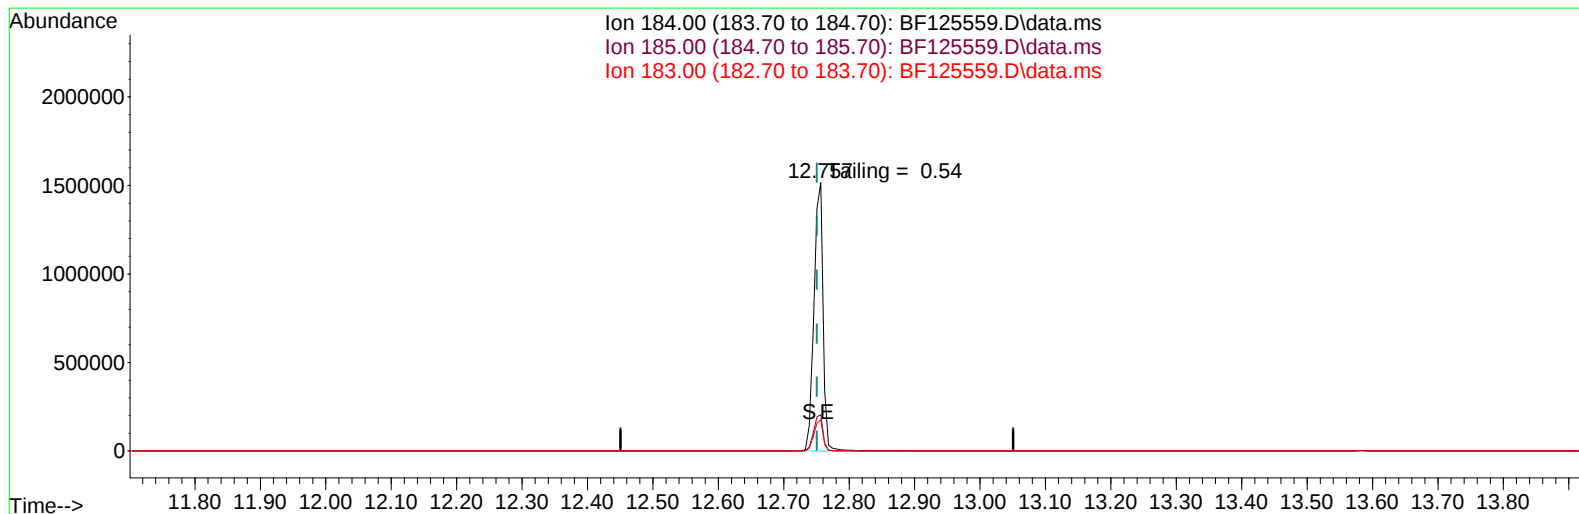

TIC: BF125559.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1469856

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.57
183.00	10.10	11.66
0.00	0.00	0.00