
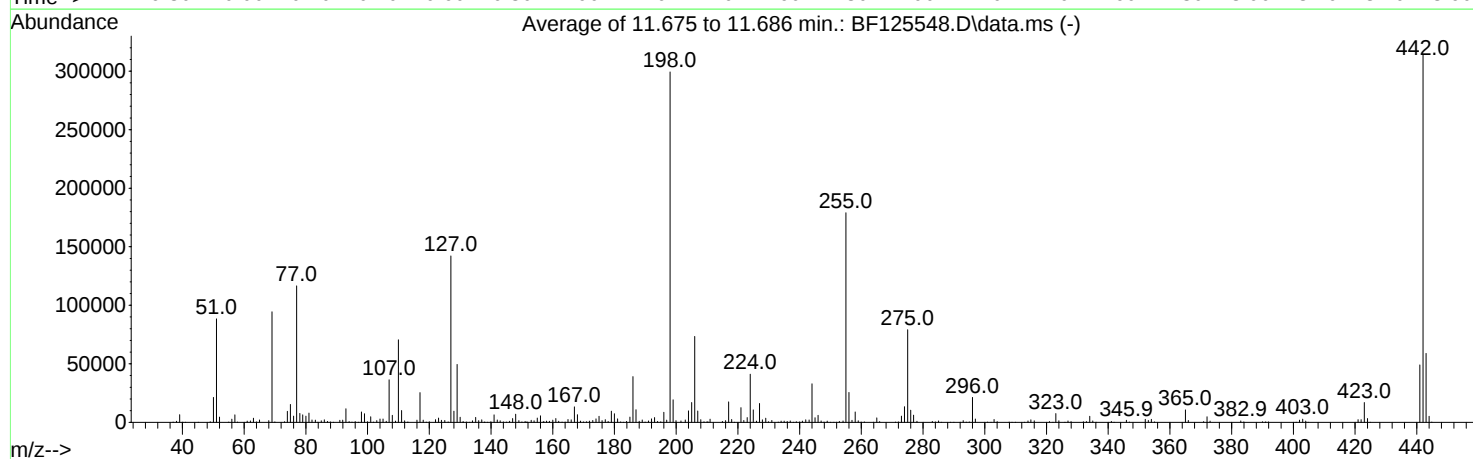


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
 Data File : BF125548.D
 Acq On : 22 Sep 2021 9:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 19:21:36 2021

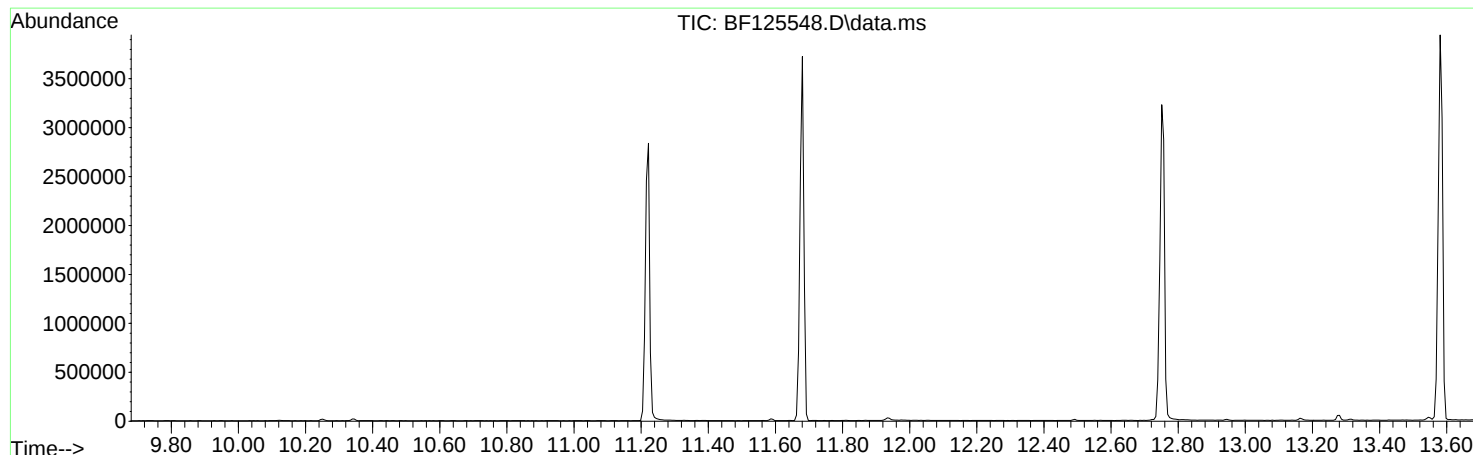

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	88403	PASS
68	69	0.00	2	1.6	1490	PASS
69	198	0.00	100	31.6	94451	PASS
70	69	0.00	2	0.5	469	PASS
127	198	10	80	47.5	142168	PASS
197	198	0.00	2	0.6	1914	PASS
198	198	100	100	100.0	299307	PASS
199	198	5	9	6.4	19263	PASS
275	198	10	60	26.4	79165	PASS
365	198	1	100	3.6	10626	PASS
441	198	0.01	100	16.4	49013	PASS
442	442	50	100	100.0	314197	PASS
443	442	15	24	18.7	58848	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2021	BNA_F	<u>BF125548.D</u>
Compound Name	Response	Retention Time
DDT	709653	13.58
DDD	9503	13.28
DDE	1643	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11146	720799	1.55

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
 Data File : BF125548.D
 Acq On : 22 Sep 2021 9:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 22 11:00:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 21 19:21:36 2021
 Response via : Initial Calibration

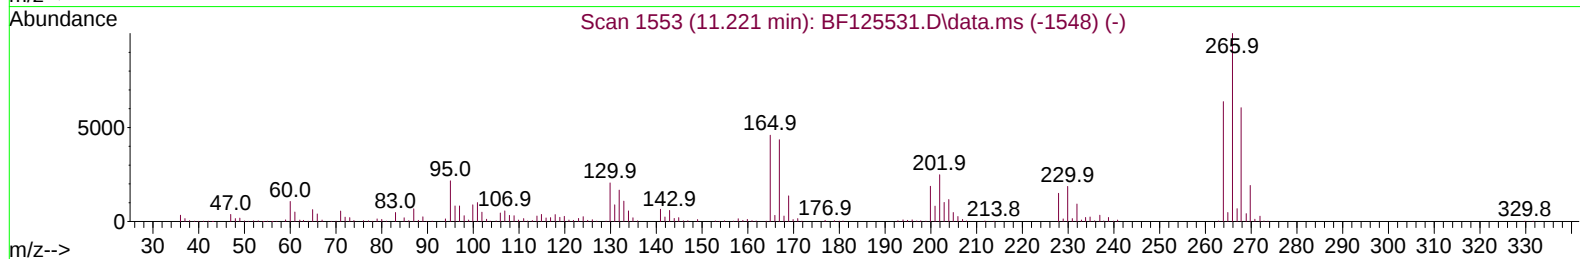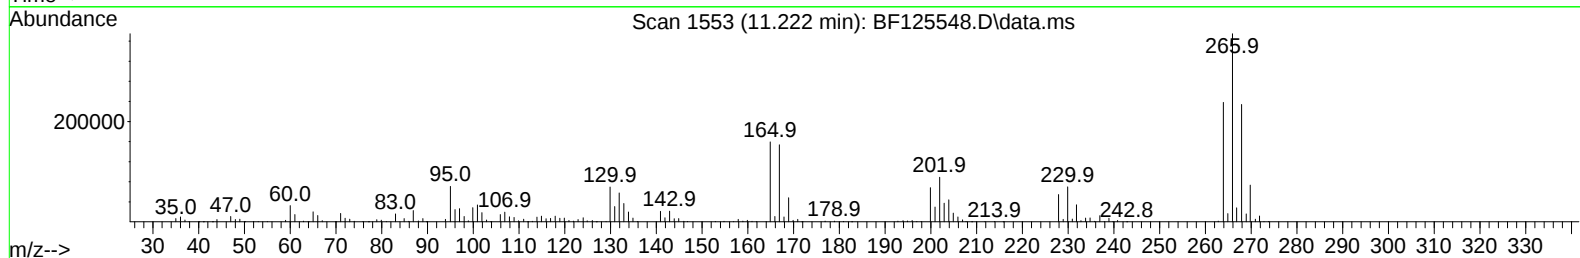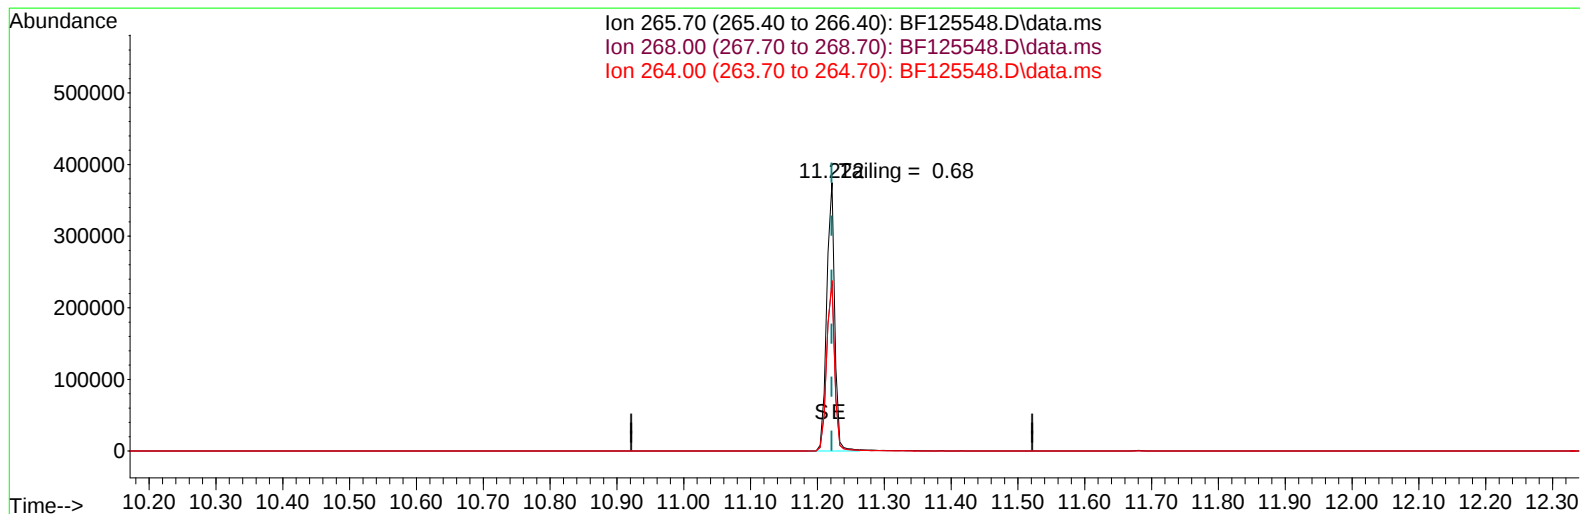

TIC: BF125548.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 41827.32 ng

response 316037

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.41
264.00	69.90	63.51
0.00	0.00	0.00

