
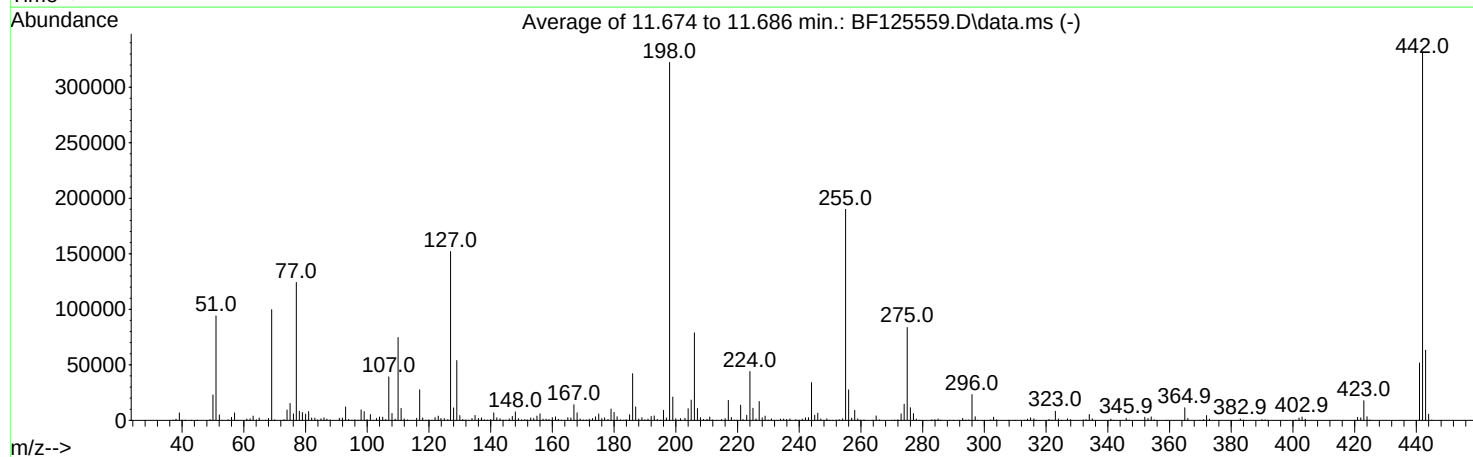


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
 Data File : BF125559.D
 Acq On : 22 Sep 2021 15:01
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 21 19:21:36 2021

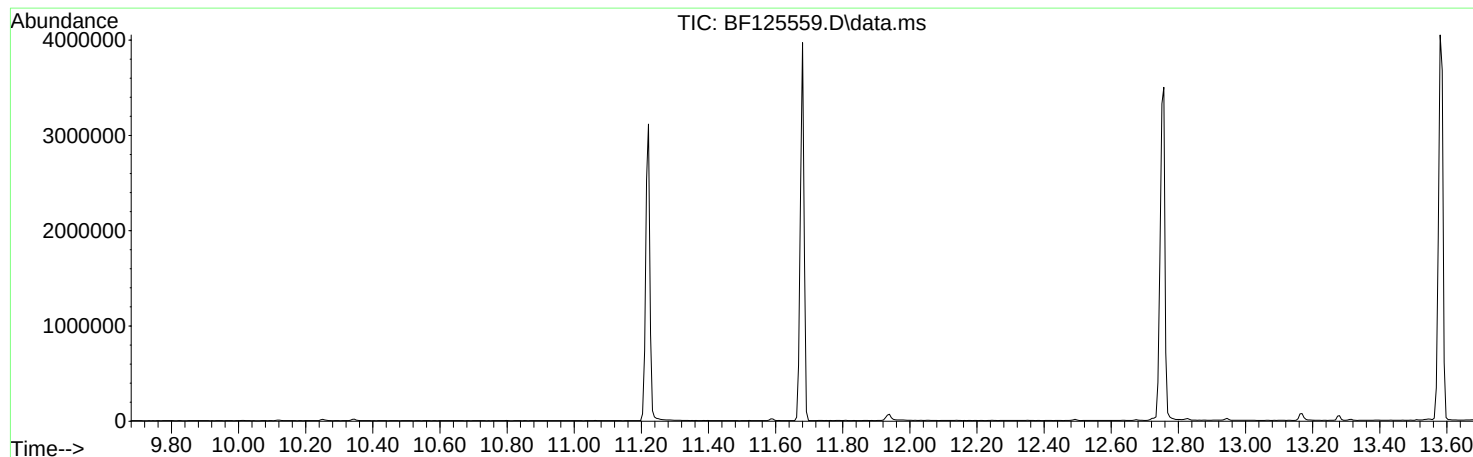

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	94072	PASS
68	69	0.00	2	1.7	1744	PASS
69	198	0.00	100	30.9	99659	PASS
70	69	0.00	2	0.4	421	PASS
127	198	10	80	47.2	152021	PASS
197	198	0.00	2	0.7	2173	PASS
198	198	100	100	100.0	322261	PASS
199	198	5	9	6.5	21055	PASS
275	198	10	60	26.0	83736	PASS
365	198	1	100	3.5	11357	PASS
441	198	0.01	100	16.1	51781	PASS
442	442	50	100	100.0	331243	PASS
443	442	15	24	19.1	63317	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2021	BNA_F	<u>BF125559.D</u>
Compound Name	Response	Retention Time
DDT	773248	13.58
DDD	9656	13.28
DDE	2782	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12438	785686	1.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
Data File : BF125559.D
Acq On : 22 Sep 2021 15:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 22 15:37:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

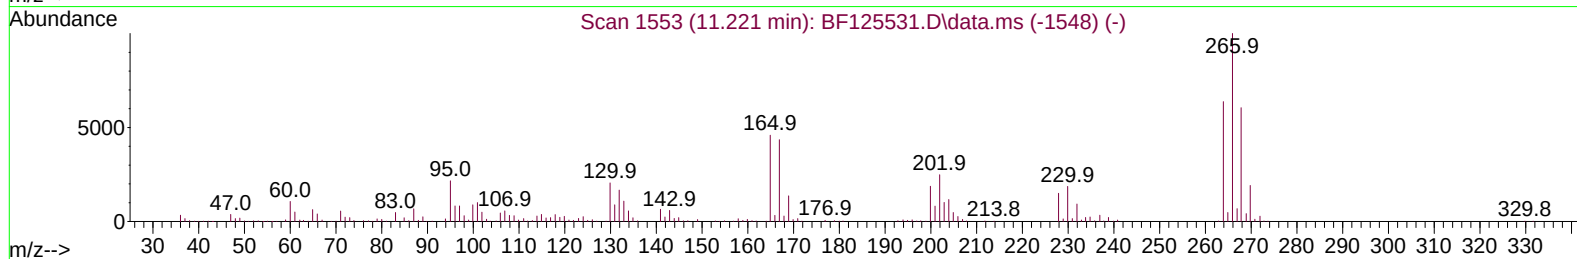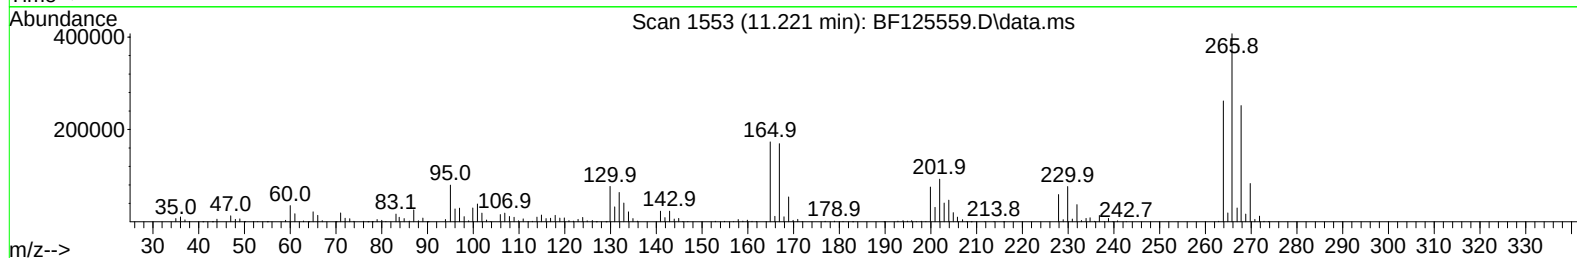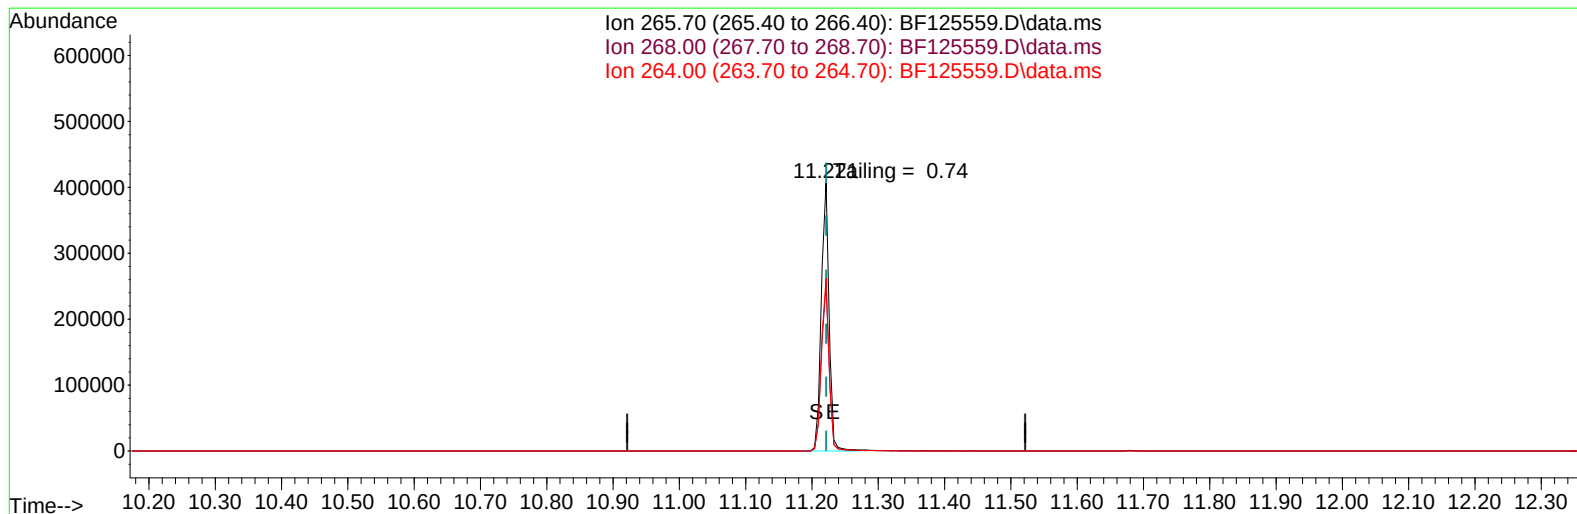

TIC: BF125559.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.000) 35072.45 ng




response 337880

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.80
264.00	69.90	64.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092221\
Data File : BF125559.D
Acq On : 22 Sep 2021 15:01
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 22 15:37:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 21 19:21:36 2021
Response via : Initial Calibration

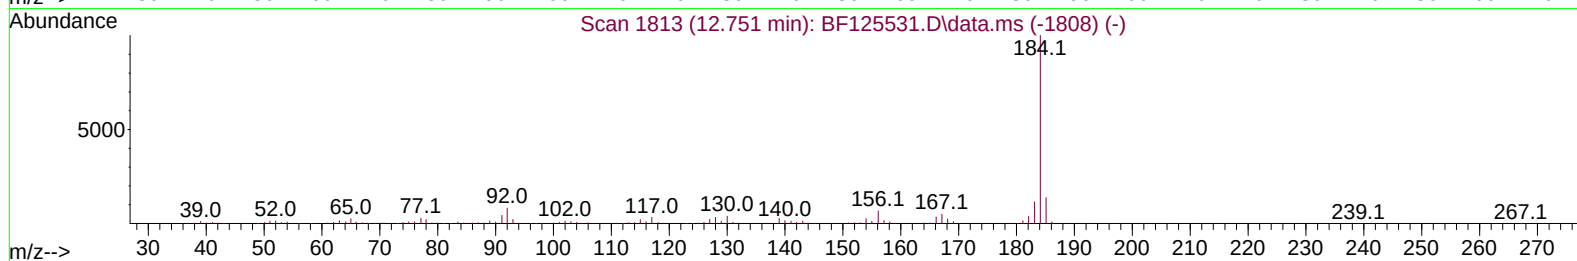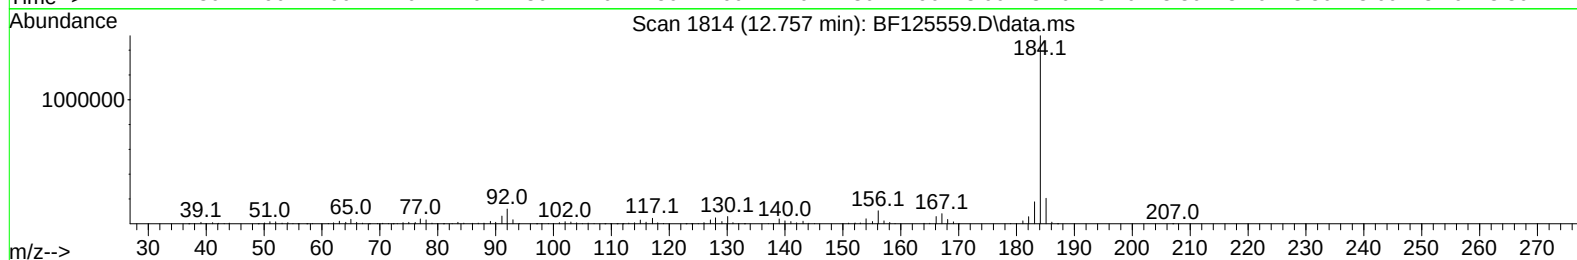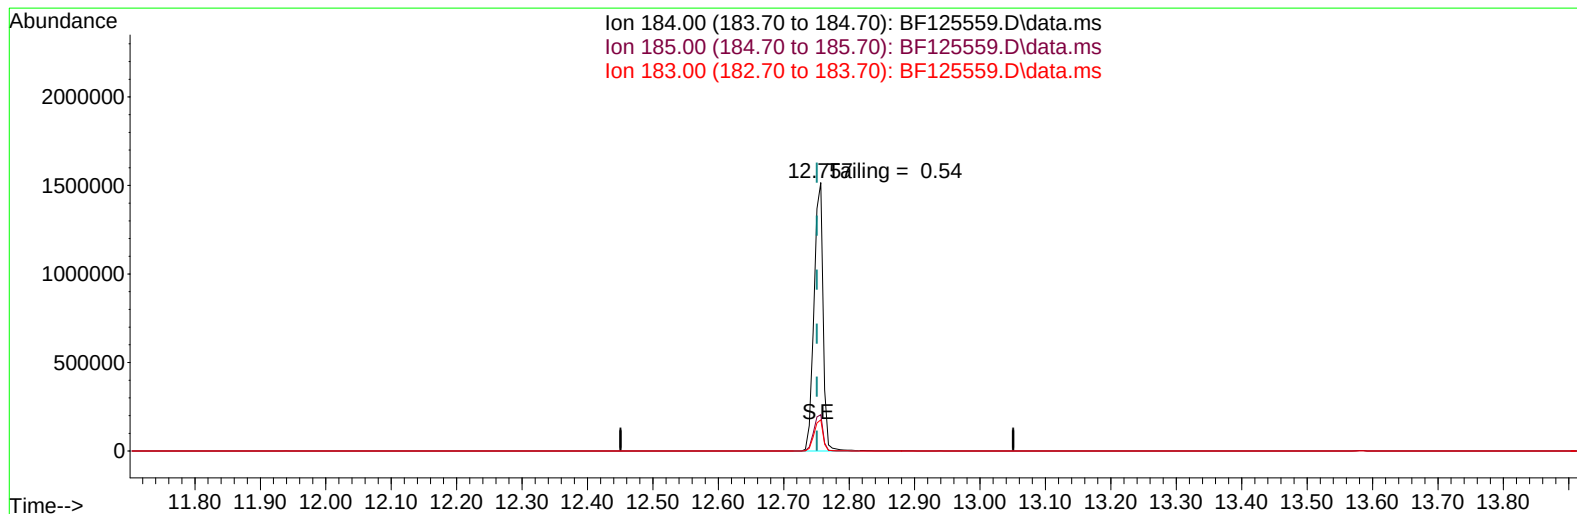

TIC: BF125559.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 1469856

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.57
183.00	10.10	11.66
0.00	0.00	0.00