

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
 Data File : BF135395.D
 Acq On : 22 Sep 2023 12:03
 Operator : CG\JU
 Sample : PB155675BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155675BL

Quant Time: Sep 23 04:40:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.757	152	134913	20.000	ng	0.00
21) Naphthalene-d8	8.033	136	514137	20.000	ng	#-0.01
39) Acenaphthene-d10	9.792	164	249775	20.000	ng	-0.01
64) Phenanthrene-d10	11.286	188	471705	20.000	ng	# 0.00
76) Chrysene-d12	13.945	240	259953	20.000	ng	0.00
86) Perylene-d12	15.415	264	255986	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.398	112	1080872	130.305	ng	0.01
7) Phenol-d6	6.404	99	1364522	129.369	ng	0.00
23) Nitrobenzene-d5	7.322	82	859557	90.830	ng	-0.01
42) 2,4,6-Tribromophenol	10.592	330	290636	117.090	ng	0.00
45) 2-Fluorobiphenyl	9.116	172	1411044	85.232	ng	-0.01
79) Terphenyl-d14	12.886	244	1352346	80.645	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.322	70	115613	17.696	ng	# 78
25) Isophorone	7.322	82	859551	49.464	ng	# 65
50) Dimethylphthalate	9.792	163	45891	2.717	ng	# 1
51) 2,6-Dinitrotoluene	9.792	165	32257	8.719	ng	# 17
57) 2,4-Dinitrotoluene	9.792	165	32257	6.965	ng	# 18
67) 4-Bromophenyl-phenylether	10.592	248	18109	3.860	ng	# 1
77) Benzidine	12.886	184	16393	3.078	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135395.D
Acq On : 22 Sep 2023 12:03
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL

Quant Time: Sep 23 04:40:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration




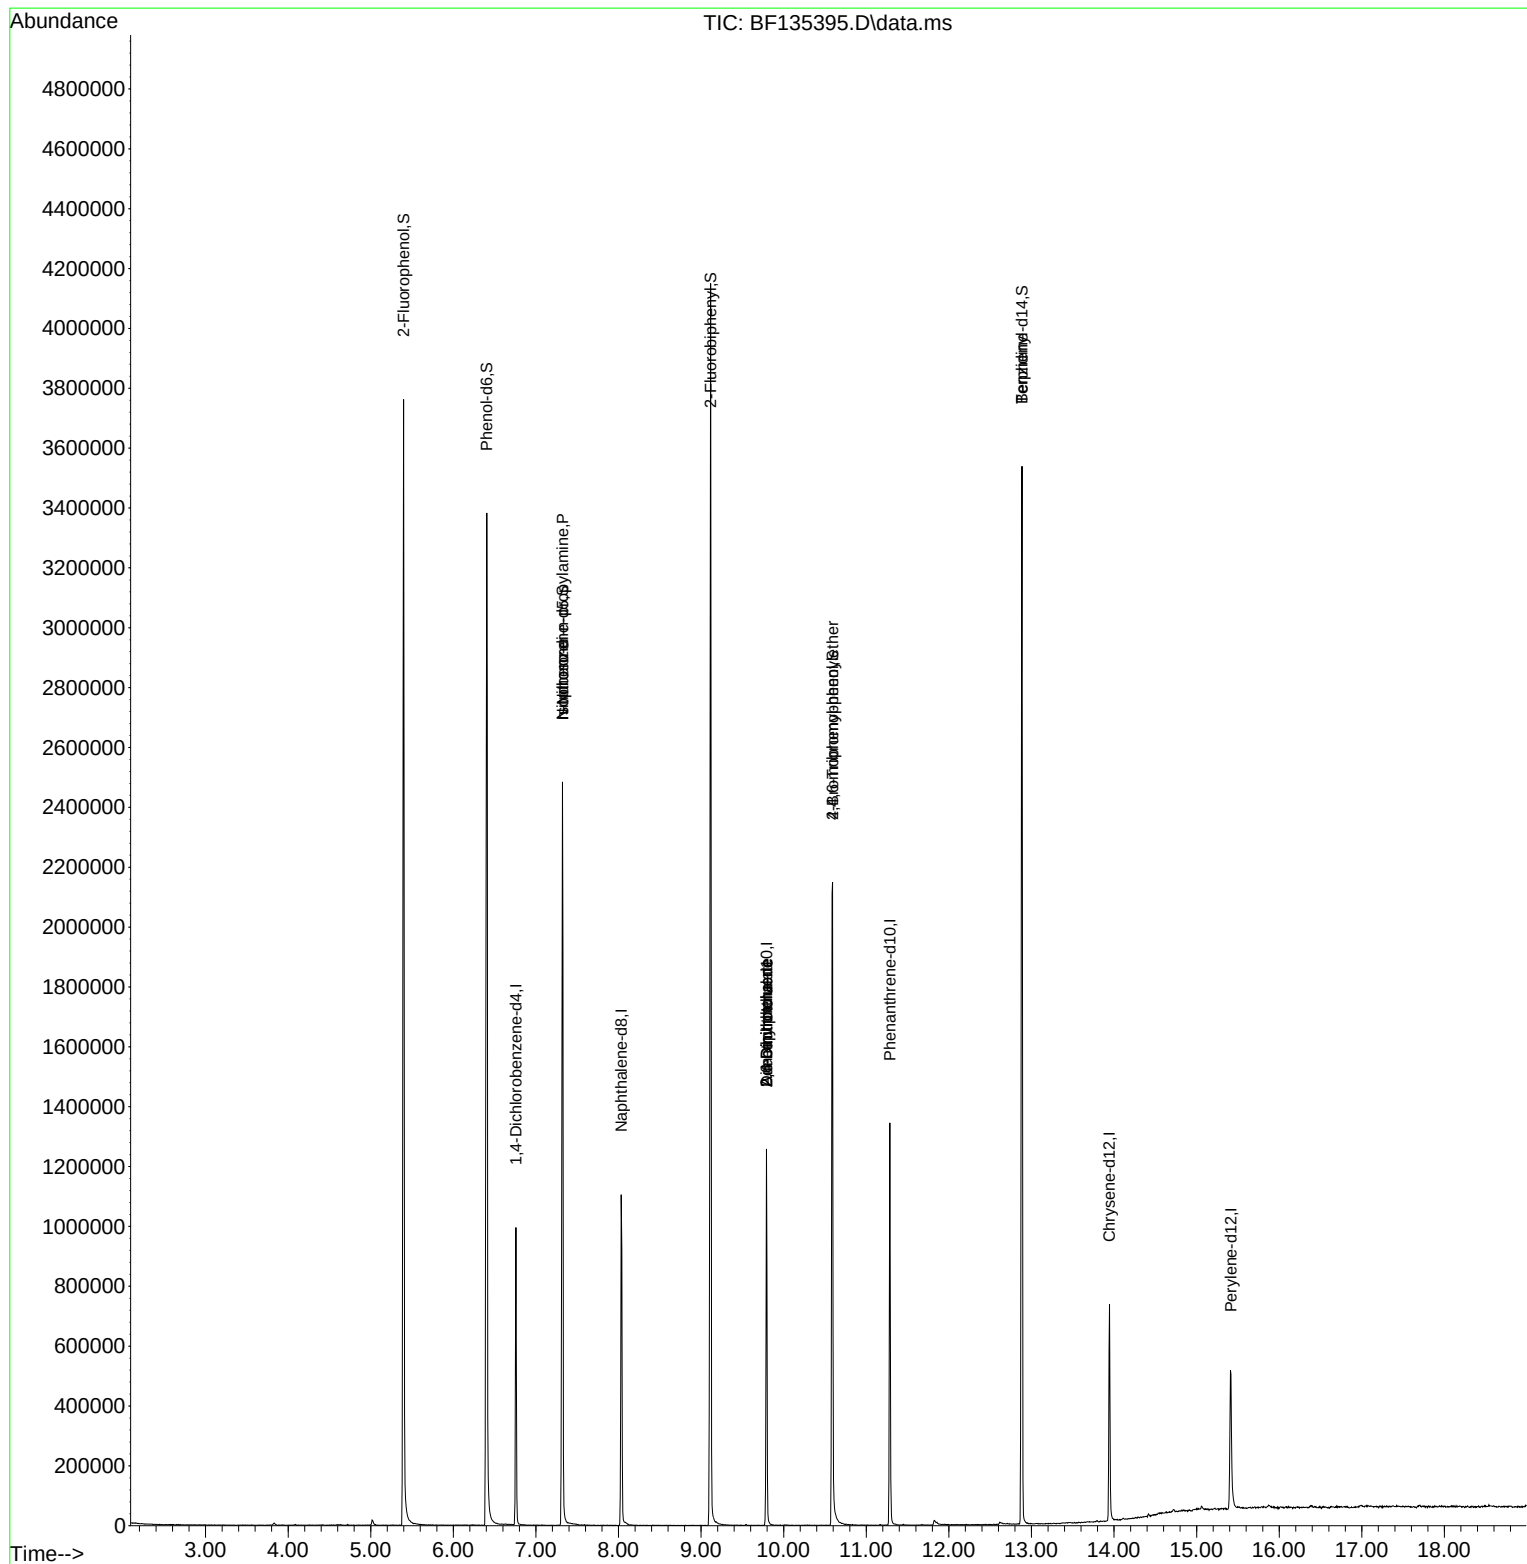




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.757 min Scan# 795
Delta R.T. -0.006 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03




Instrument :
BNA_F
ClientSampleId :
PB155675BL


Tgt Ion:152 Resp: 134913
Ion Ratio Lower Upper
152 100
150 160.6 127.8 191.6
115 59.6 49.8 74.8

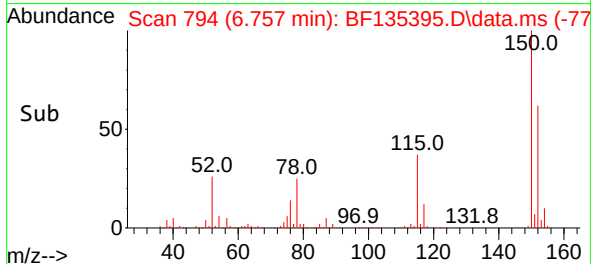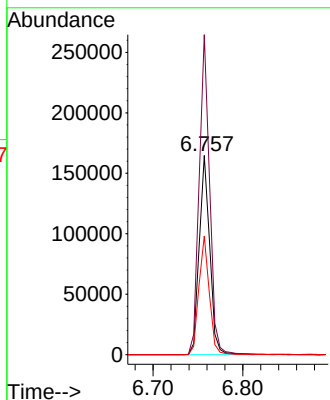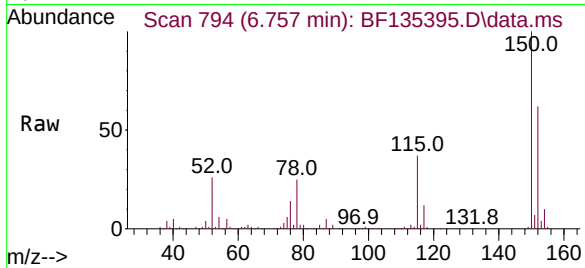

#5
2-Fluorophenol
Concen: 130.305 ng
RT: 5.398 min Scan# 563
Delta R.T. 0.012 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03

Tgt Ion:112 Resp: 1080872
Ion Ratio Lower Upper
112 100
64 68.1 55.9 83.9
63 35.1 29.0 43.6


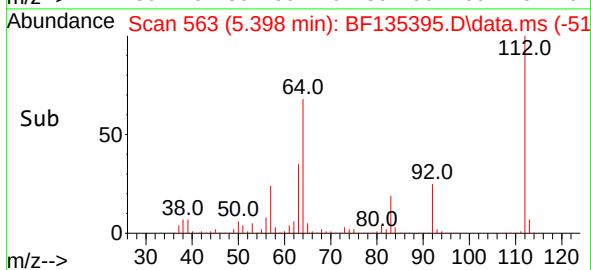
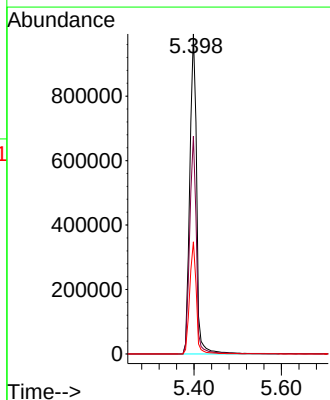
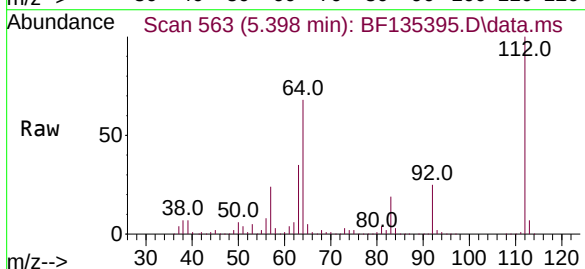




#7
Phenol-d6
Concen: 129.369 ng
RT: 6.404 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03




Instrument :
BNA_F
ClientSampleId :
PB155675BL


Tgt Ion: 99 Resp: 1364522
Ion Ratio Lower Upper
99 100
42 23.2 17.9 26.9
71 32.8 27.0 40.6

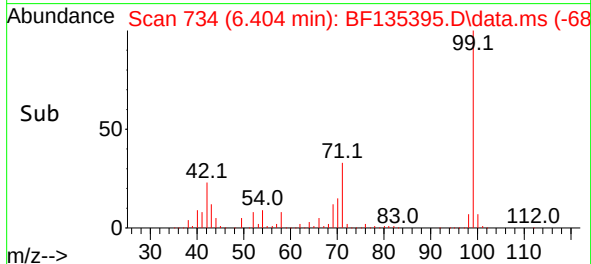

#19
n-Nitroso-di-n-propylamine
Concen: 17.696 ng
RT: 7.322 min Scan# 890
Delta R.T. 0.135 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03

Tgt Ion: 70 Resp: 115613
Ion Ratio Lower Upper
70 100
42 57.0 55.4 83.0
101 0.0 7.7 11.5#
130 2.0 17.0 25.6#


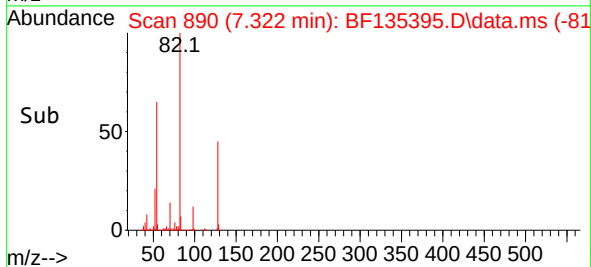

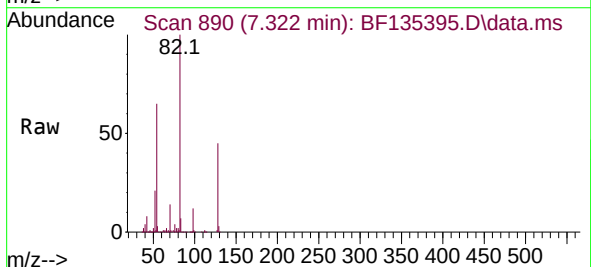




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.033 min Scan# 1011
Delta R.T. -0.012 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03




Instrument :
BNA_F
ClientSampleId :
PB155675BL


Tgt Ion:136	Resp: 514137
Ion Ratio	Lower Upper
136	100
137	11.4 8.8 13.2
54	11.4 7.7 11.5
68	7.1 4.6 6.8

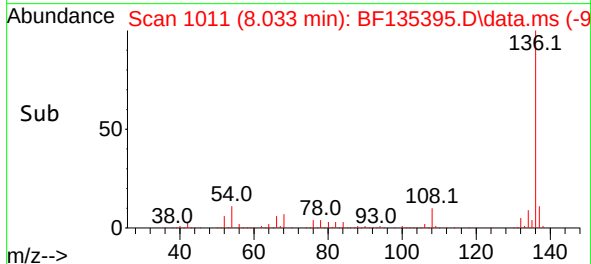

#23
Nitrobenzene-d5
Concen: 90.830 ng
RT: 7.322 min Scan# 890
Delta R.T. -0.012 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03

Tgt Ion: 82	Resp: 859557
Ion Ratio	Lower Upper
82	100
128	45.1 35.8 53.6
54	65.1 50.6 76.0


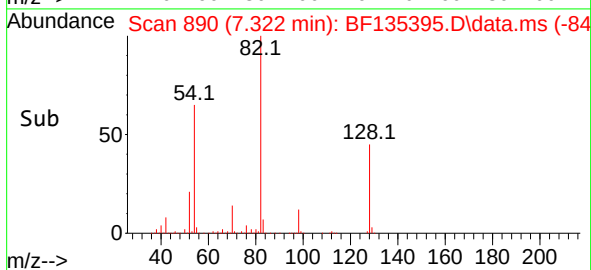

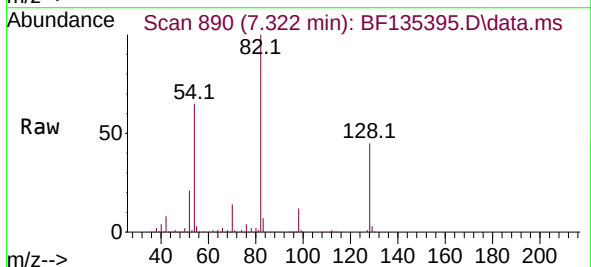




#25
Isophorone
Concen: 49.464 ng
RT: 7.322 min Scan# 89
Delta R.T. -0.271 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03




Instrument :
BNA_F
ClientSampleId :
PB155675BL


Tgt Ion: 82 Resp: 859551
Ion Ratio Lower Upper
82 100
95 0.0 6.0 9.0#
138 0.0 14.5 21.7#

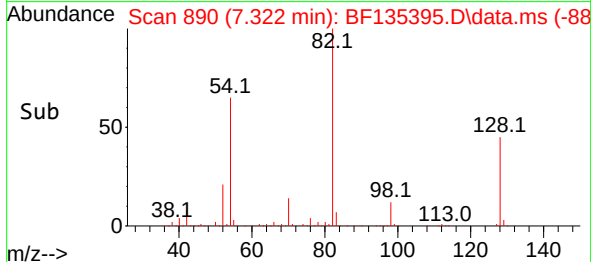

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.792 min Scan# 1310
Delta R.T. -0.012 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03

Tgt Ion: 164 Resp: 249775
Ion Ratio Lower Upper
164 100
162 100.6 81.0 121.4
160 45.8 37.0 55.4

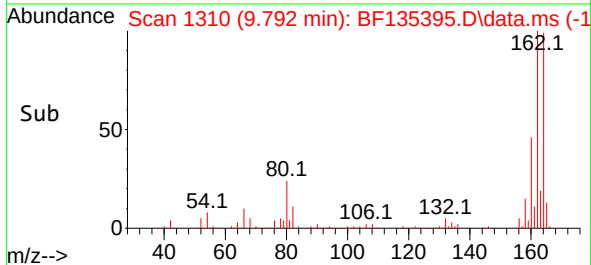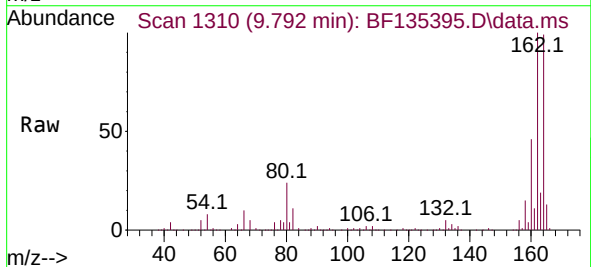



#42

2,4,6-Tribromophenol

Concen: 117.090 ng

RT: 10.592 min Scan# 1446

Delta R.T. -0.006 min

Lab File: BF135395.D

Acq: 22 Sep 2023 12:03

Instrument :

BNA_F

ClientSampleId :

PB155675BL





Tgt Ion:330 Resp: 290636

Ion Ratio Lower Upper

330 100

332 94.7 77.3 115.9

141 34.0 25.8 38.8

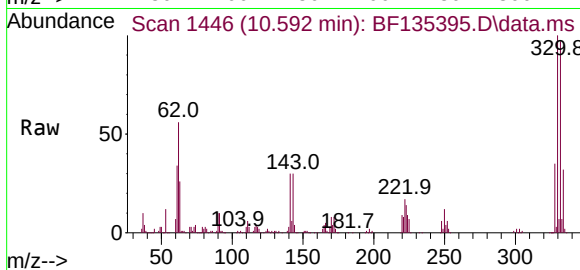

#45

2-Fluorobiphenyl

Concen: 85.232 ng

RT: 9.116 min Scan# 1195

Delta R.T. -0.012 min

Lab File: BF135395.D

Acq: 22 Sep 2023 12:03




Tgt Ion:172 Resp: 1411044


Ion Ratio Lower Upper

172 100

171 35.6 28.4 42.6

170 24.1 19.0 28.4


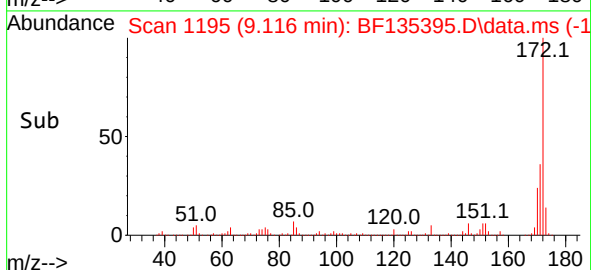

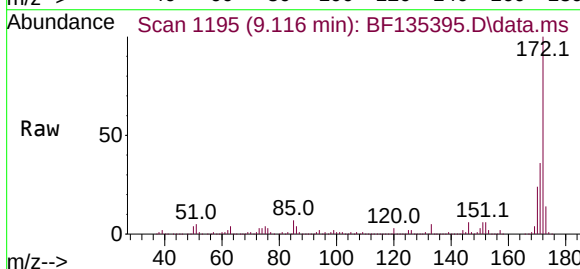




#50
Dimethylphthalate
Concen: 2.717 ng
RT: 9.792 min Scan# 11
Delta R.T. 0.259 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03




Instrument :
BNA_F
ClientSampleId :
PB155675BL


Tgt Ion:163 Resp: 45891
Ion Ratio Lower Upper
163 100
194 0.0 3.1 4.7#
164 530.2 8.1 12.1#

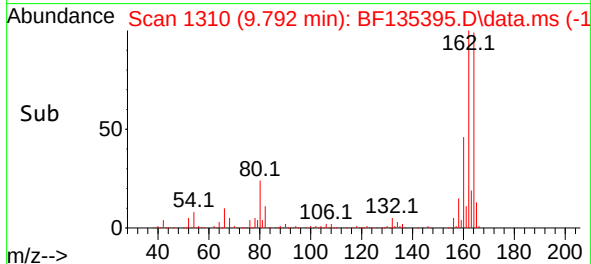

#51
2,6-Dinitrotoluene
Concen: 8.719 ng
RT: 9.792 min Scan# 1310
Delta R.T. 0.200 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03


Tgt Ion:165 Resp: 32257
Ion Ratio Lower Upper
165 100
63 1.3 59.4 89.2#
89 1.0 49.8 74.8#

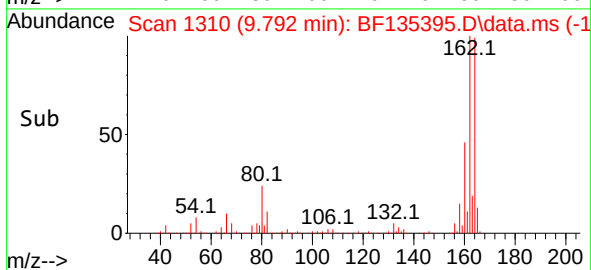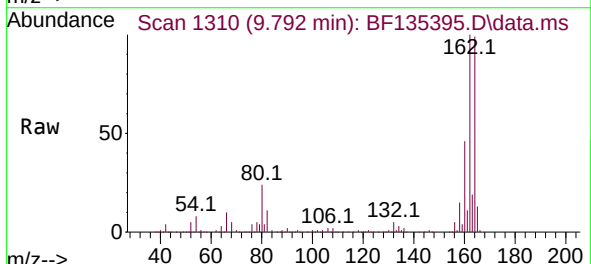






#57
2,4-Dinitrotoluene
Concen: 6.965 ng
RT: 9.792 min Scan# 11
Delta R.T. -0.212 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03


Instrument :
BNA_F
ClientSampleId :
PB155675BL

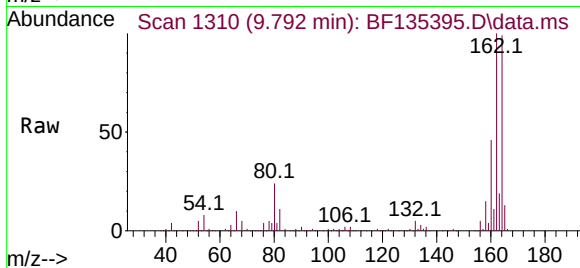



Tgt Ion:165 Resp: 32257
Ion Ratio Lower Upper
165 100
63 1.3 50.1 75.1#
89 1.0 59.3 88.9#
182 0.0 2.3 3.5#




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.286 min Scan# 1564
Delta R.T. -0.006 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03

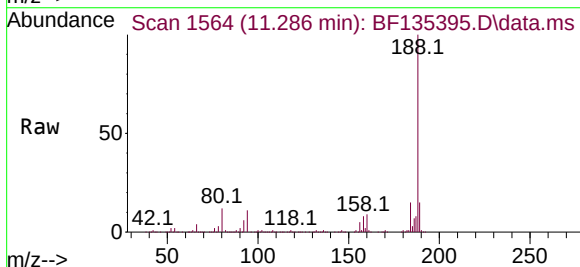

Tgt Ion:188 Resp: 471705
Ion Ratio Lower Upper
188 100
94 10.7 7.0 10.6#
80 11.9 7.5 11.3#





#67

4-Bromophenyl-phenylether

Concen: 3.860 ng

RT: 10.592 min Scan# 14

Delta R.T. -0.247 min

Lab File: BF135395.D

Acq: 22 Sep 2023 12:03

Instrument :

BNA_F

ClientSampleId :

PB155675BL





Tgt Ion:248 Resp: 18109

Ion Ratio Lower Upper

248 100

250 197.9 78.6 117.8#

141 498.2 54.2 81.2#

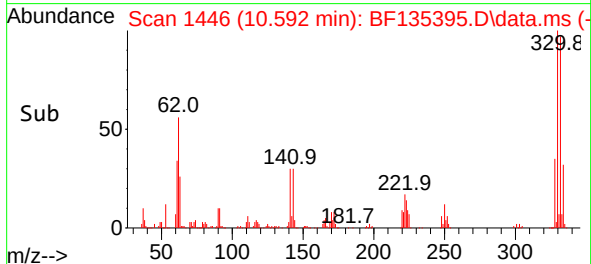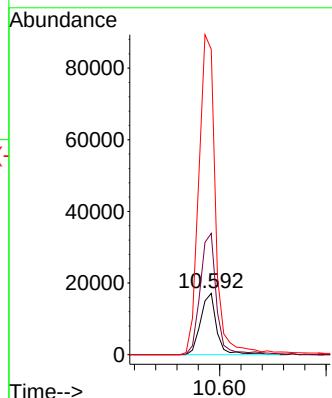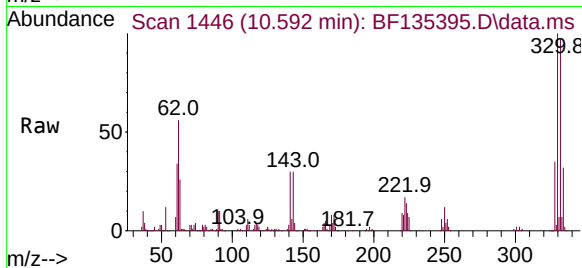

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.945 min Scan# 2016

Delta R.T. 0.000 min

Lab File: BF135395.D

Acq: 22 Sep 2023 12:03




Tgt Ion:240 Resp: 259953


Ion Ratio Lower Upper

240 100

120 12.7 9.4 14.2

236 25.9 19.8 29.8



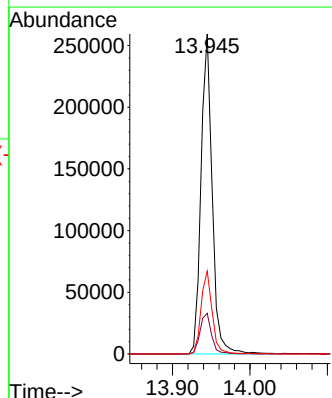
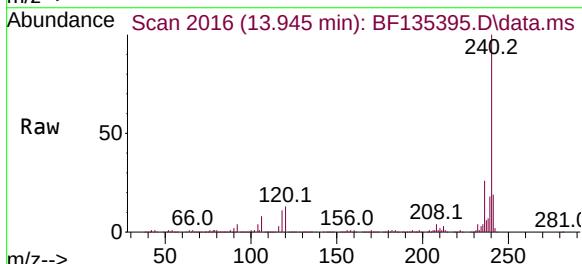




#77
Benzidine
Concen: 3.078 ng
RT: 12.886 min Scan# 1836
Delta R.T. 0.247 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03




Instrument :
BNA_F
ClientSampleId :
PB155675BL


Tgt Ion:184 Resp: 16393
Ion Ratio Lower Upper
184 100
185 18.8 11.7 17.5#
183 7.0 8.2 12.4#

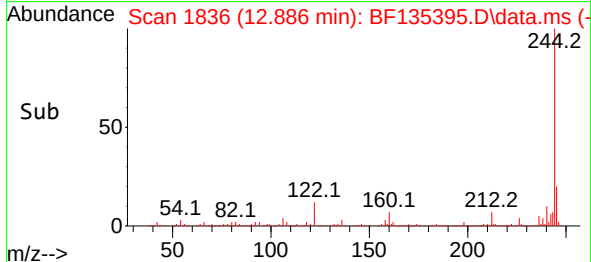

#79
Terphenyl-d14
Concen: 80.645 ng
RT: 12.886 min Scan# 1836
Delta R.T. -0.006 min
Lab File: BF135395.D
Acq: 22 Sep 2023 12:03

Tgt Ion:244 Resp: 1352346
Ion Ratio Lower Upper
244 100
212 7.0 5.1 7.7
122 12.0 7.9 11.9#

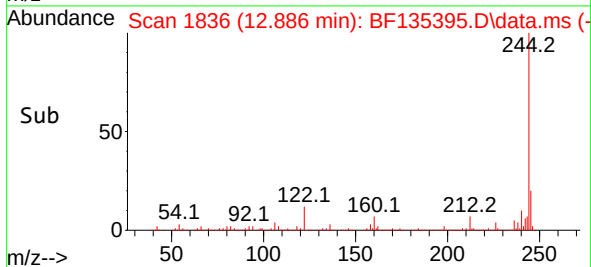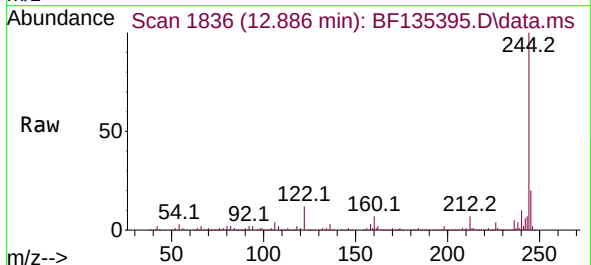

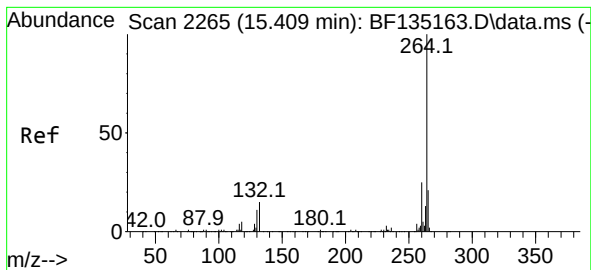

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.415 min Scan# 21

Delta R.T. 0.006 min

Lab File: BF135395.D


Acq: 22 Sep 2023 12:03

Instrument :

BNA_F

ClientSampleId :

PB155675BL

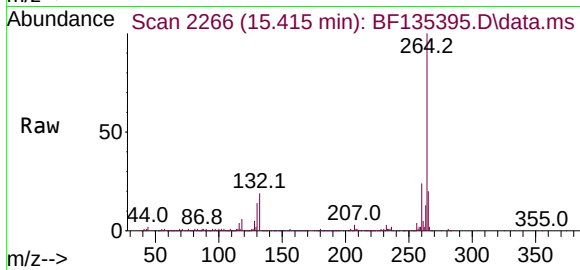

Tgt Ion:264 Resp: 255986

Ion Ratio Lower Upper

264 100

260 24.2 19.8 29.6

265 20.3 17.0 25.4

