
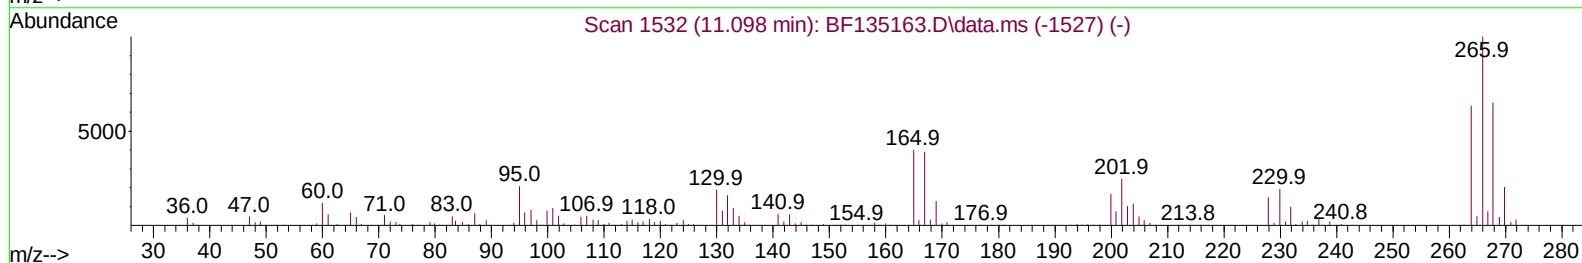
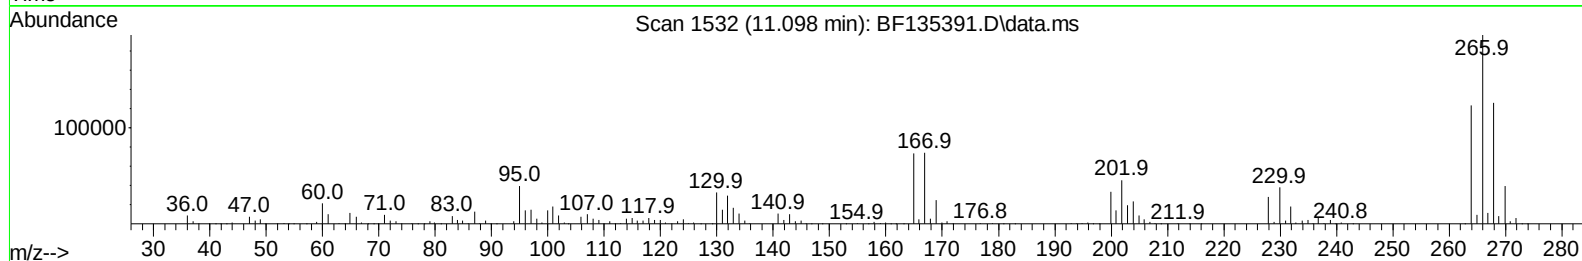


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135391.D
Acq On : 22 Sep 2023 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 06:01:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

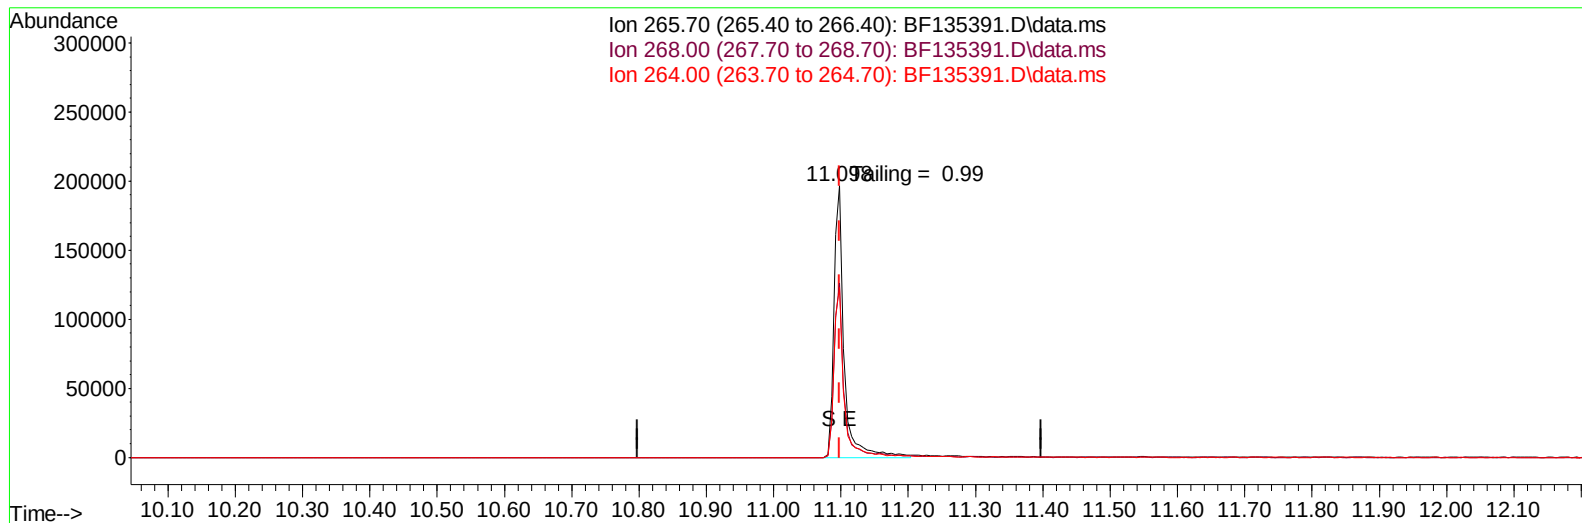

TIC: BF135391.D\data.ms

(70) Pentachlorophenol (C)




11.098min (+ 0.000) 41091.90 ng

response 207507

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.18
264.00	63.50	62.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135391.D
Acq On : 22 Sep 2023 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 23 06:01:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

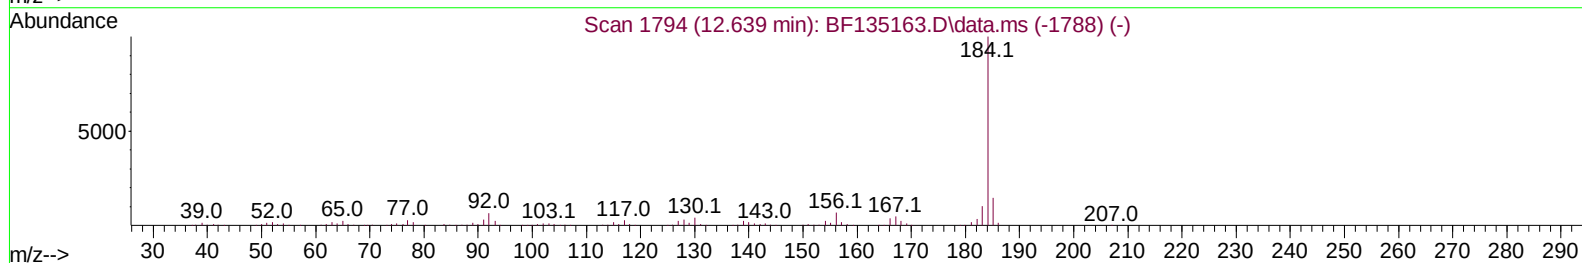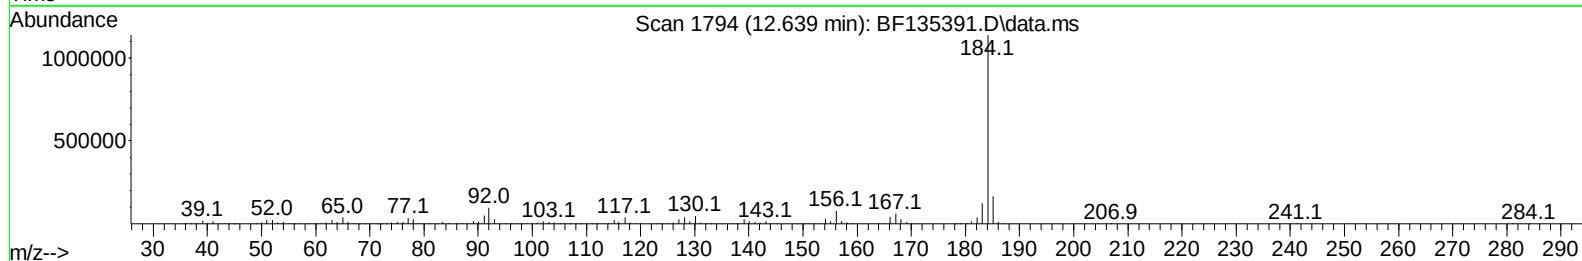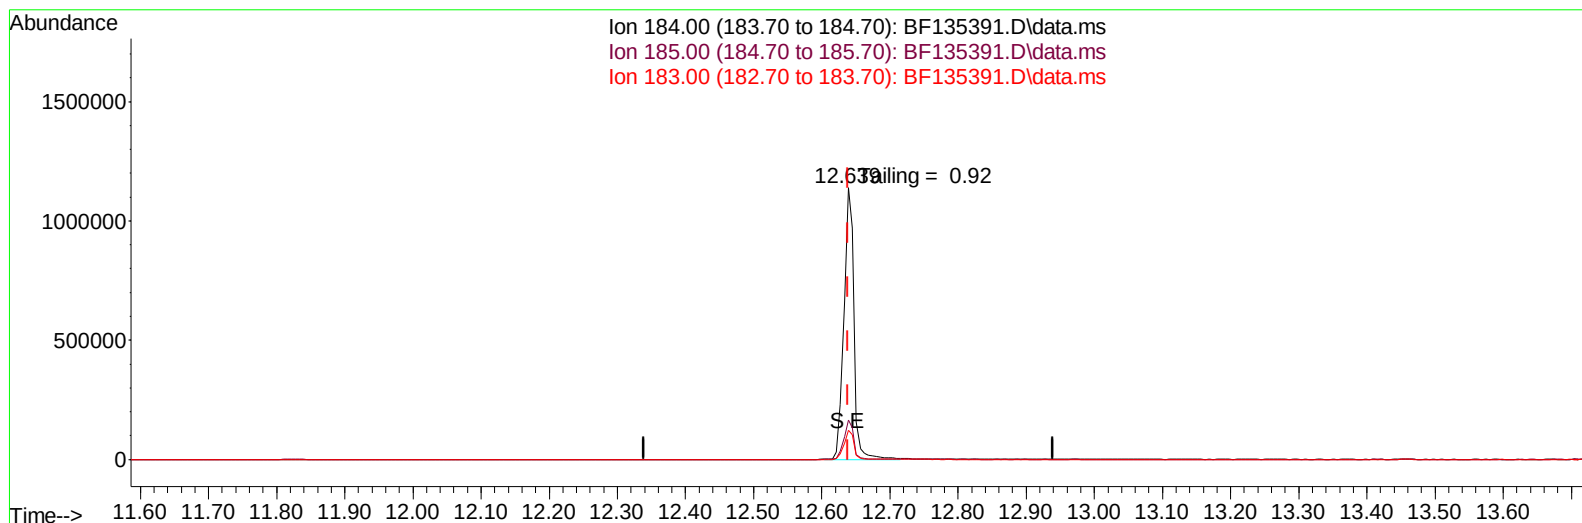

TIC: BF135391.D\data.ms

(77) Benzidine**12.639min (+ 0.000) 467921.80 ng m****response 1179107**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.49
183.00	10.30	10.76
0.00	0.00	0.00