

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
 Data File : BF135393.D
 Acq On : 22 Sep 2023 11:00
 Operator : CG\JU
 Sample : PB155676BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155676BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	559	563	586	rBV	3706223	4182950	97.30%	14.857%
2	6.404	729	734	737	rBV	3426412	4065511	94.57%	14.440%
3	6.757	790	794	803	rBV	1155676	918632	21.37%	3.263%
4	7.322	885	890	893	rBV	2550434	2756065	64.11%	9.789%
5	8.034	1007	1011	1015	rBV	1289507	1169190	27.20%	4.153%
6	9.116	1189	1195	1198	rBV	4165313	4298882	100.00%	15.269%
7	9.792	1305	1310	1322	rBV	1481876	1276975	29.70%	4.536%
8	10.592	1441	1446	1465	rBV	2259304	2561280	59.58%	9.097%
9	11.286	1560	1564	1572	rBV	1557634	1309841	30.47%	4.652%
10	11.822	1649	1655	1664	rBV4	29026	59317	1.38%	0.211%
11	12.886	1831	1836	1839	rBV	3781620	3860173	89.79%	13.711%
12	13.939	2012	2015	2025	rVB	837255	880271	20.48%	3.127%
13	15.410	2260	2265	2276	rBV	565097	814774	18.95%	2.894%




Sum of corrected areas: 28153861

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135393.D
Acq On : 22 Sep 2023 11:00
Operator : CG\JU
Sample : PB155676BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155676BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

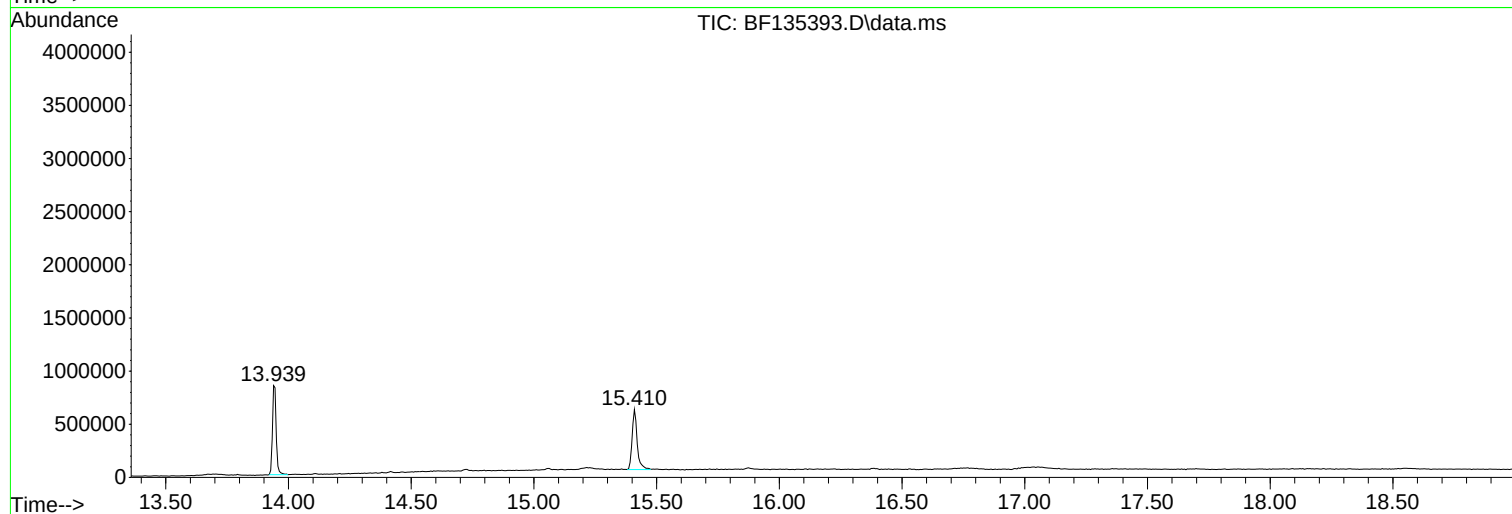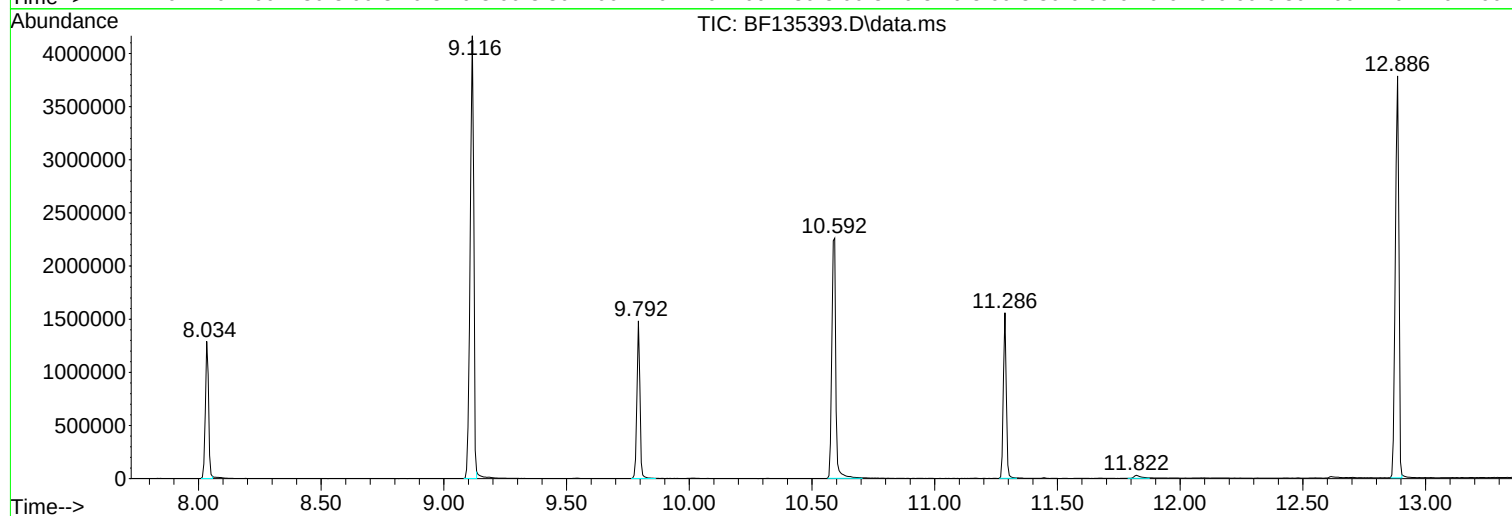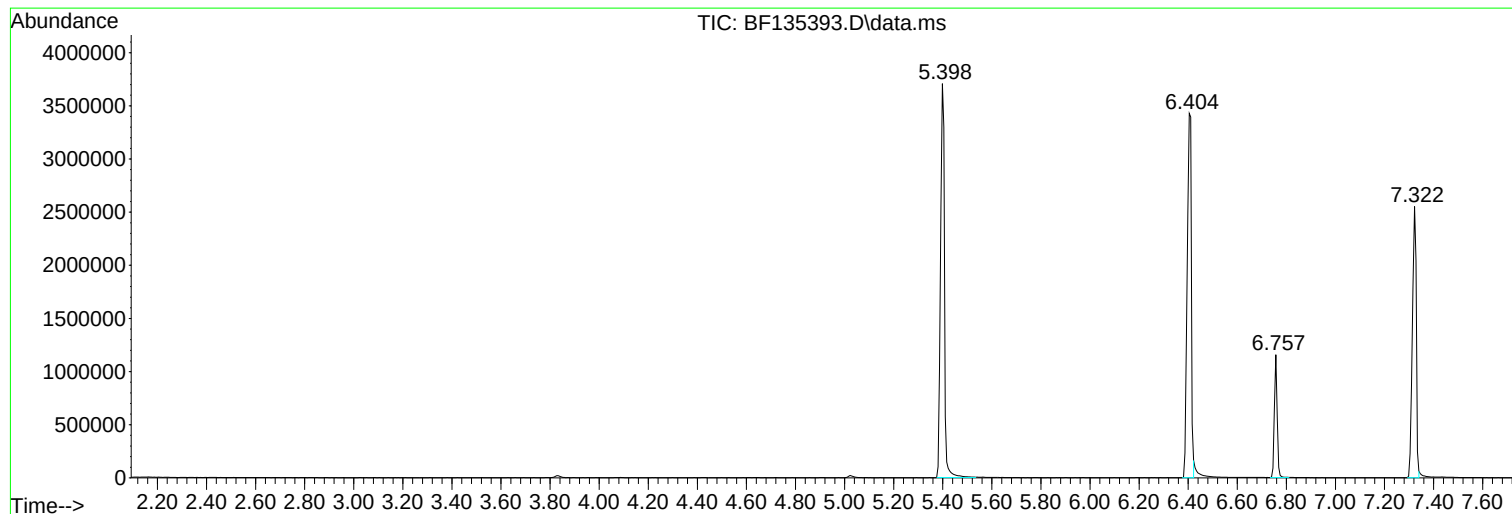

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135393.D
Acq On : 22 Sep 2023 11:00
Operator : CG\JU
Sample : PB155676BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155676BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135393.D
Acq On : 22 Sep 2023 11:00
Operator : CG\JU
Sample : PB155676BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155676BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------