

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
 Data File : BF135395.D
 Acq On : 22 Sep 2023 12:03
 Operator : CG\JU
 Sample : PB155675BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155675BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	559	563	566	rBV	3759915	3824147	95.29%	14.827%
2	6.404	729	734	737	rBV	3382053	3855378	96.07%	14.948%
3	6.757	790	794	804	rBV	993127	806491	20.10%	3.127%
4	7.322	885	890	893	rBV	2483249	2600073	64.79%	10.081%
5	8.033	1007	1011	1028	rBV	1105009	1055551	26.30%	4.093%
6	9.116	1189	1195	1198	rBV	4148925	4013021	100.00%	15.559%
7	9.792	1305	1310	1324	rBV	1257335	1107578	27.60%	4.294%
8	10.592	1441	1446	1462	rBV	2148747	2397447	59.74%	9.295%
9	11.286	1560	1564	1573	rBV	1343608	1134562	28.27%	4.399%
10	12.886	1831	1836	1839	rBV	3533590	3550577	88.48%	13.766%
11	13.945	2012	2016	2027	rBV	721626	732133	18.24%	2.839%
12	15.409	2260	2265	2279	rBV	464142	714730	17.81%	2.771%




Sum of corrected areas: 25791688

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135395.D
Acq On : 22 Sep 2023 12:03
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

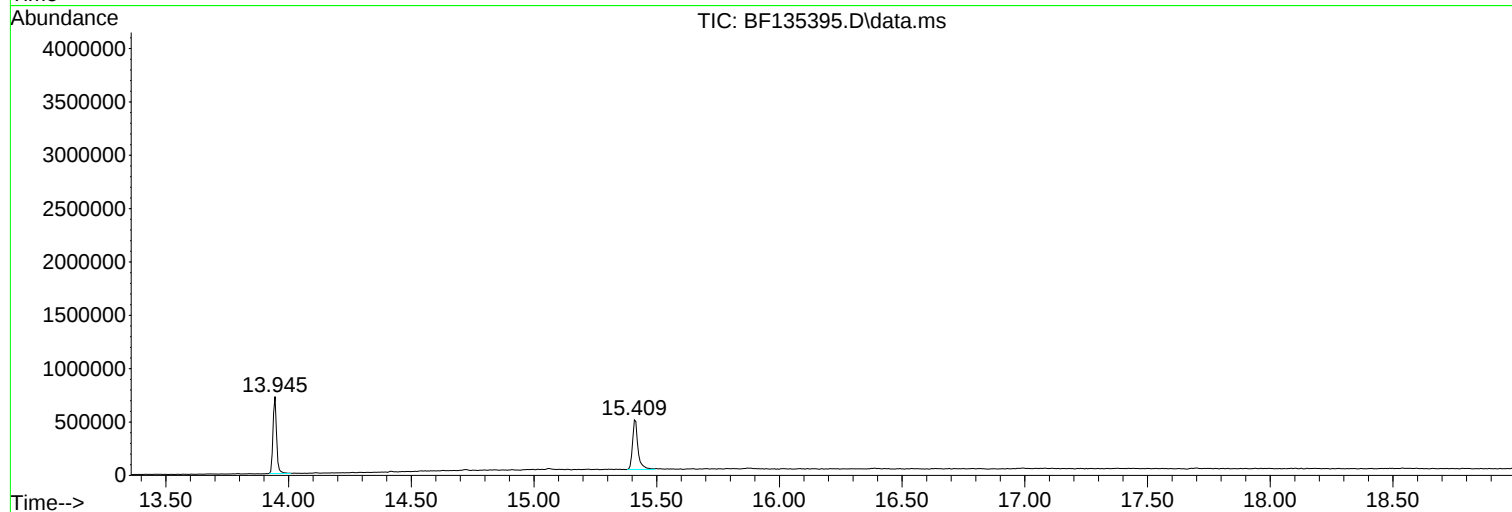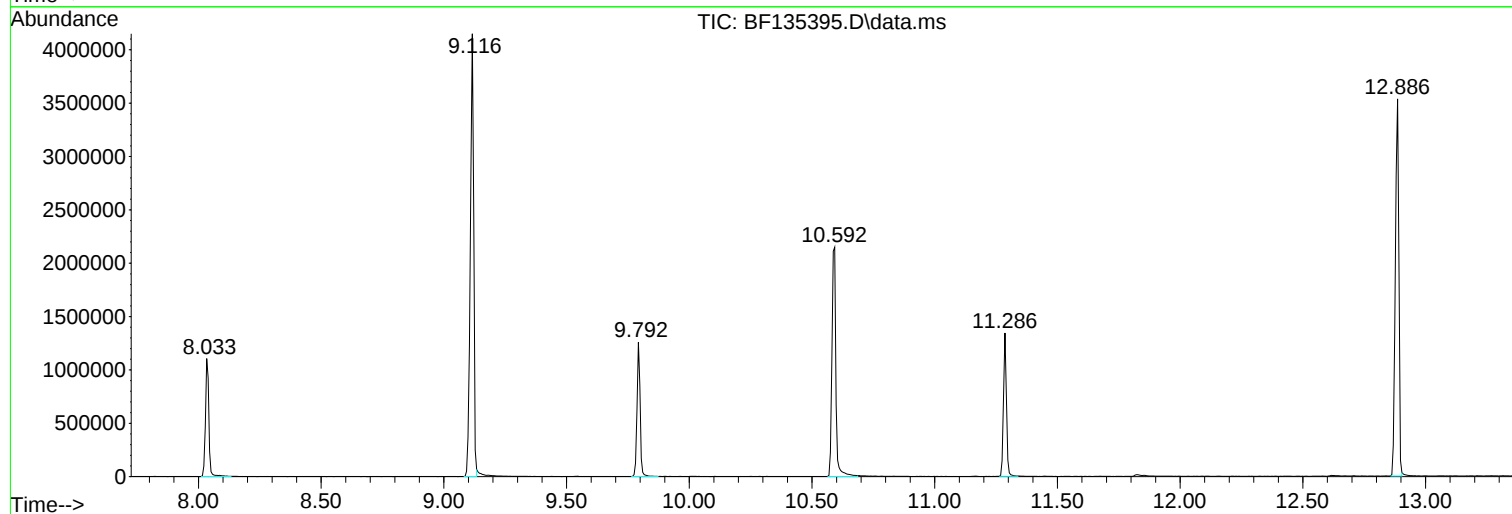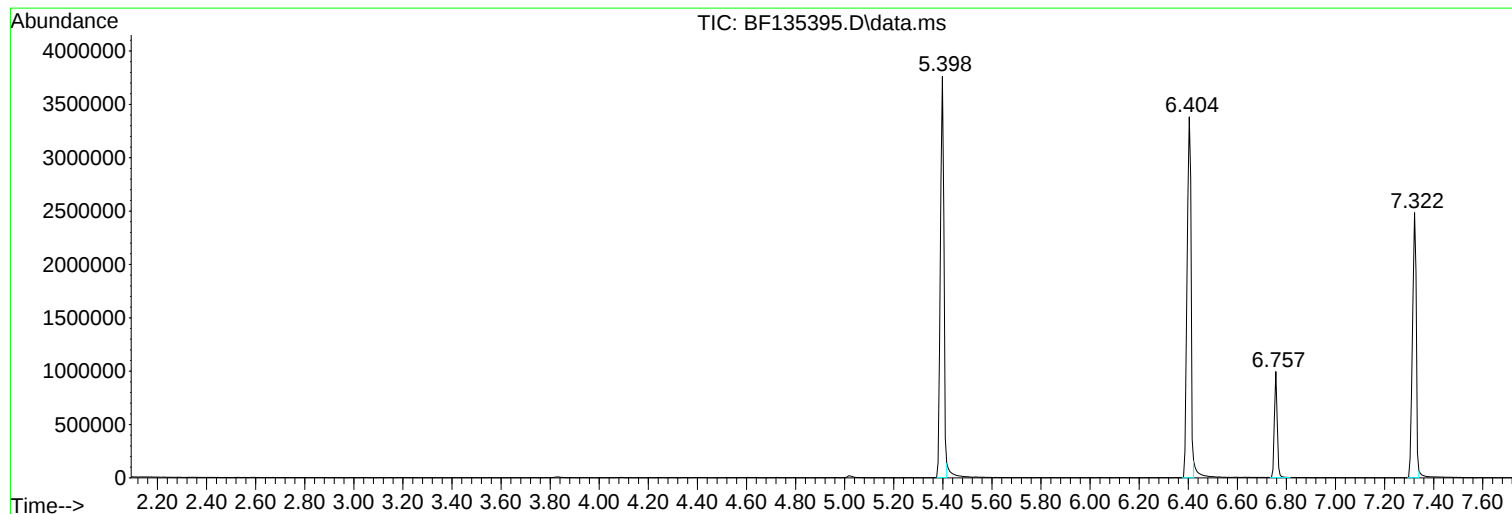

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135395.D
Acq On : 22 Sep 2023 12:03
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135395.D
Acq On : 22 Sep 2023 12:03
Operator : CG\JU
Sample : PB155675BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155675BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------