


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135391.D
Acq On : 22 Sep 2023 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023



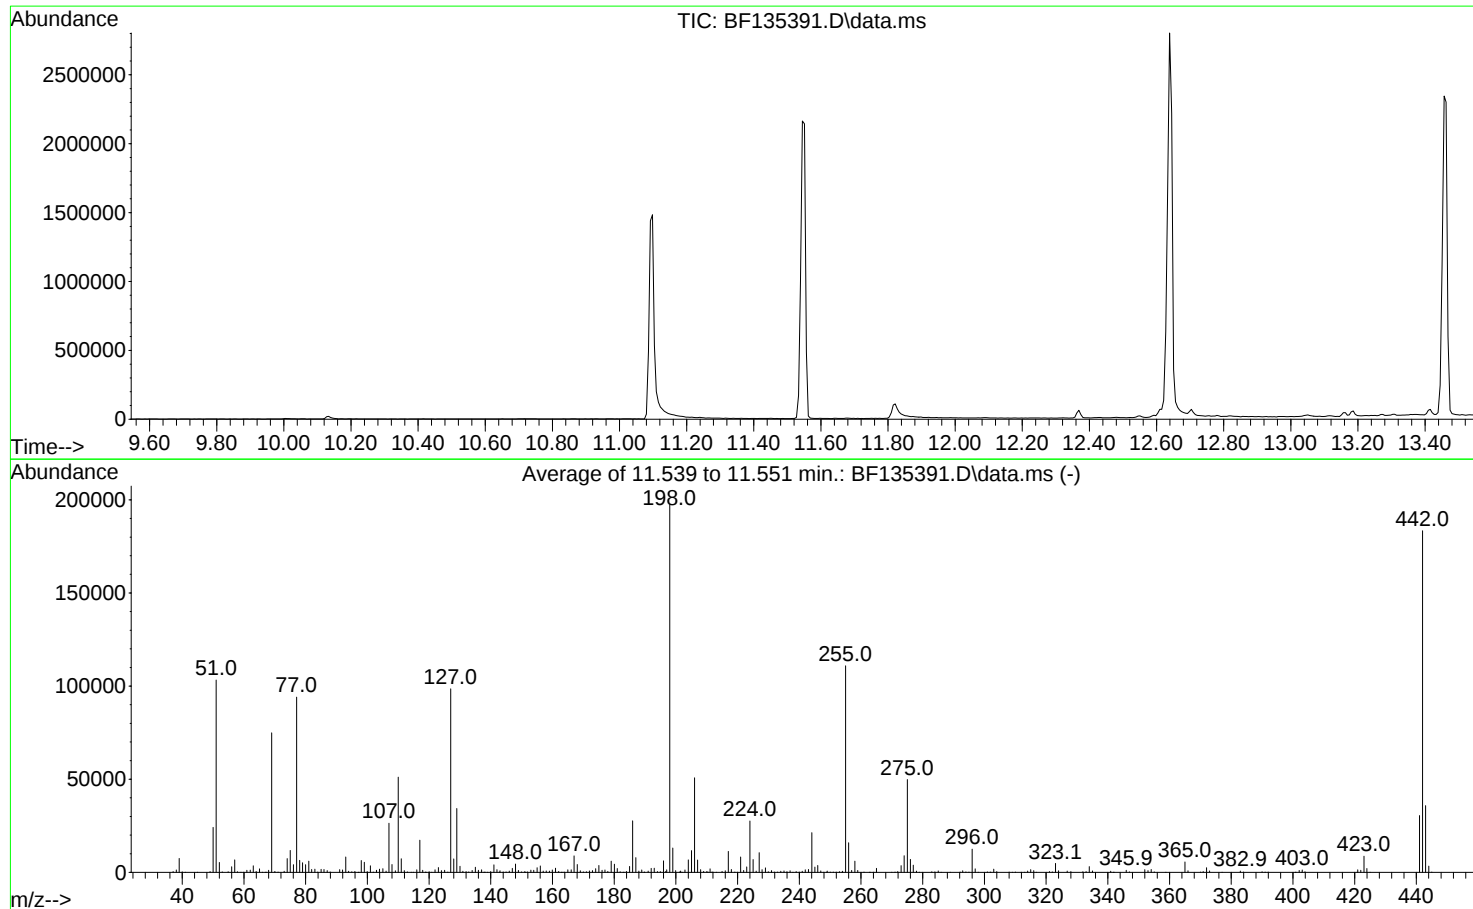


AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	103288	PASS
68	69	0.00	2	1.5	1107	PASS
69	198	0.00	100	37.9	74933	PASS
70	69	0.00	2	0.7	493	PASS
127	198	10	80	49.9	98501	PASS
197	198	0.00	2	0.7	1416	PASS
198	198	100	100	100.0	197499	PASS
199	198	5	9	6.6	13092	PASS
275	198	10	60	25.2	49787	PASS
365	198	1	100	2.8	5550	PASS
441	198	0.01	100	15.5	30541	PASS
442	442	50	100	100.0	183387	PASS
443	442	15	24	19.6	35859	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\  
Data File : BF135391.D  
Acq On    : 22 Sep 2023   09:58  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Sep 23 06:01:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

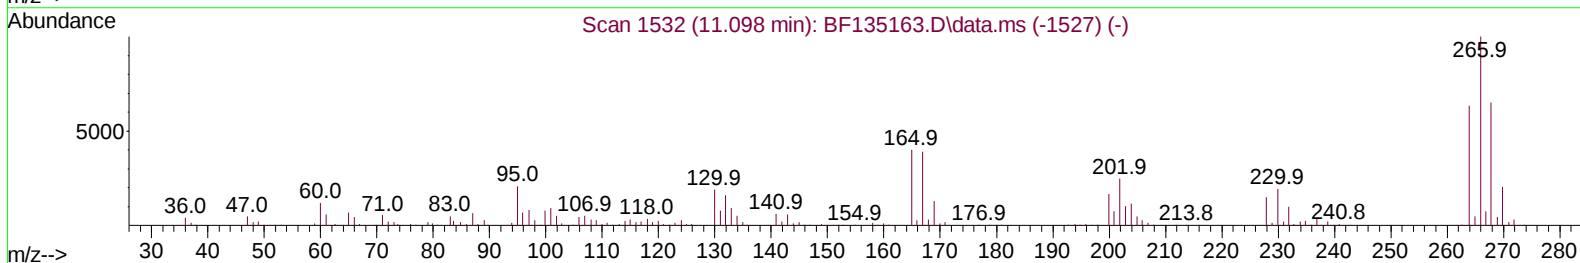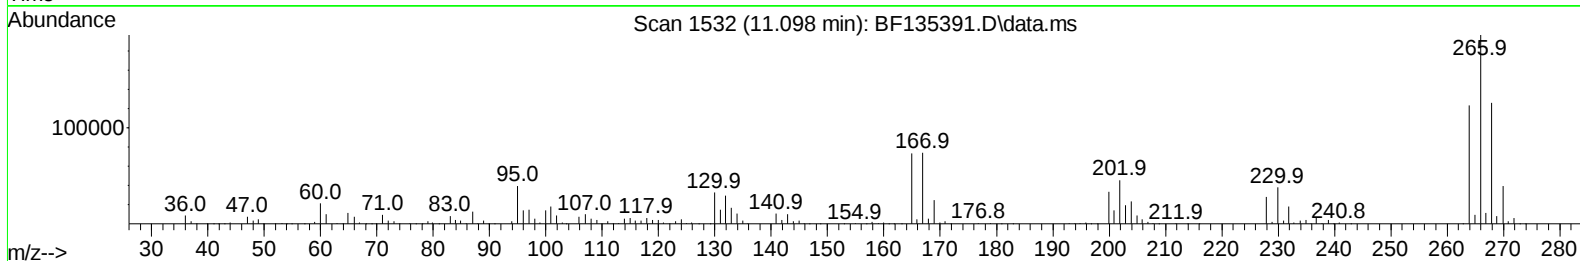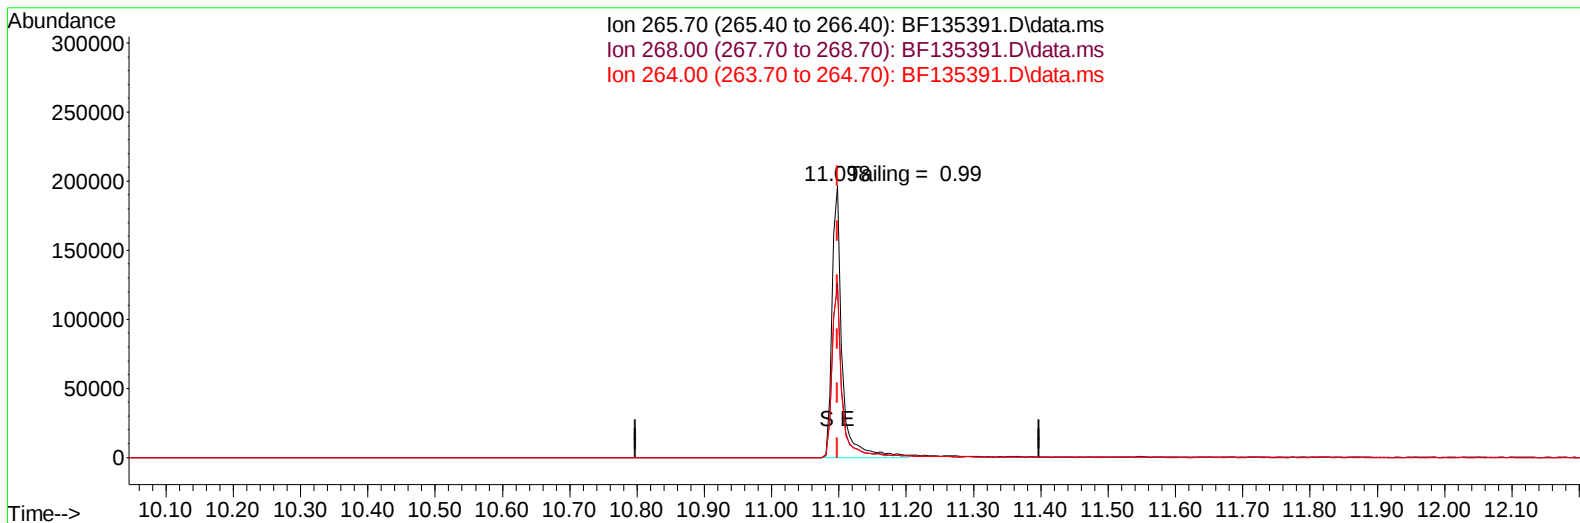

TIC: BF135391.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.000) 41091.90 ng




response **207507**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.18
264.00	63.50	62.68
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\  
Data File : BF135391.D  
Acq On    : 22 Sep 2023   09:58  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 06:01:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

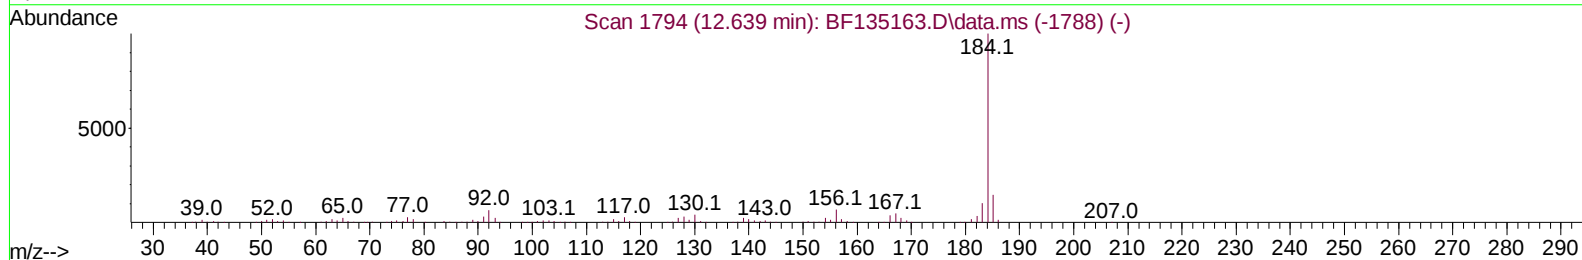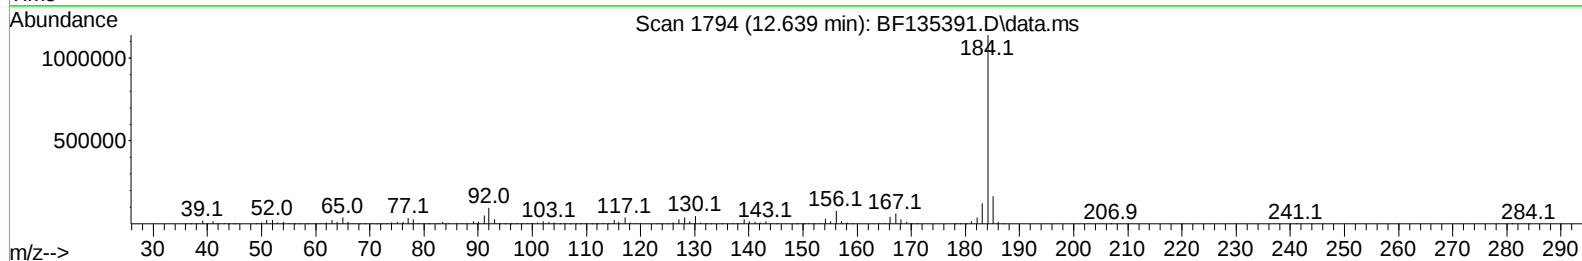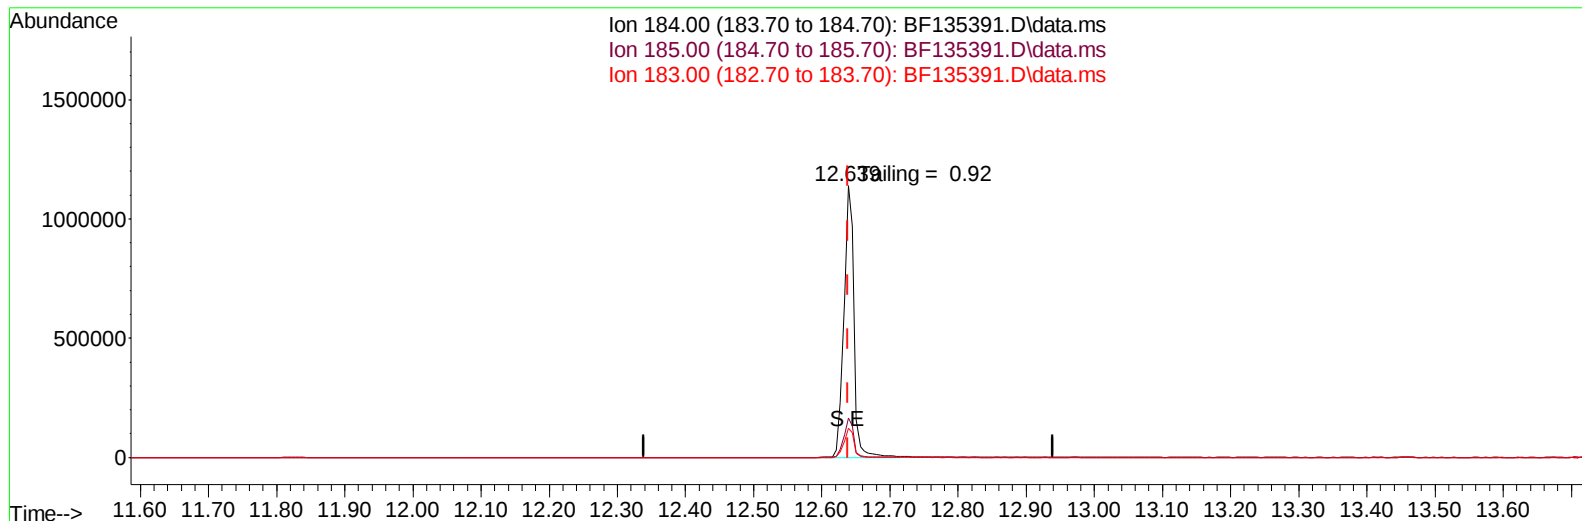

TIC: BF135391.D\data.ms

(77) Benzidine

12.639min (+ 0.000) 467921.80 ng m

response **1179107**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.49
183.00	10.30	10.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2023	BNA_F	<u>BF135391.D</u>
Compound Name	Response	Retention Time
DDT	471680	13.463
DDD	12582	13.186
DDE	1051	12.815
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13633	485313	2.81

Instrument :
BNA_F
ClientSampleId :
DFTPP