


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135400.D
Acq On : 22 Sep 2023 14:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

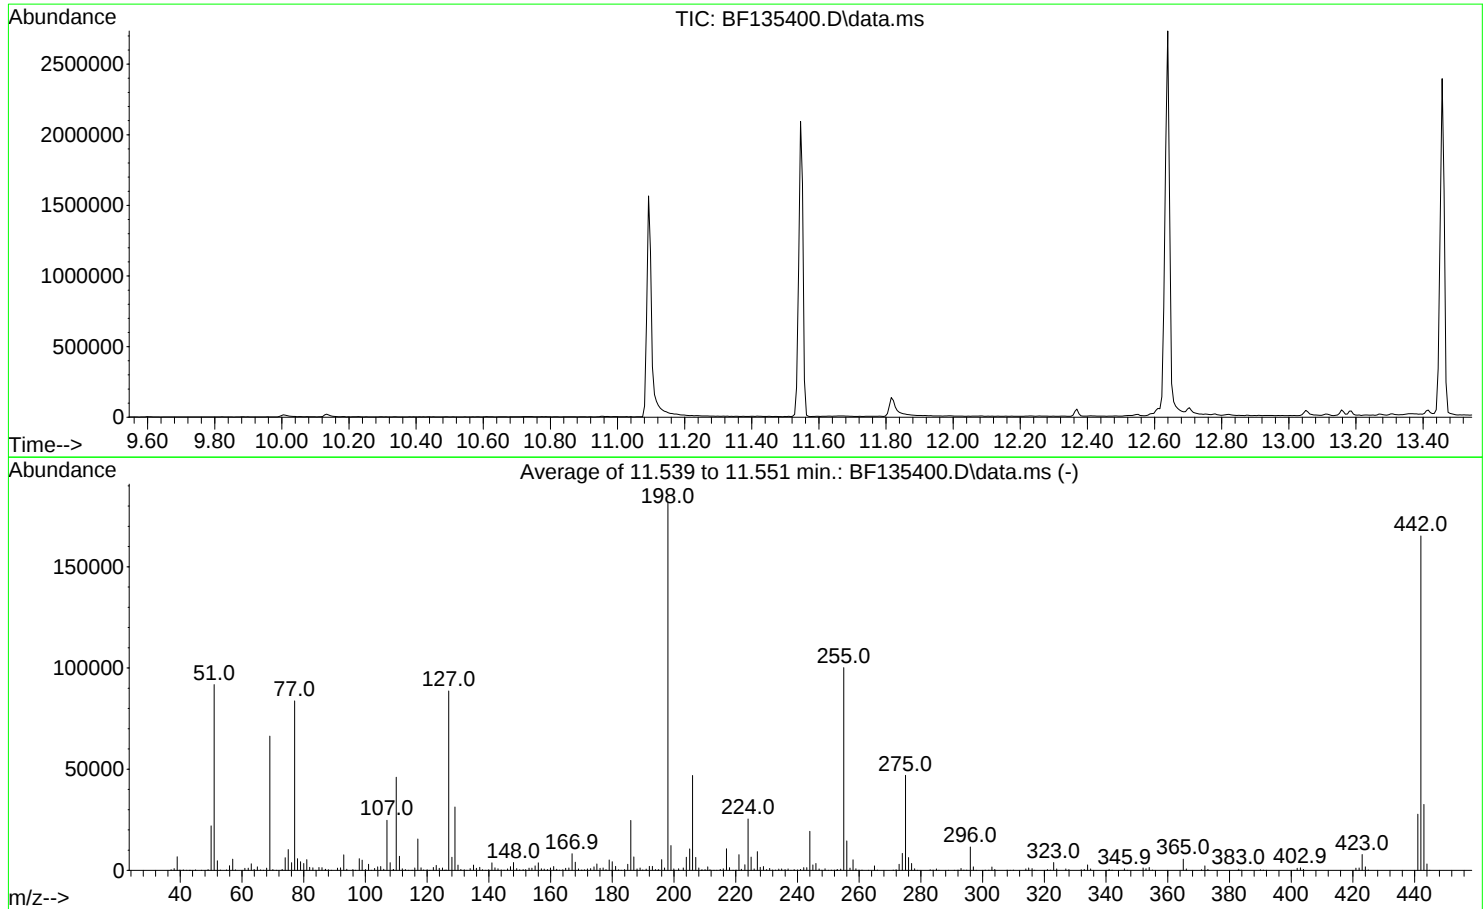




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	91790	PASS
68	69	0.00	2	1.7	1112	PASS
69	198	0.00	100	36.5	66313	PASS
70	69	0.00	2	0.6	428	PASS
127	198	10	80	48.8	88613	PASS
197	198	0.00	2	0.6	1155	PASS
198	198	100	100	100.0	181768	PASS
199	198	5	9	6.8	12302	PASS
275	198	10	60	25.8	46944	PASS
365	198	1	100	3.0	5507	PASS
441	198	0.01	100	15.3	27723	PASS
442	442	50	100	100.0	165272	PASS
443	442	15	24	19.7	32576	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092223\
Data File : BF135400.D
Acq On : 22 Sep 2023 14:44
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 23 06:04:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

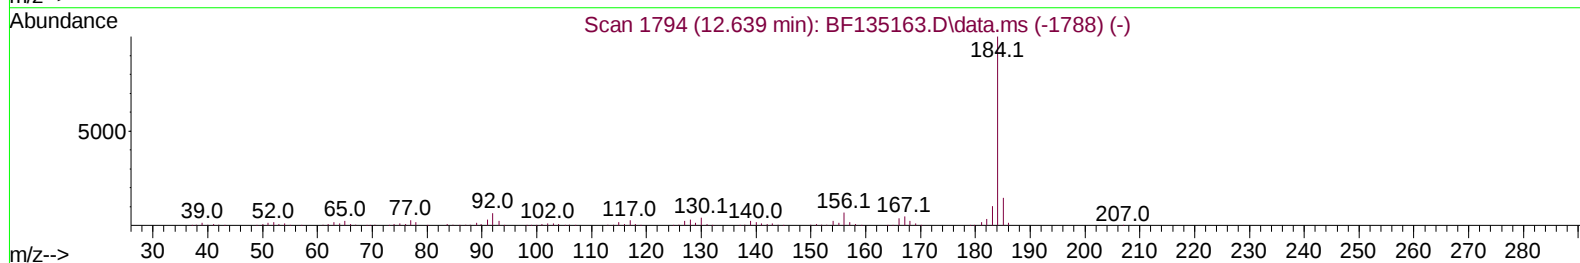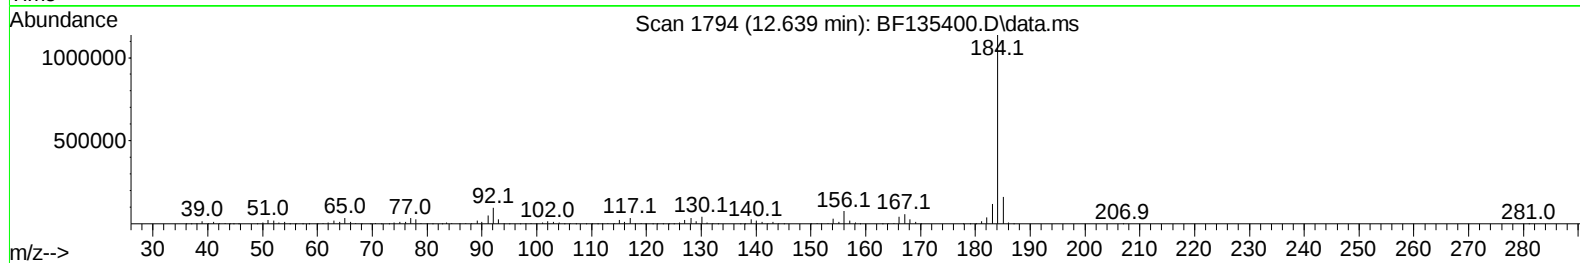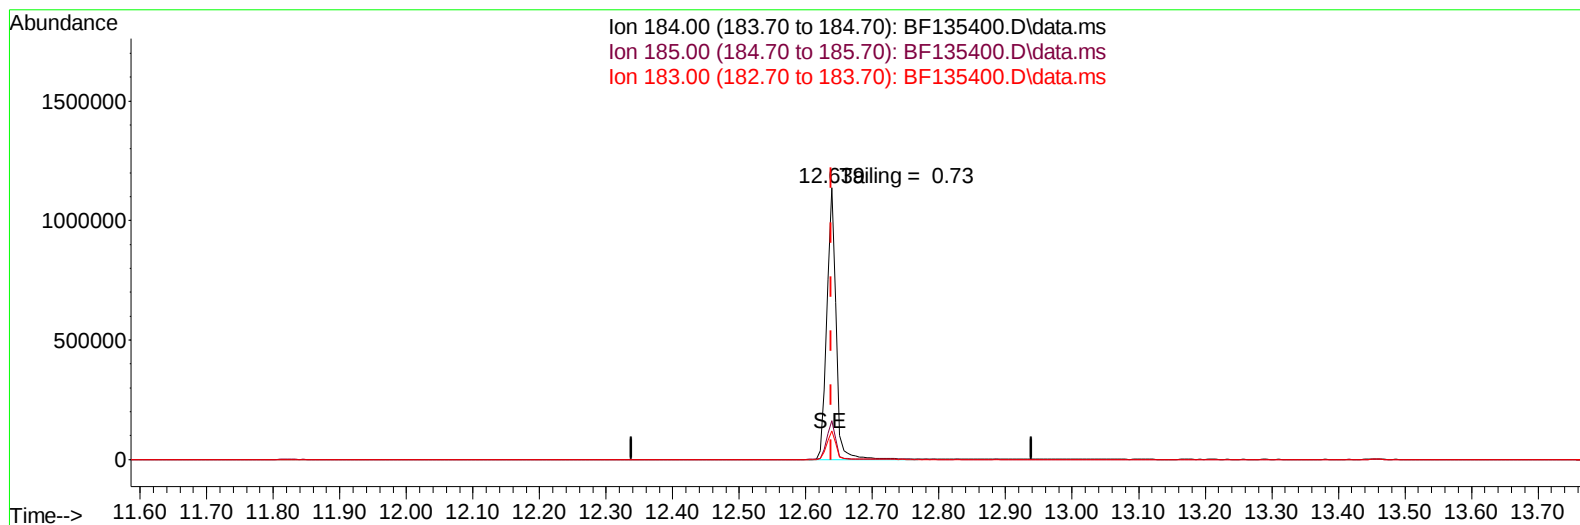

TIC: BF135400.D\data.ms

(77) Benzidine

12.639min (+ 0.000) 621392.11 ng

response 1107541

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.33
183.00	10.30	10.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/22/2023	BNA_F	<u>BF135400.D</u>
Compound Name	Response	Retention Time
DDT	422617	13.457
DDD	12233	13.157
DDE	950	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13183	435800	3.03

Instrument :
BNA_F
ClientSampleId :
DFTPP