
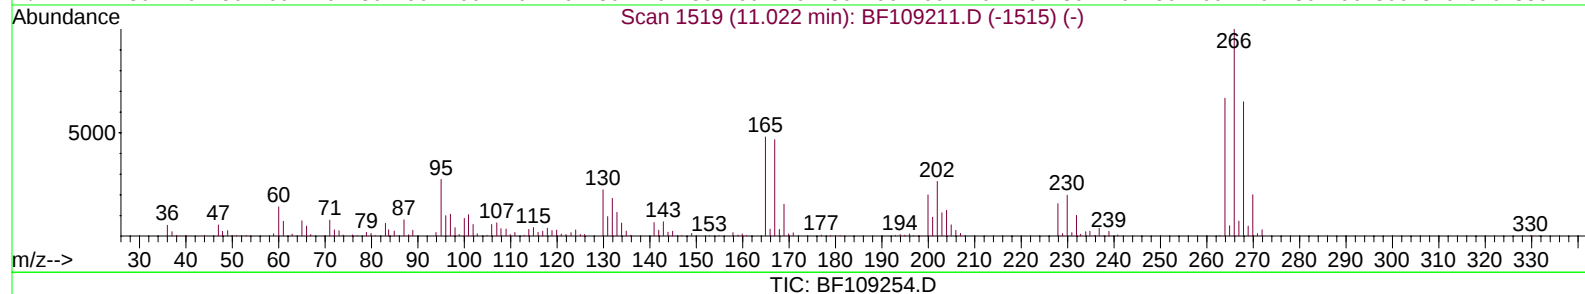
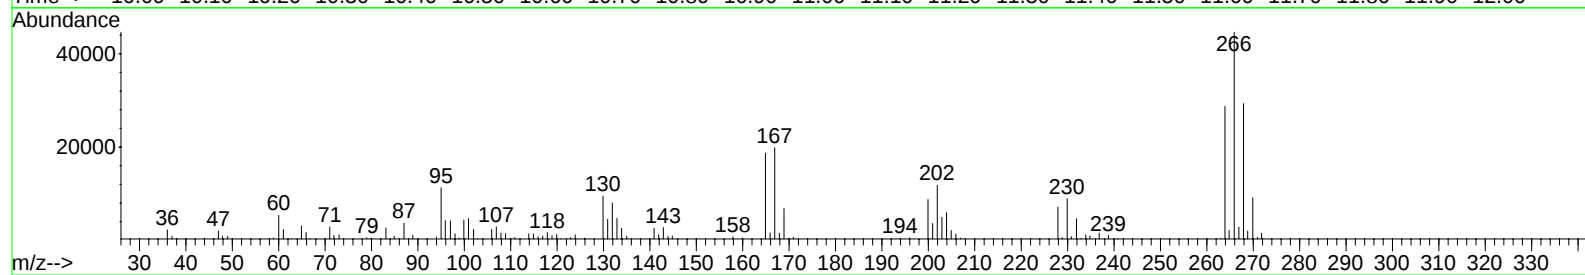


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092418\  
Data File   : BF109254.D  
Acq On      : 24 Sep 2018    9:22  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Sep 24 19:28:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

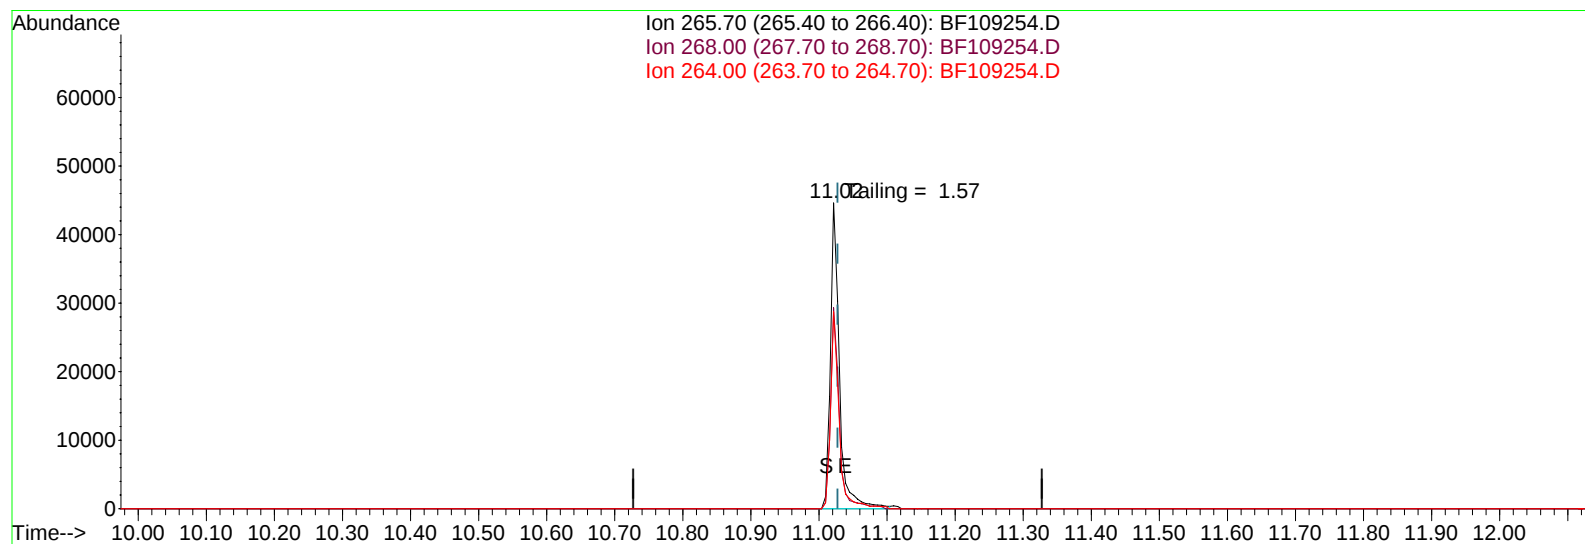

(69) Pentachlorophenol (C)




11.022min (-0.006) 0.00ng

response 41334

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.72
264.00	61.90	64.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092418\
Data File : BF109254.D
Acq On : 24 Sep 2018 9:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:28:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

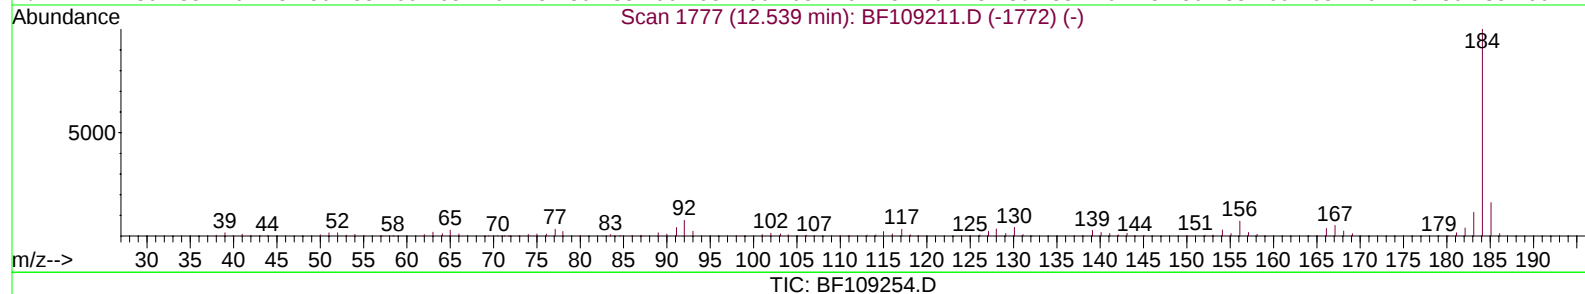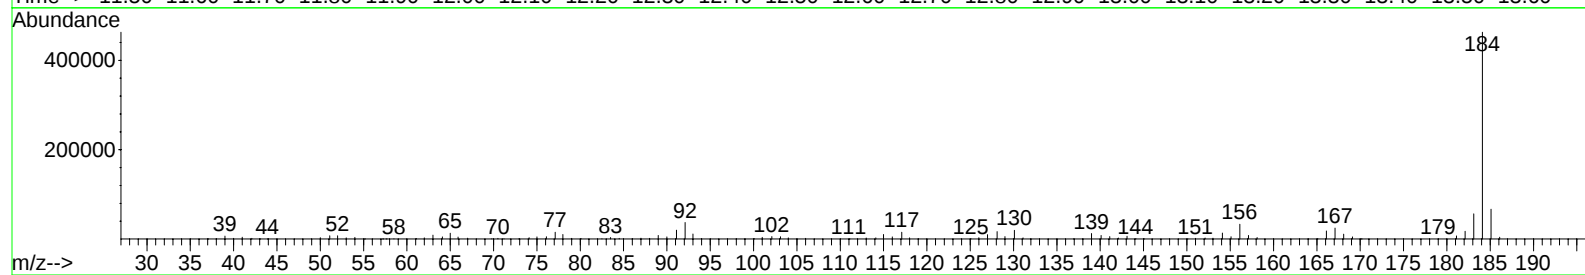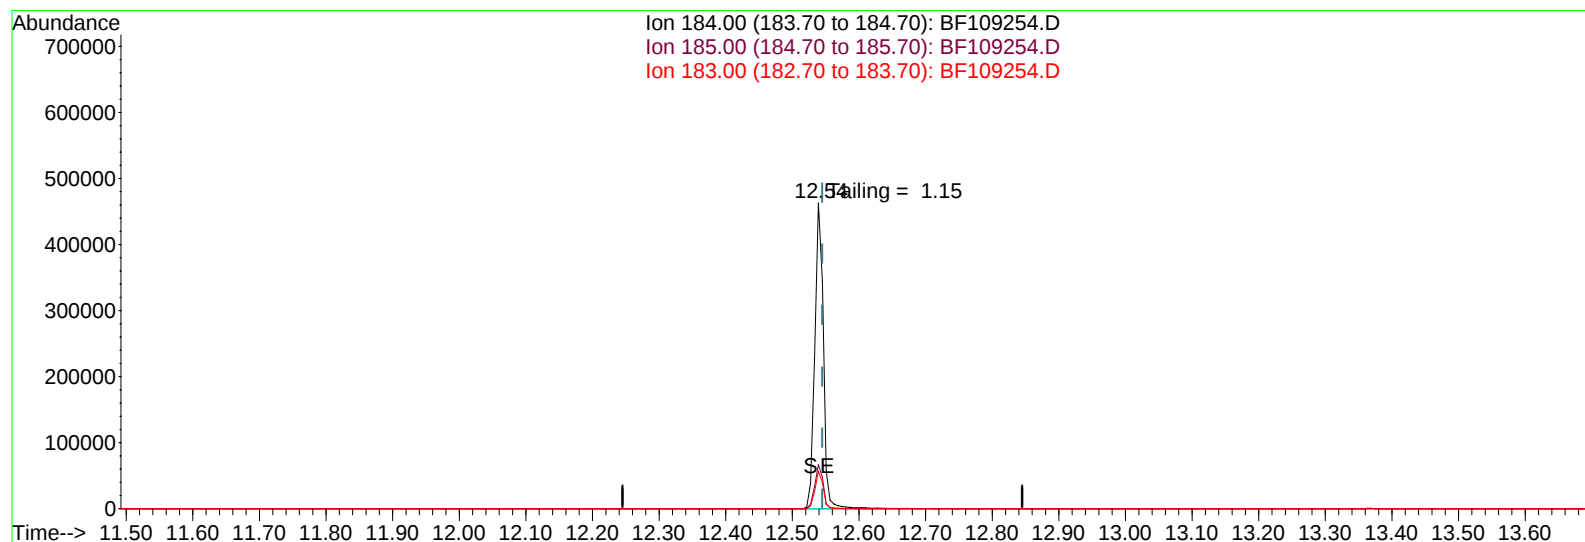

(76) Benzidine

12.539min (-0.006) 0.00ng

response 416577

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.46
183.00	11.60	12.25
0.00	0.00	0.00