

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092418\
 Data File : BF109278.D
 Acq On : 24 Sep 2018 19:55
 Operator : JU/SJ
 Sample : J4770-19 2X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 JC-02-092118-J

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.887	473	476	485	rVB	22772	24837	3.33%	0.268%
2	5.310	545	548	560	rBV	716258	687849	92.14%	7.435%
3	6.339	720	723	735	rBV	826095	722349	96.76%	7.808%
4	6.475	742	746	750	rBV	893005	727833	97.49%	7.867%
5	6.710	782	786	790	rBV	755204	575930	77.15%	6.225%
6	6.863	809	812	816	rBV	654900	529997	70.99%	5.729%
7	7.263	877	880	884	rBV	468485	406891	54.50%	4.398%
8	7.992	1000	1004	1007	rBV	902054	697380	93.41%	7.538%
9	9.063	1183	1186	1190	rBV	833676	682930	91.48%	7.382%
10	9.457	1250	1253	1257	rBV	211900	158698	21.26%	1.715%
11	9.739	1298	1301	1305	rBV2	853249	724794	97.09%	7.834%
12	10.522	1431	1434	1439	rBV	513725	438005	58.67%	4.734%
13	10.669	1454	1459	1465	rVB8	12322	21257	2.85%	0.230%
14	11.133	1536	1538	1543	rVB2	15121	12380	1.66%	0.134%
15	11.216	1549	1552	1555	rBV	800512	746555	100.00%	8.070%
16	11.239	1555	1556	1559	rVB	26656	18225	2.44%	0.197%
17	11.621	1619	1621	1624	rVB	20804	18374	2.46%	0.199%
18	11.757	1641	1644	1648	rBV3	31517	33441	4.48%	0.361%
19	11.827	1654	1656	1659	rBV4	10992	10475	1.40%	0.113%
20	12.269	1729	1731	1733	rBV2	12019	11559	1.55%	0.125%
21	12.304	1734	1737	1739	rVV	72023	62292	8.34%	0.673%
22	12.327	1739	1741	1743	rVB	62797	45528	6.10%	0.492%
23	12.421	1754	1757	1761	rBV	67336	60752	8.14%	0.657%
24	12.651	1793	1796	1799	rBV	57758	51169	6.85%	0.553%
25	12.798	1817	1821	1824	rBV	887387	716301	95.95%	7.743%
26	12.833	1825	1827	1830	rVB	40440	33535	4.49%	0.362%
27	13.845	1995	1999	2002	rBV	733870	654221	87.63%	7.072%
28	15.251	2235	2238	2241	rVB	367479	377888	50.62%	4.085%


Sum of corrected areas: 9251445

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092418\
Data File : BF109278.D
Acq On : 24 Sep 2018 19:55
Operator : JU/SJ
Sample : J4770-19 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-02-092118-J

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

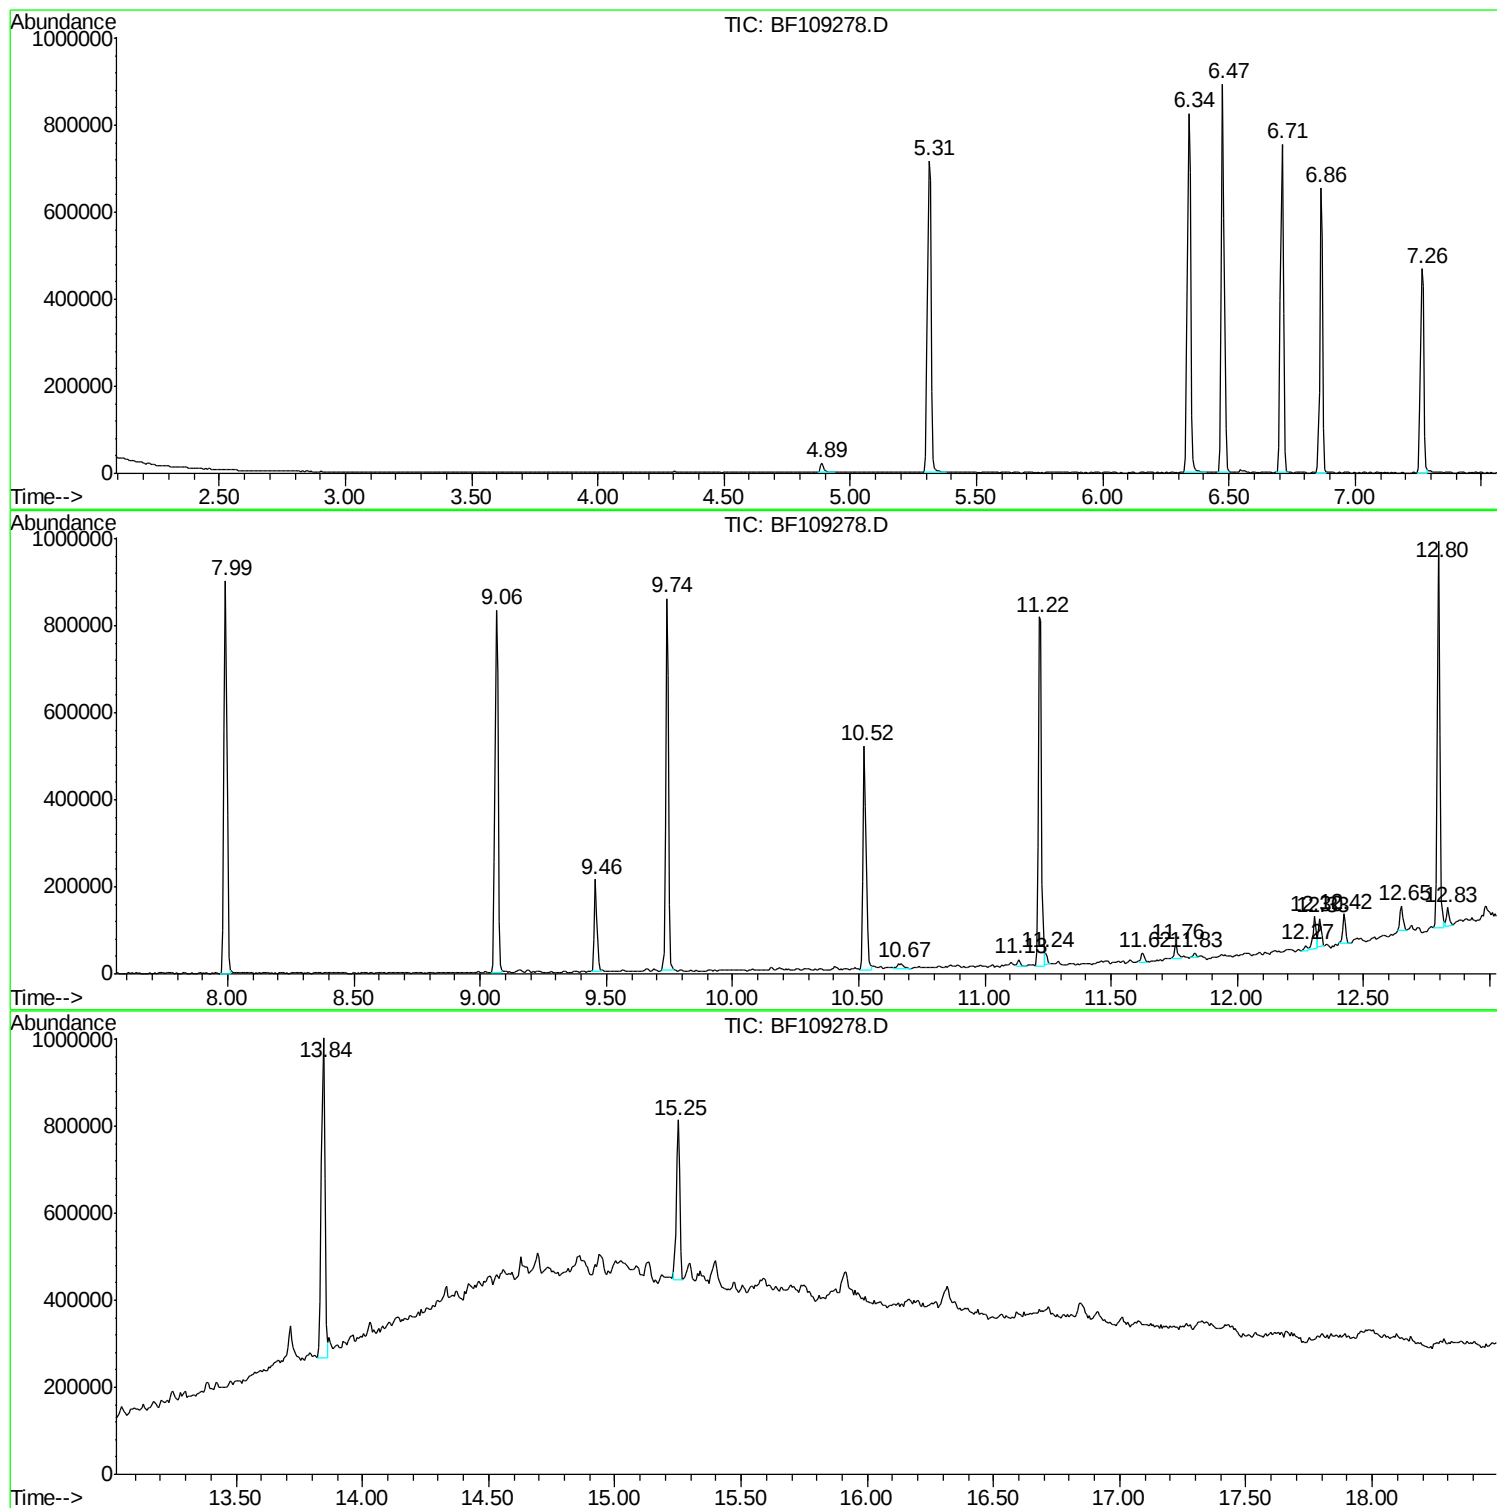

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092418\
Data File : BF109278.D
Acq On : 24 Sep 2018 19:55
Operator : JU/SJ
Sample : J4770-19 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-02-092118-J










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	25.28 ng	727833	1,4-Dichlorobenzene-d4	6.71

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

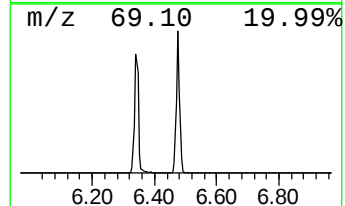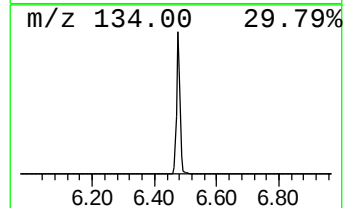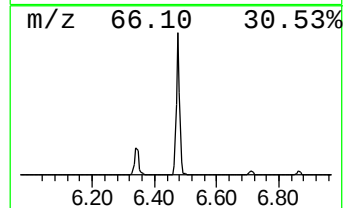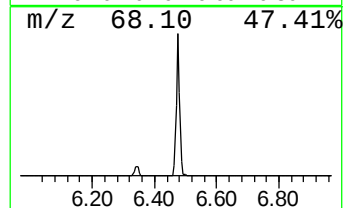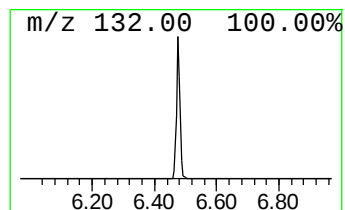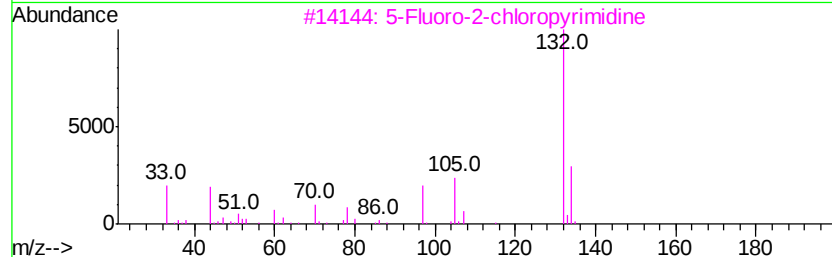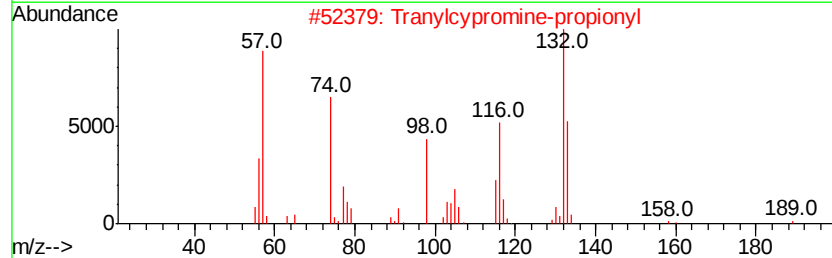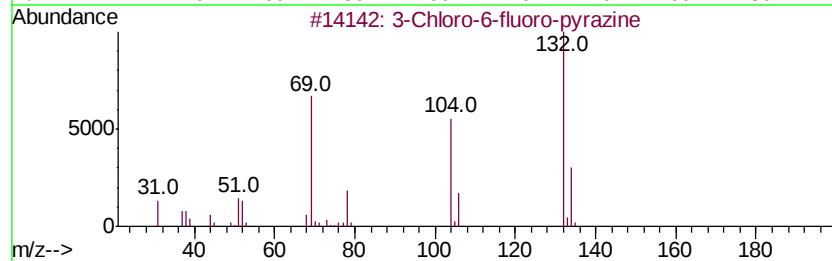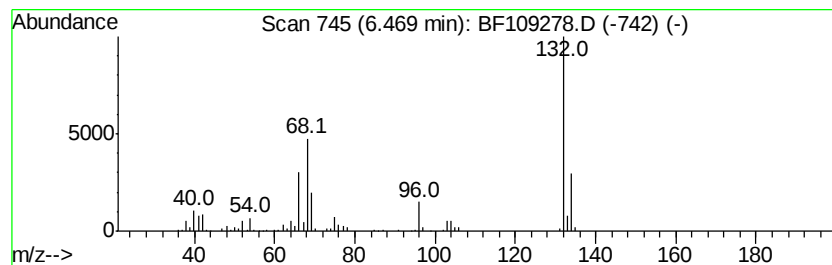

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092418\
Data File : BF109278.D
Acq On : 24 Sep 2018 19:55
Operator : JU/SJ
Sample : J4770-19 2X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
JC-02-092118-J

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.47	6.47	25.3	ng	727833	1	6.71	575930	20.0