


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092418\
Data File : BF109254.D
Acq On : 24 Sep 2018 9:22
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 22 13:32:18 2018

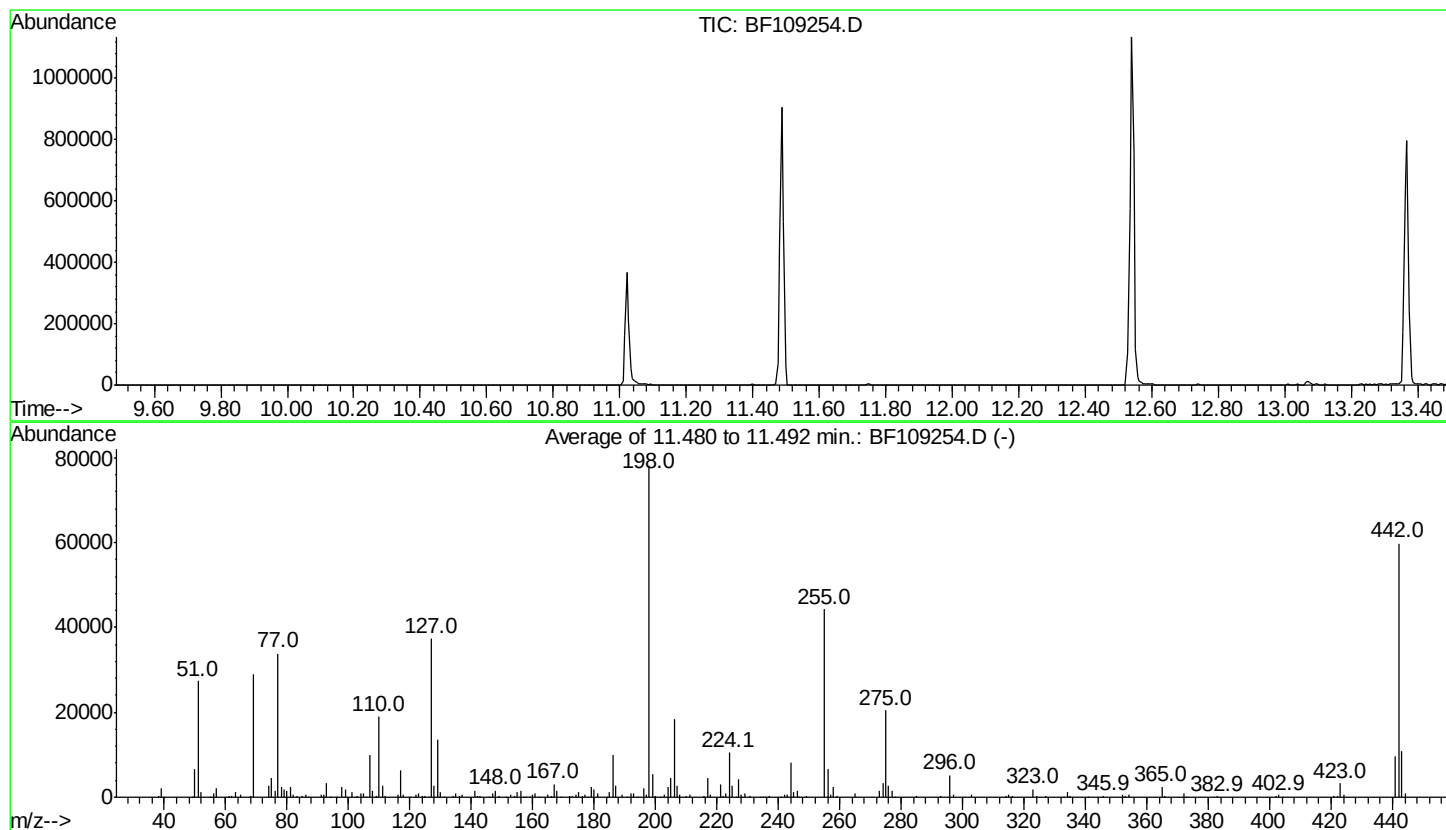

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	27301	PASS
68	69	0.00	2	1.4	409	PASS
69	198	0.00	100	37.2	29090	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	37354	PASS
197	198	0.00	2	0.8	587	PASS
198	198	100	100	100.0	78109	PASS
199	198	5	9	7.1	5508	PASS
275	198	10	60	26.1	20412	PASS
365	198	1	100	3.1	2458	PASS
441	198	0.01	100	12.2	9514	PASS
442	198	50	100	76.5	59776	PASS
443	442	15	24	18.2	10908	PASS