

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092419\  
 Data File : BF117224.D  
 Acq On : 24 Sep 2019 19:14  
 Operator : JU  
 Sample : K5008-07  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :

Quant Time: Sep 25 02:38:56 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Sep 13 16:23:17 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 6.81  | 152  | 25444    | 20.00 | ng    | -0.01    |
| 21) Naphthalene-d8        | 8.09  | 136  | 102866   | 20.00 | ng    | -0.01    |
| 39) Acenaphthene-d10      | 9.85  | 164  | 56893    | 20.00 | ng    | -0.01    |
| 64) Phenanthrene-d10      | 11.33 | 188  | 89909    | 20.00 | ng    | 0.00     |
| 76) Chrysene-d12          | 13.97 | 240  | 64383    | 20.00 | ng    | 0.00     |
| 87) Perylene-d12          | 15.43 | 264  | 70262    | 20.00 | ng    | 0.00     |

| System Monitoring Compounds | R.T.  | QIon | Response | Conc   | Units | Dev(Min) |
|-----------------------------|-------|------|----------|--------|-------|----------|
| 5) 2-Fluorophenol           | 5.43  | 112  | 157403   | 96.58  | ng    | 0.00     |
| 7) Phenol-d6                | 6.45  | 99   | 217180   | 103.12 | ng    | 0.00     |
| 23) Nitrobenzene-d5         | 7.37  | 82   | 135555   | 69.24  | ng    | -0.01    |
| 42) 2,4,6-Tribromophenol    | 10.64 | 330  | 48069    | 101.09 | ng    | 0.00     |
| 45) 2-Fluorobiphenyl        | 9.17  | 172  | 240146   | 66.00  | ng    | 0.00     |
| 79) Terphenyl-d14           | 12.92 | 244  | 222576   | 64.62  | ng    | 0.00     |


| Target Compounds               | R.T.  | QIon | Response | Conc      | Units | Qvalue |
|--------------------------------|-------|------|----------|-----------|-------|--------|
| 9) Benzaldehyde                | 6.59  | 77   | 4328     | Below Cal |       | # 72   |
| 10) Phenol                     | 6.46  | 94   | 6928     | 2.984     | ng    | # 80   |
| 19) n-Nitroso-di-n-propylamine | 7.37  | 70   | 17492    | 13.639    | ng    | # 82   |
| 25) Isophorone                 | 7.37  | 82   | 135554   | 39.105    | ng    | # 66   |
| 50) Dimethylphthalate          | 9.56  | 163  | 37203    | 9.235     | ng    | # 99   |
| 57) 2,4-Dinitrotoluene         | 9.85  | 165  | 7213     | 6.773     | ng    | # 18   |
| 67) 4-Bromophenyl-phenylether  | 10.63 | 248  | 3413     | 3.717     | ng    | # 1    |
| 75) Fluoranthene               | 12.54 | 202  | 16156    | 3.079     | ng    | 99     |
| 78) Pyrene                     | 12.77 | 202  | 17259    | 3.195     | ng    | 98     |
| 81) Benzo(a)anthracene         | 13.96 | 228  | 15961    | 3.711     | ng    | # 91   |
| 83) Chrysene                   | 14.00 | 228  | 15894    | 3.788     | ng    | 95     |
| 86) Indeno(1,2,3-cd)pyrene     | 16.87 | 276  | 13671    | 4.467     | ng    | 96     |
| 88) Benzo(b)fluoranthene       | 15.01 | 252  | 37053    | 8.706     | ng    | 98     |
| 89) Benzo(k)fluoranthene       | 15.01 | 252  | 37053    | 9.191     | ng    | 98     |
| 90) Benzo(a)pyrene             | 15.37 | 252  | 19292    | 5.166     | ng    | 94     |
| 92) Benzo(g,h,i)perylene       | 17.31 | 276  | 11939    | 4.027     | ng    | 97     |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092419\  
Data File : BF117224.D  
Acq On : 24 Sep 2019 19:14  
Operator : JU  
Sample : K5008-07  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :

Quant Time: Sep 25 02:38:56 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 13 16:23:17 2019  
Response via : Initial Calibration

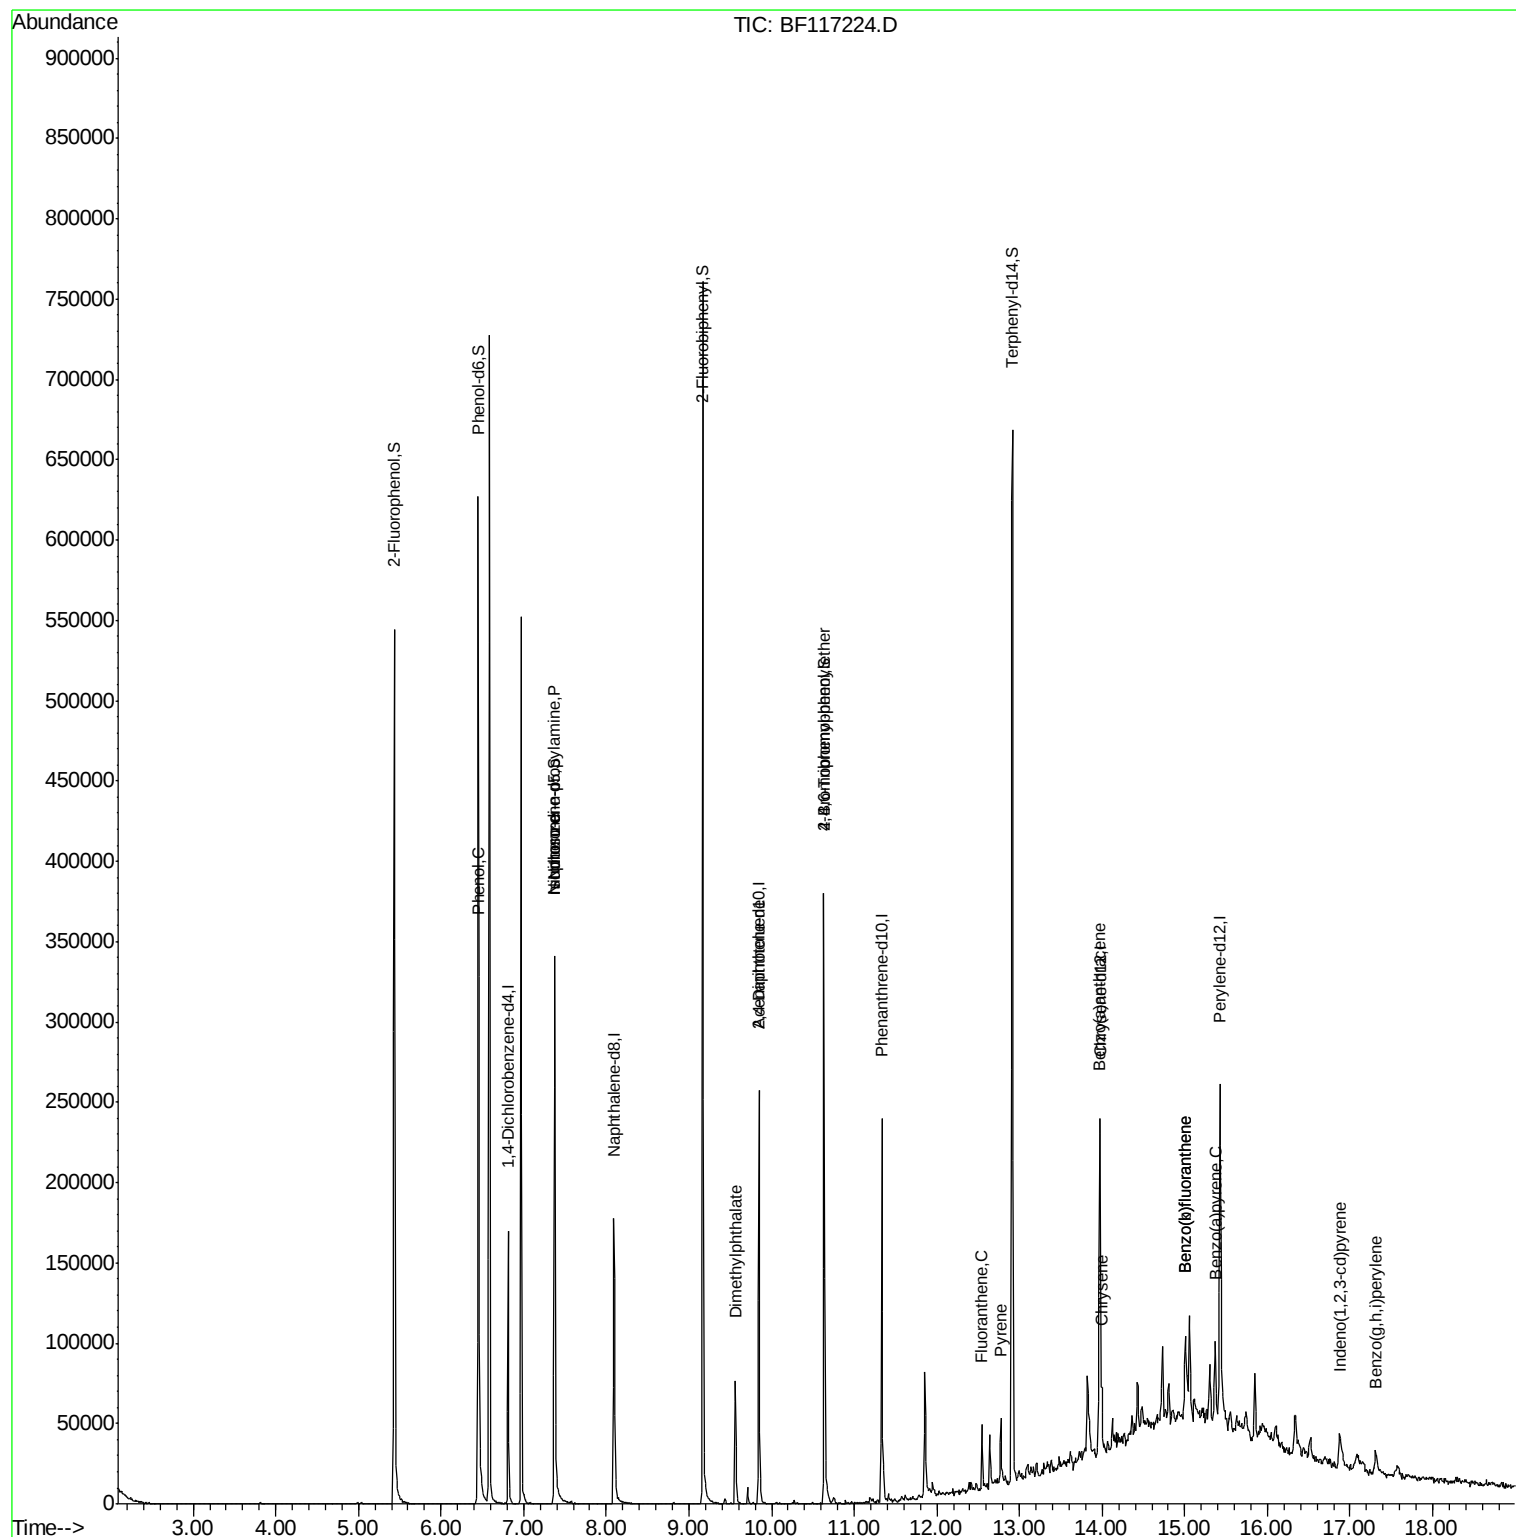




#1



1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 6.81 min Scan# 803  
Delta R.T. -0.01 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Instrument :  
BNA\_F  
ClientSampleId :

Tot Ion:152 Resp: 25444  
Ion Ratio Lower Upper  
152 100  
150 163.8 127.5 191.3  
115 74.4 55.0 82.4

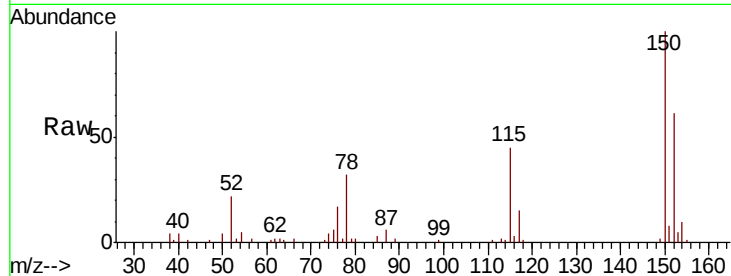


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

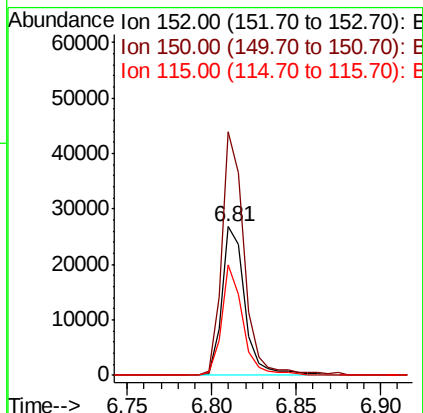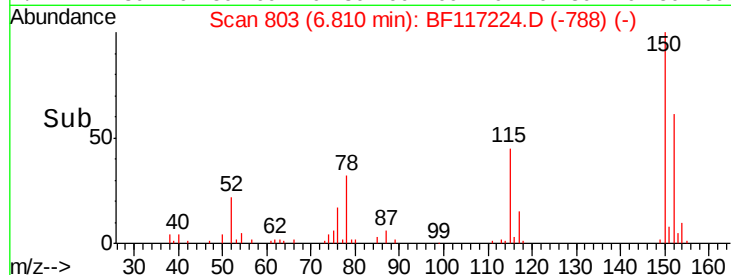



#5

2-Fluorophenol  
Concen: 96.583 ng  
RT: 5.43 min Scan# 569  
Delta R.T. -0.01 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Tgt Ion:112 Resp: 157403  
Ion Ratio Lower Upper  
112 100  
64 56.1 45.7 68.5  
63 31.7 24.9 37.3

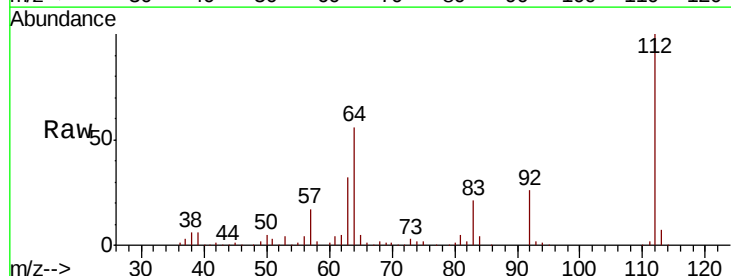

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BF1  
Ion 63.00 (62.70 to 63.70): BF1

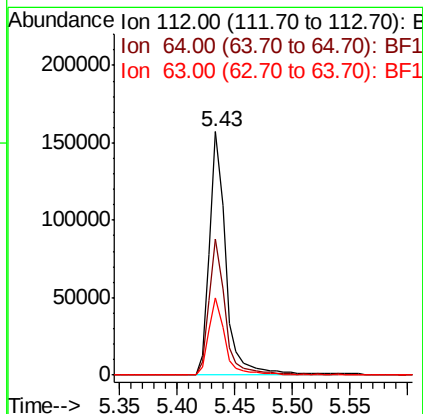



#7

Phenol-d6

Concen: 103.115 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Instrument :

BNA\_F

ClientSampled :


Tot Ion: 99 Resp: 217180

Ion Ratio Lower Upper




99 100

42 16.7 12.2 18.2

71 40.3 29.8 44.8

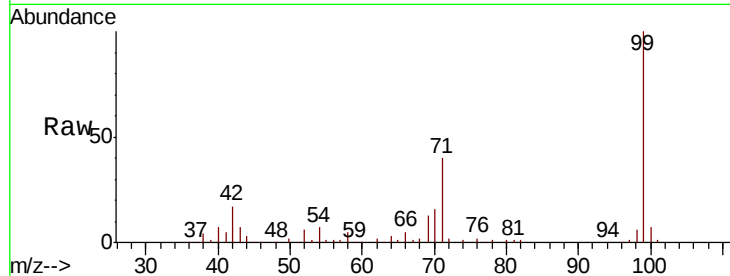

Abundance Ion 99.00 (98.70 to 99.70): BF1  
Ion 42.00 (41.70 to 42.70): BF1  
Ion 71.00 (70.70 to 71.70): BF1

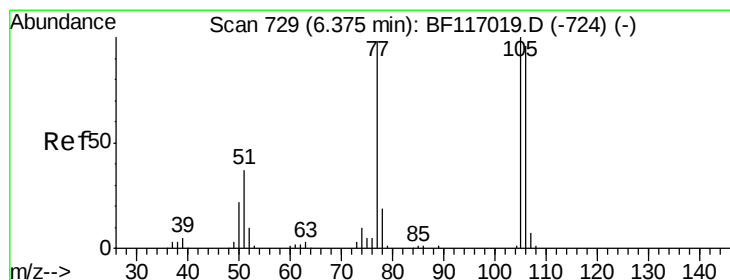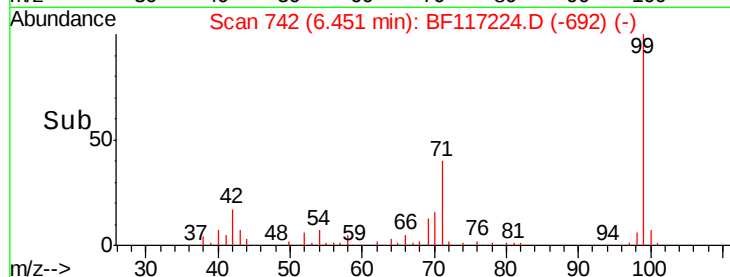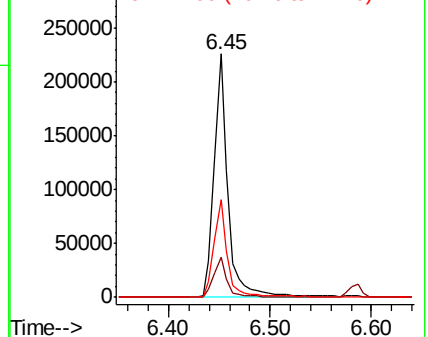

#9

Benzaldehyde

Concen: Below Cal

RT: 6.59 min Scan# 765

Delta R.T. 0.21 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14


Tgt Ion: 77 Resp: 4328

Ion Ratio Lower Upper



77 100


105 81.6 81.8 121.8#

106 61.9 77.3 117.3#

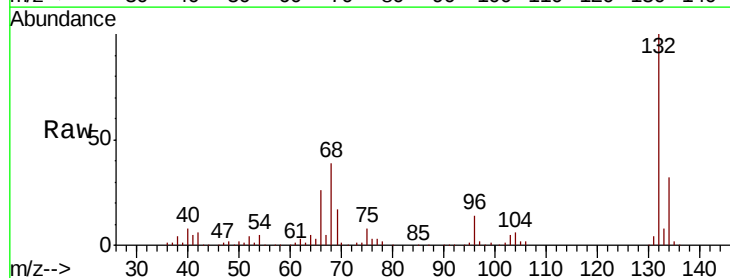

Abundance Ion 77.00 (76.70 to 77.70): BF1  
Ion 105.00 (104.70 to 105.70): E  
Ion 106.00 (105.70 to 106.70): E

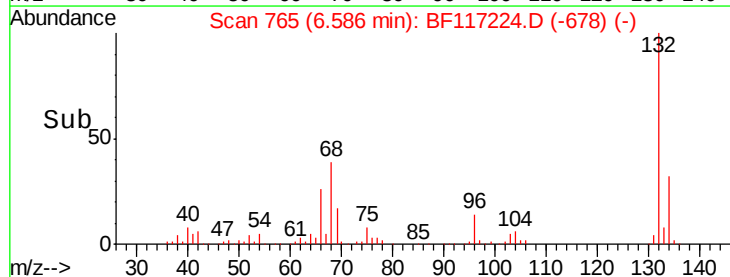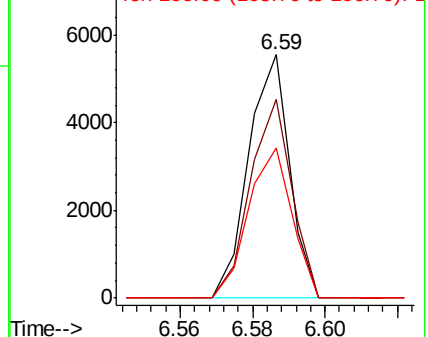

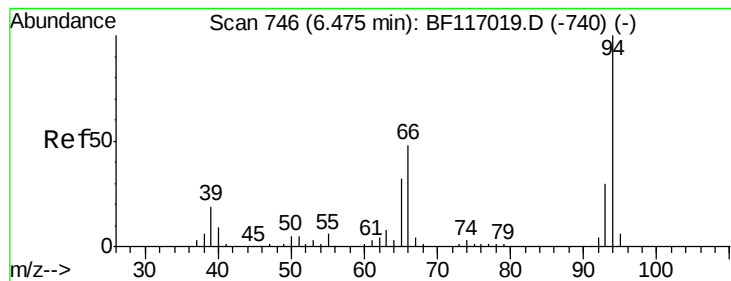

#10

Phenol

Concen: 2.984 ng

RT: 6.46 min Scan# 744

Delta R.T. -0.01 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Instrument :

BNA\_F

ClientSampleId :





Tot Ion: 94 Resp: 6928

Ion Ratio Lower Upper

94 100

65 35.2 12.5 52.5

66 69.4 28.9 68.9#

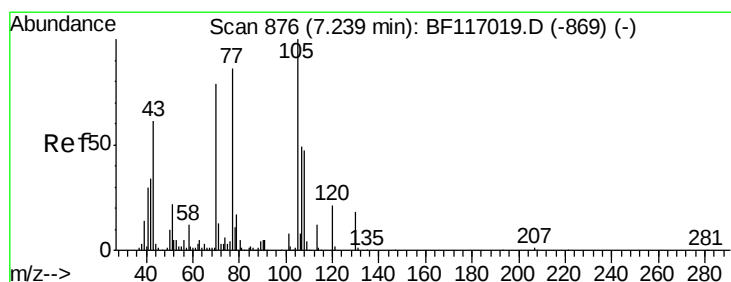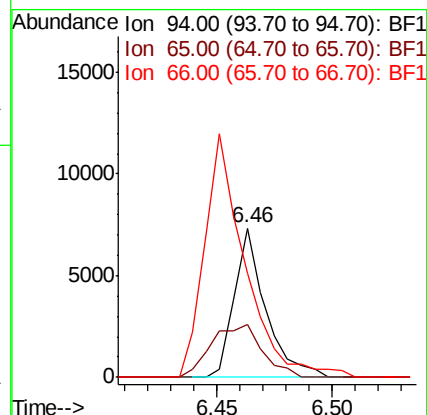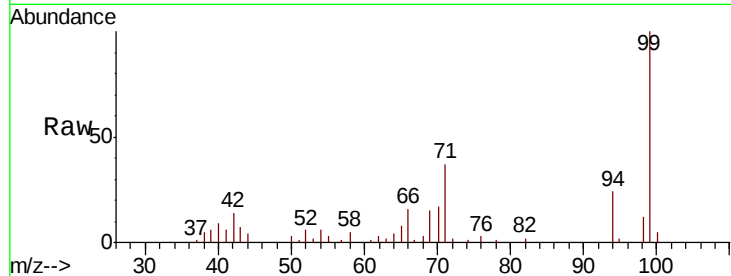

#19

n-Nitroso-di-n-propylamine

Concen: 13.639 ng

RT: 7.37 min Scan# 899

Delta R.T. 0.14 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Tgt Ion: 70 Resp: 17492




Ion Ratio Lower Upper


70 100

42 41.8 34.0 51.0

101 0.0 7.8 11.6#

130 0.0 17.8 26.8#

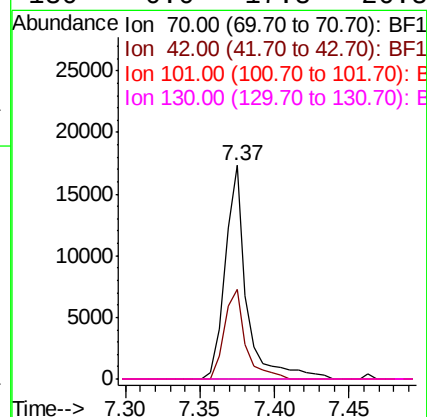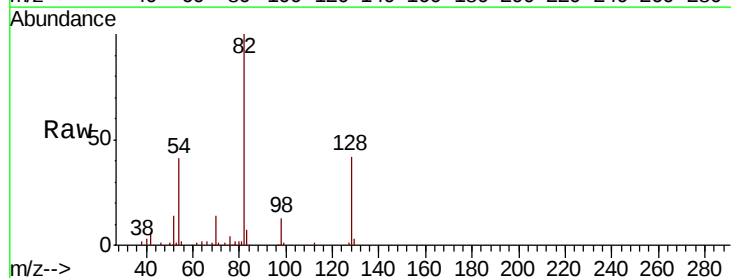

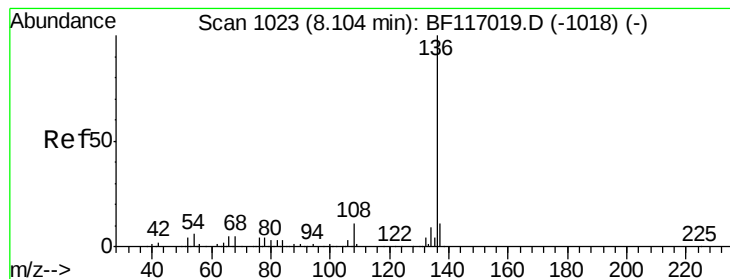

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1021

Delta R.T. -0.01 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Instrument :

BNA\_F

ClientSampleId :

Tot Ion:136 Resp: 102866


Ion Ratio Lower Upper

136 100

137 13.0 9.0 13.4

54 6.5 4.5 6.7

68 4.5 4.0 6.0



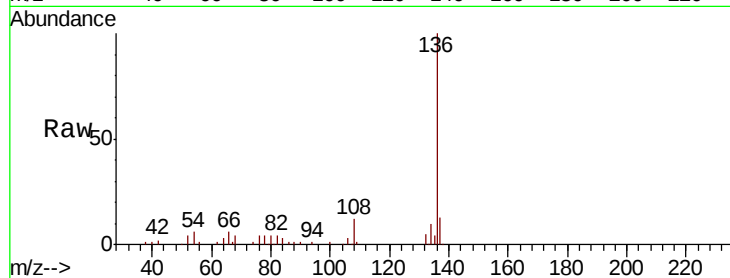


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

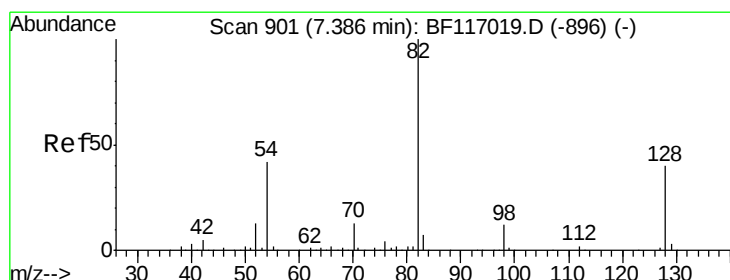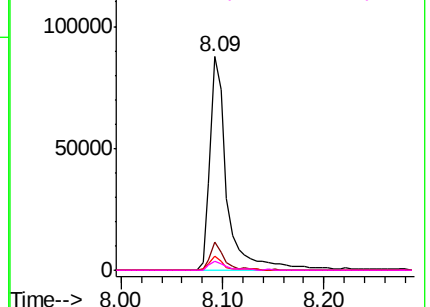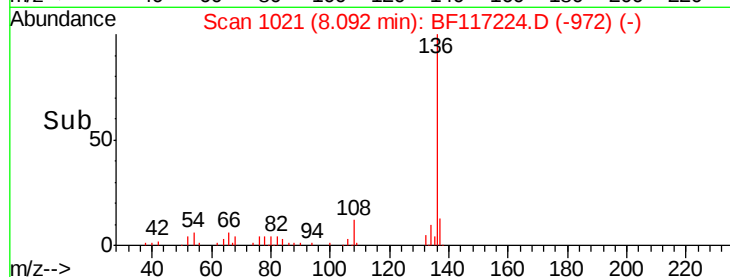

#23

Nitrobenzene-d5

Concen: 69.239 ng

RT: 7.37 min Scan# 899

Delta R.T. -0.01 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14


Tgt Ion: 82 Resp: 135555

Ion Ratio Lower Upper

82 100

128 41.9 32.3 48.5



54 40.6 33.3 49.9

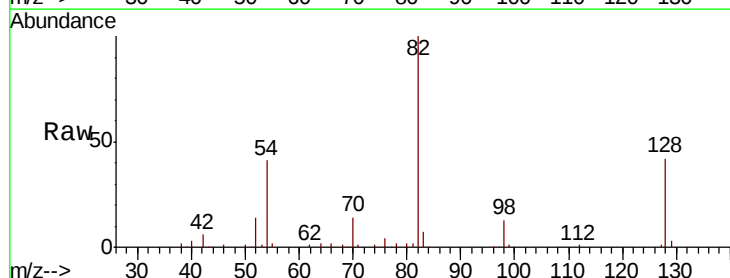


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

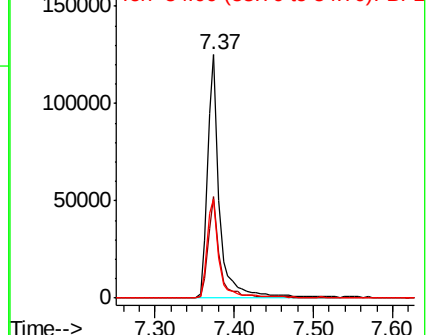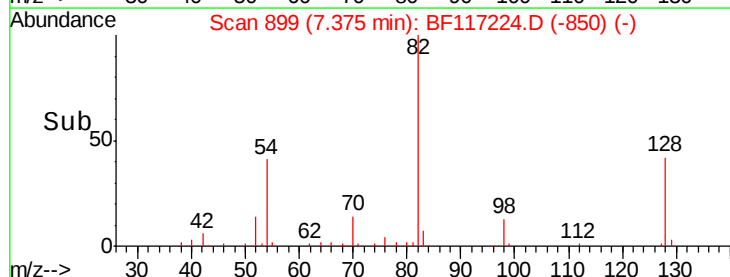

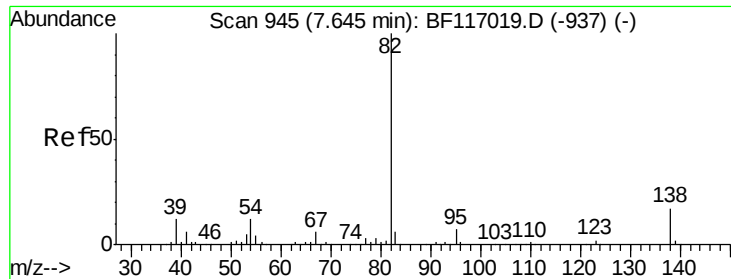

#25

Isophorone

Concen: 39.105 ng

RT: 7.37 min Scan# 899

Delta R.T. -0.27 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Instrument :

BNA\_F

ClientSampleId :


Tot Ion: 82 Resp: 135554

Ion Ratio Lower Upper

82 100

95 0.0 5.8 8.6#




138 0.0 13.5 20.3#

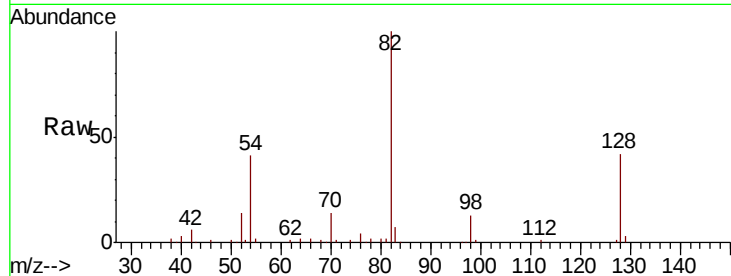

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

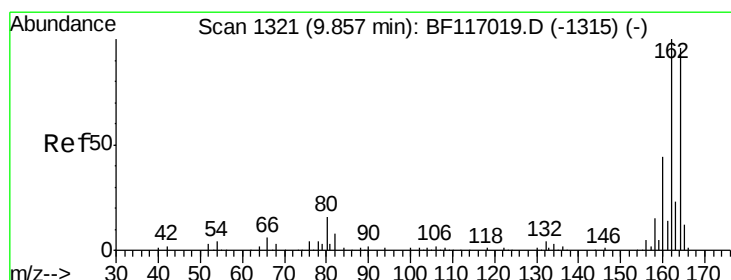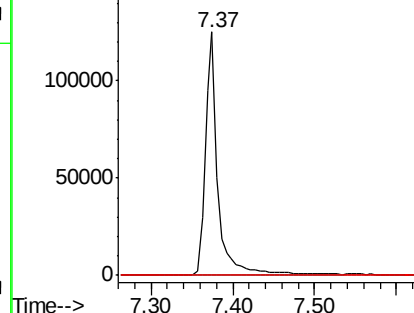

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.85 min Scan# 1319

Delta R.T. -0.01 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14


Tgt Ion: 164 Resp: 56893

Ion Ratio Lower Upper

164 100

162 103.0 83.4 125.2



160 45.2 36.4 54.6

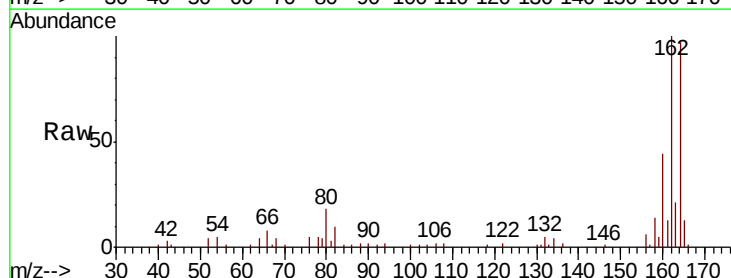

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

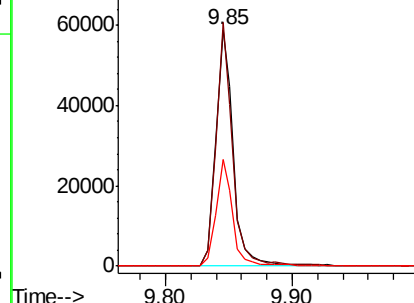




#42  
 2,4,6-Tribromophenol  
 Concen: 101.093 ng  
 RT: 10.64 min Scan# 1454  
 Delta R.T. -0.01 min  
 Lab File: BF117224.D  
 Acq: 24 Sep 2019 19:14

Instrument :  
 BNA\_F  
 ClientSampled :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 330     | 100   |       |       |
| 332     | 96.5  | 78.0  | 117.0 |
| 141     | 45.6  | 35.8  | 53.6  |



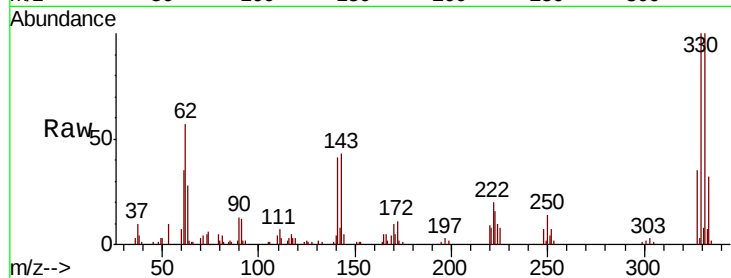


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

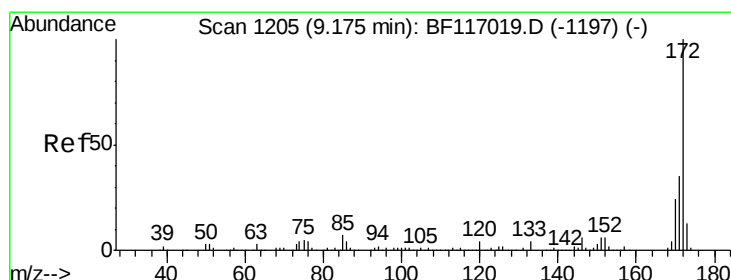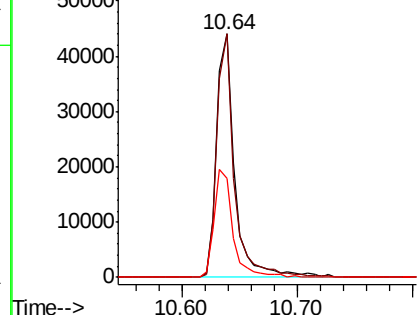

#45  
 2-Fluorobiphenyl  
 Concen: 65.999 ng  
 RT: 9.17 min Scan# 1204  
 Delta R.T. -0.01 min  
 Lab File: BF117224.D  
 Acq: 24 Sep 2019 19:14

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 172     | 100   |       |       |
| 171     | 34.6  | 28.2  | 42.2  |
| 170     | 22.5  | 18.9  | 28.3  |


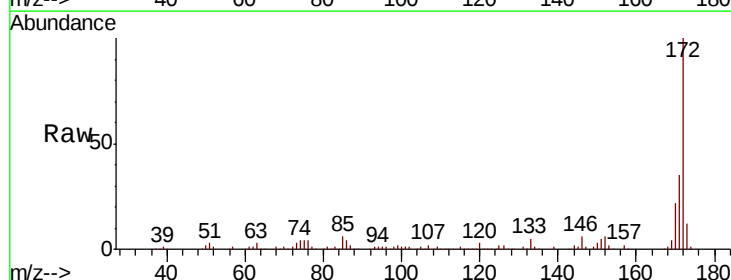



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

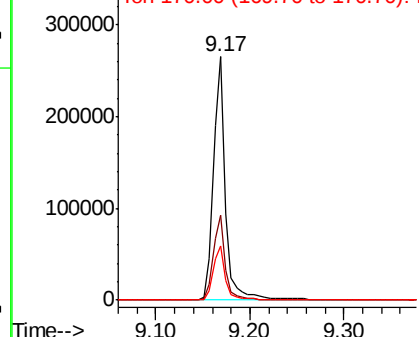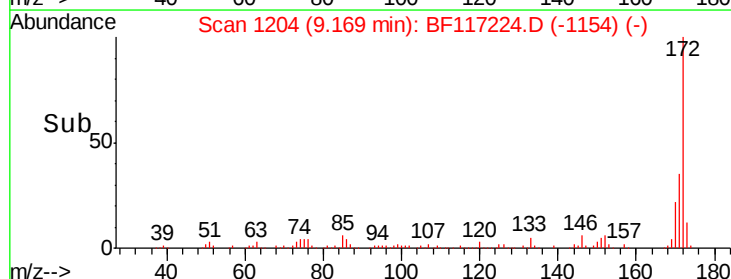


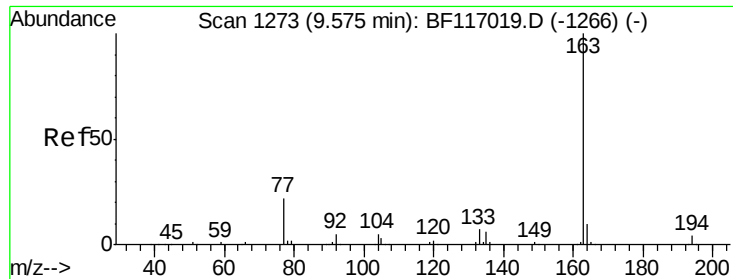



#50  
Dimethylphthalate  
Concen: 9.235 ng  
RT: 9.56 min Scan# 1271  
Delta R.T. -0.01 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Instrument :  
BNA\_F  
ClientSampled :

Tot Ion:163 Resp: 37203  
Ion Ratio Lower Upper  
163 100  
194 4.5 2.9 4.3#  
164 10.5 8.2 12.4

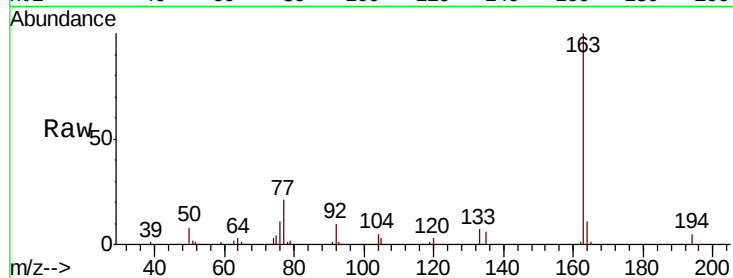


Abundance Ion 163.00 (162.70 to 163.70): E  
Ion 194.00 (193.70 to 194.70): E  
Ion 164.00 (163.70 to 164.70): E

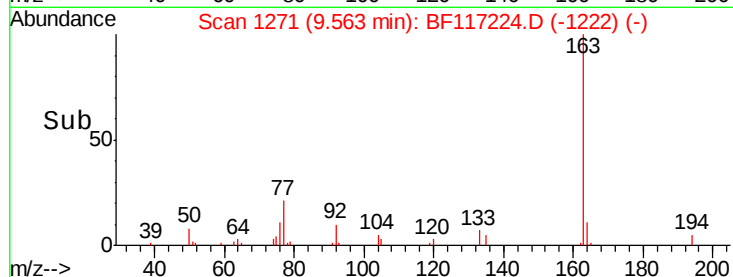
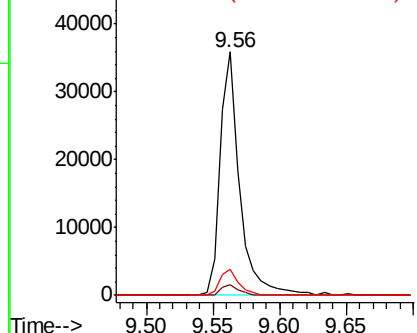


#57  
2,4-Dinitrotoluene  
Concen: 6.773 ng  
RT: 9.85 min Scan# 1319  
Delta R.T. -0.20 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Tgt Ion:165 Resp: 7213  
Ion Ratio Lower Upper  
165 100  
63 0.0 35.0 52.4#  
89 0.0 66.1 99.1#  
182 0.0 2.0 3.0#

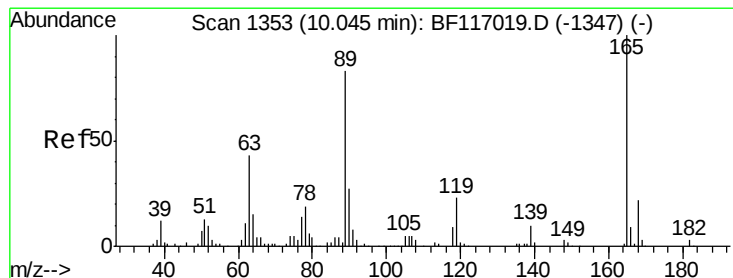

Abundance Ion 165.00 (164.70 to 165.70): E  
Ion 63.00 (62.70 to 63.70): BF1  
Ion 89.00 (88.70 to 89.70): BF1  
Ion 182.00 (181.70 to 182.70): E

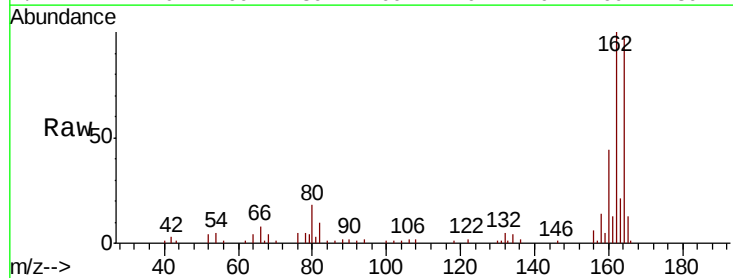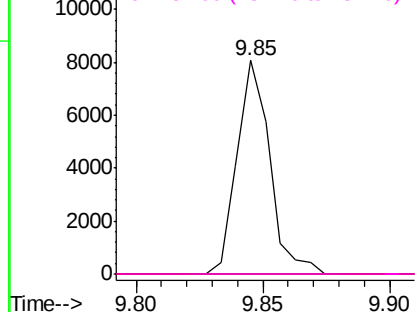



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1572

Delta R.T. -0.00 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Instrument :

BNA\_F

ClientSampleId :


Tot Ion:188 Resp: 89909

Ion Ratio Lower Upper

188 100

94 8.9 8.2 12.2




80 8.7 9.0 13.6#

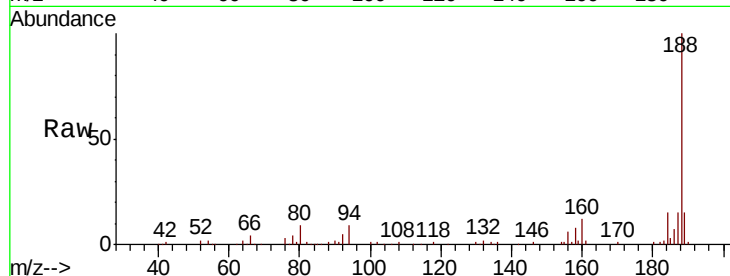

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

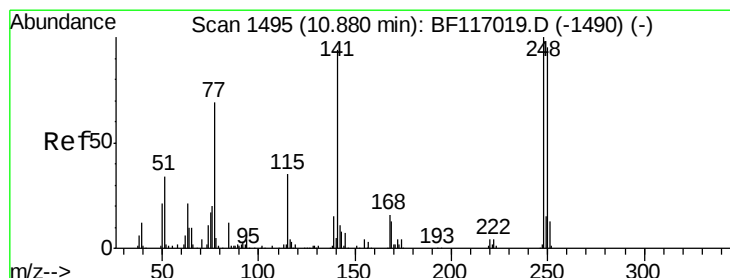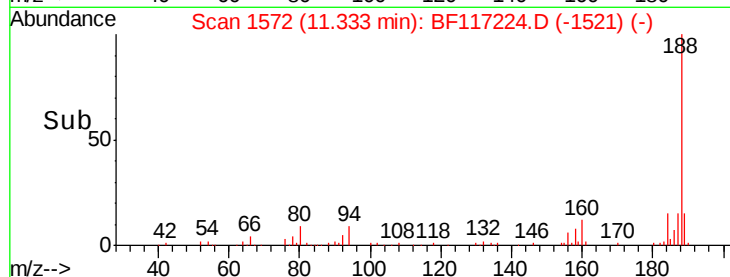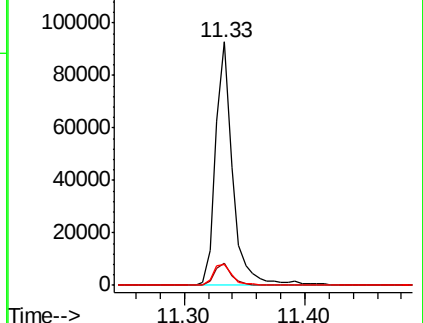

#67

4-Bromophenyl-phenylether

Concen: 3.717 ng

RT: 10.63 min Scan# 1453

Delta R.T. -0.25 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14


Tgt Ion:248 Resp: 3413

Ion Ratio Lower Upper

248 100

250 151.8 76.2 114.4#



141 576.0 75.0 112.4#

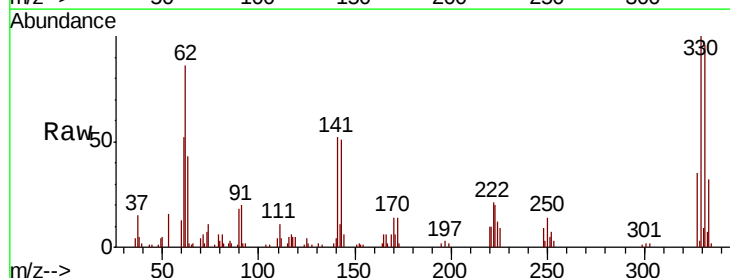


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

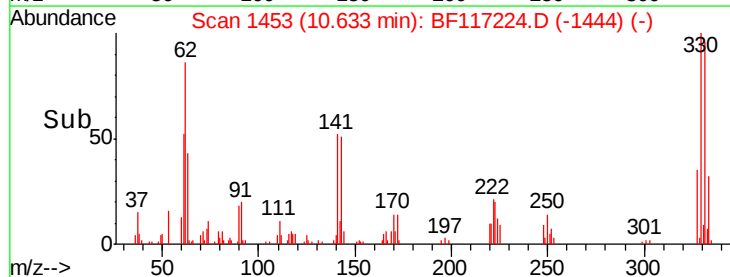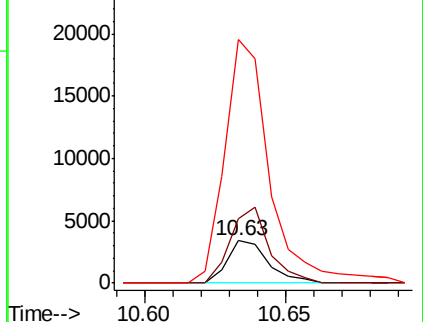


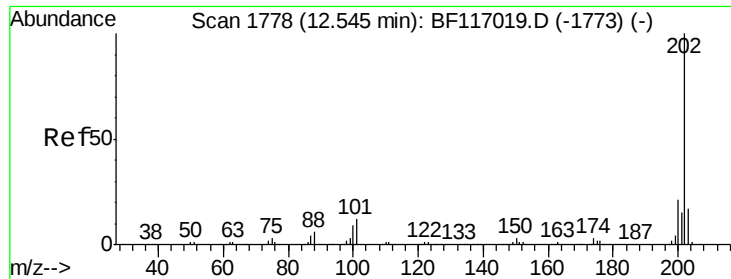




#75  
 Fluoranthene  
 Concen: 3.079 ng  
 RT: 12.54 min Scan# 1778  
 Delta R.T. -0.00 min  
 Lab File: BF117224.D  
 Acq: 24 Sep 2019 19:14

Instrument :  
 BNA\_F  
 ClientSampleId :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 101     | 12.6  | 0.0   | 32.3  |
| 203     | 17.4  | 0.0   | 37.1  |

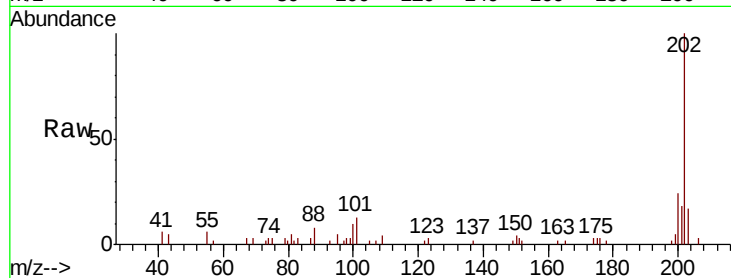


Abundance Ion 202.00 (201.70 to 202.70): E  
 Ion 101.00 (100.70 to 101.70): E  
 Ion 203.00 (202.70 to 203.70): E

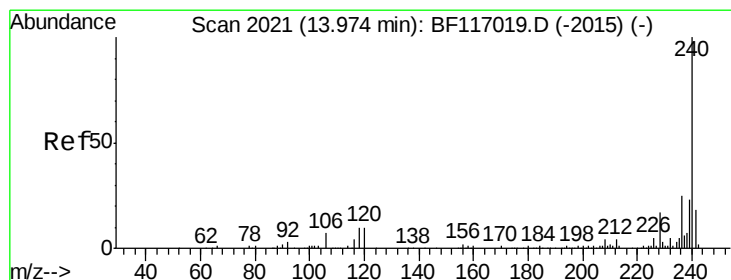
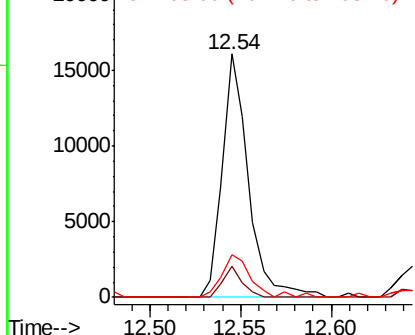



#76  
 Chrysene-d12  
 Concen: 20.000 ng  
 RT: 13.97 min Scan# 2021  
 Delta R.T. 0.00 min  
 Lab File: BF117224.D  
 Acq: 24 Sep 2019 19:14

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 240     | 100   |       |       |
| 120     | 9.2   | 8.3   | 12.5  |
| 236     | 26.4  | 20.3  | 30.5  |

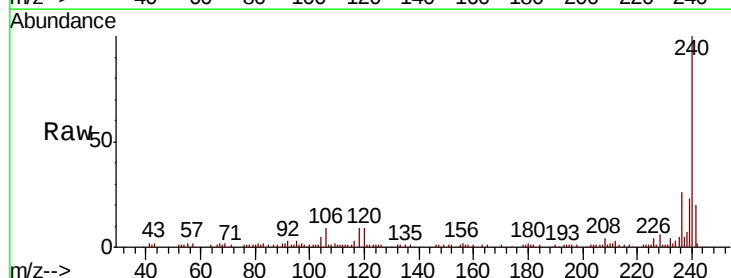

Abundance Ion 240.00 (239.70 to 240.70): E  
 Ion 120.00 (119.70 to 120.70): E  
 Ion 236.00 (235.70 to 236.70): E




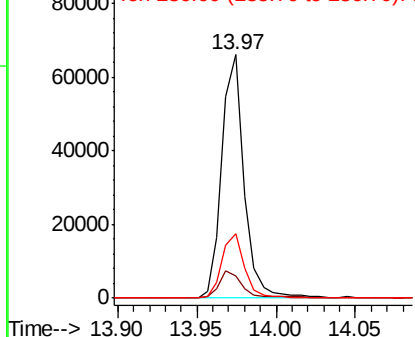


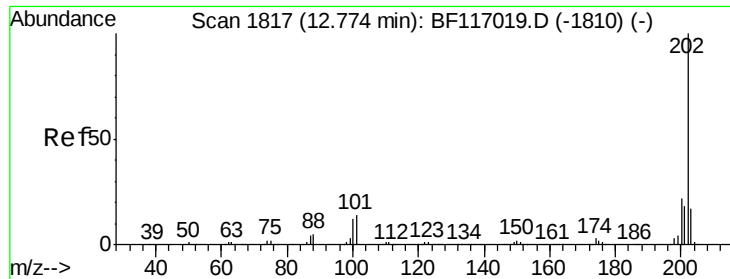

#78  
Pvrene  
Concen: 3.195 ng  
RT: 12.77 min Scan# 1817  
Delta R.T. -0.00 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14




Instrument :  
BNA\_F  
ClientSampleId :


Tot Ion:202 Resp: 17259  
Ion Ratio Lower Upper  
202 100  
200 22.9 17.2 25.8  
203 17.9 14.0 21.0

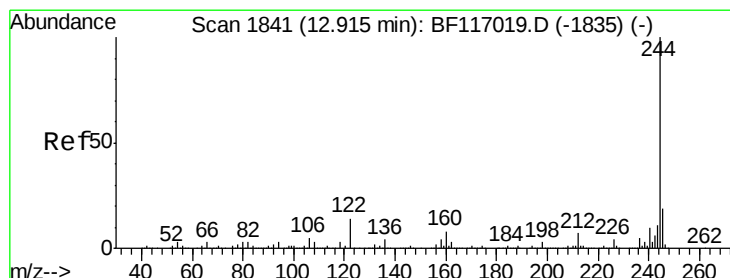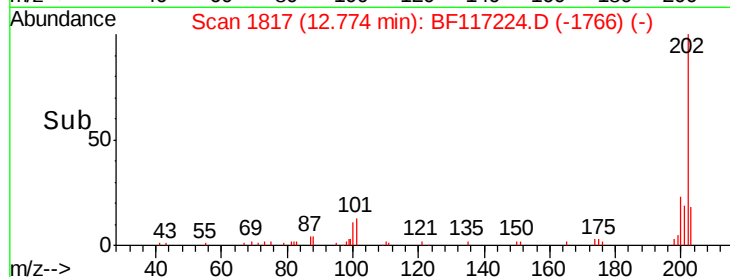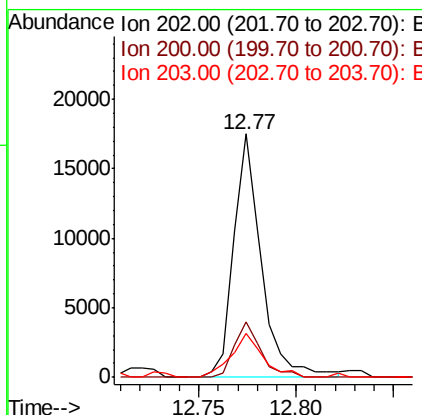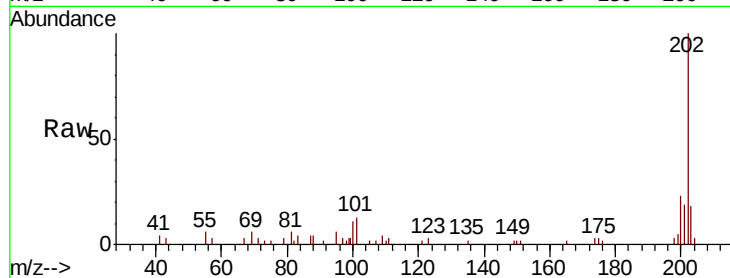

#79  
Terphenyl-d14  
Concen: 64.620 ng  
RT: 12.92 min Scan# 1841  
Delta R.T. -0.00 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Tgt Ion:244 Resp: 222576  
Ion Ratio Lower Upper  
244 100  
212 7.1 5.8 8.8  
122 10.9 11.3 16.9#

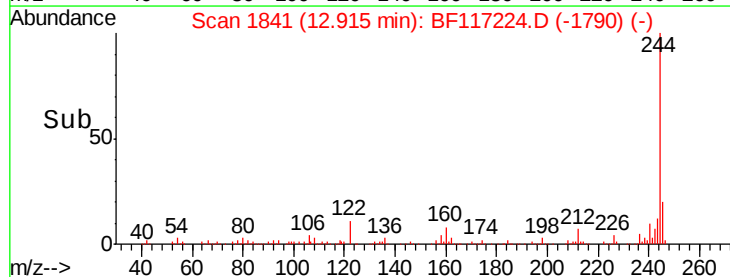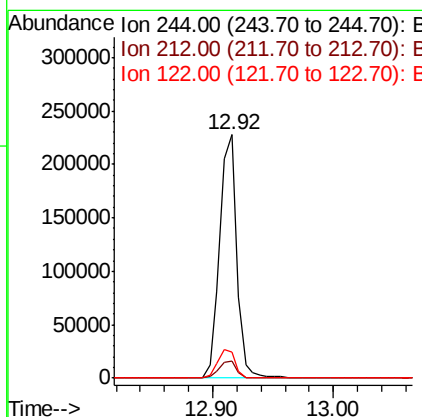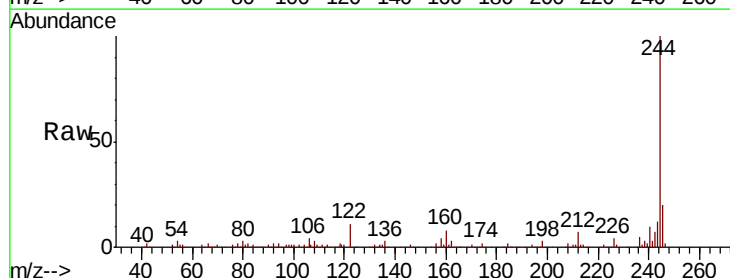


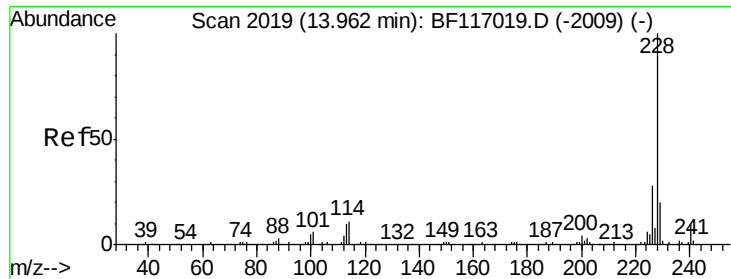

#81  
Benzo(a)anthracene  
Concen: 3.711 ng  
RT: 13.96 min Scan# 2019  
Delta R.T. 0.00 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Instrument :  
BNA\_F  
ClientSampleId :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 228     | 100   |       |       |
| 226     | 33.6  | 22.3  | 33.5# |
| 229     | 22.7  | 15.9  | 23.9  |



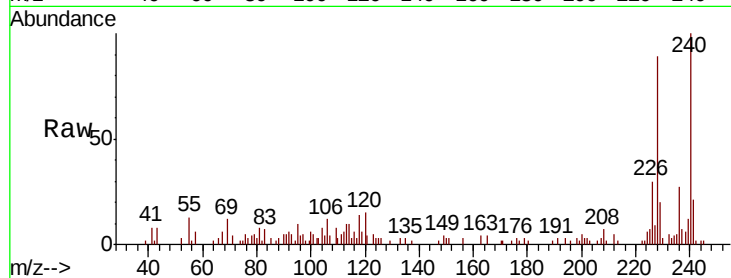


Abundance

Ion 228.00 (227.70 to 228.70): E


Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

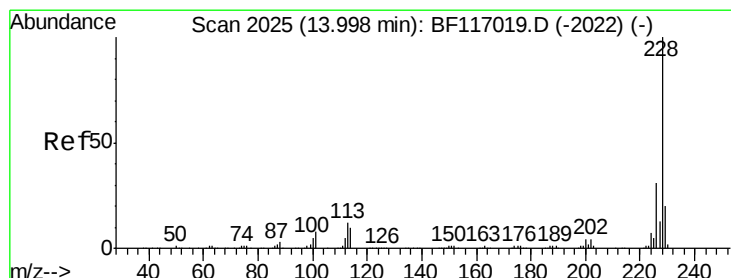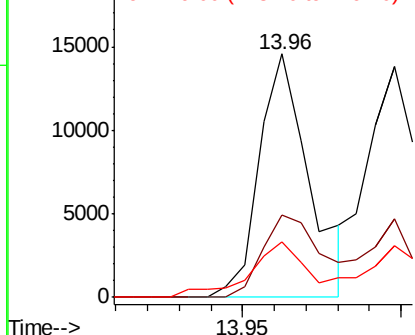

#83  
Chrysene  
Concen: 3.788 ng  
RT: 14.00 min Scan# 2025  
Delta R.T. -0.00 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 228     | 100   |       |       |
| 226     | 33.8  | 24.8  | 37.2  |
| 229     | 22.2  | 15.8  | 23.8  |


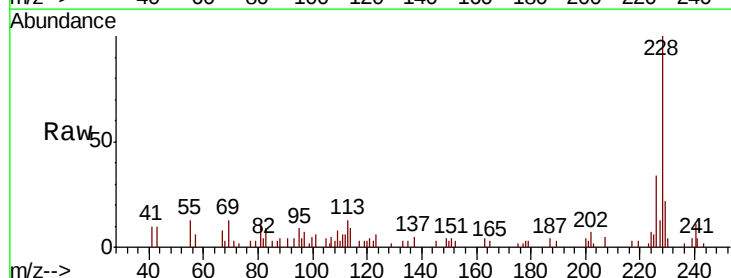



Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

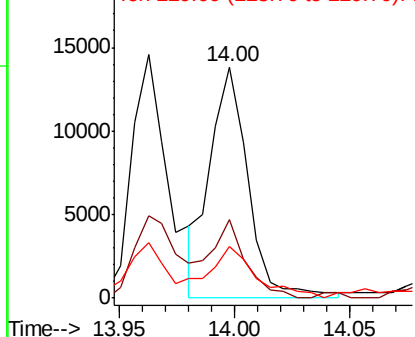


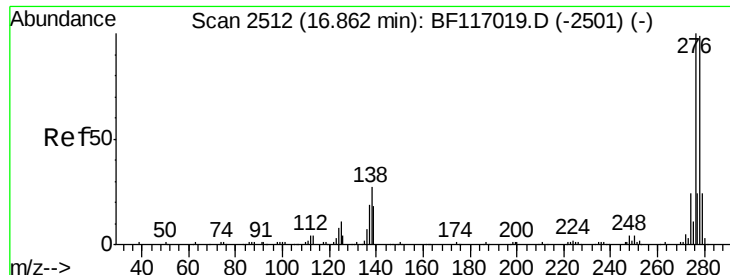




#86  
 Indeno(1,2,3-cd)pyrene  
 Concen: 4.467 ng  
 RT: 16.87 min Scan# 2514  
 Delta R.T. 0.01 min  
 Lab File: BF117224.D  
 Acq: 24 Sep 2019 19:14

Instrument :  
 BNA\_F  
 ClientSampleId :

Tot Ion:276 Resp: 13671  
 Ion Ratio Lower Upper  
 276 100  
 138 23.4 20.7 31.1  
 277 26.0 19.8 29.8

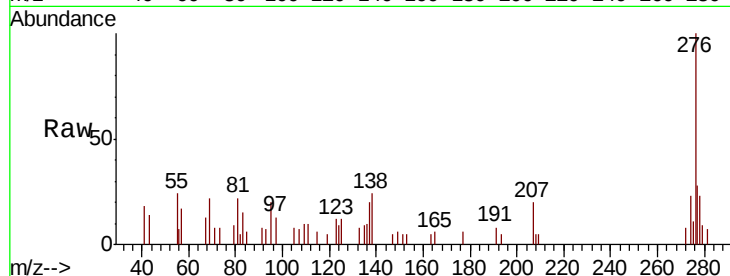


Abundance Ion 276.00 (275.70 to 276.70): E  
 Ion 138.00 (137.70 to 138.70): E  
 Ion 277.00 (276.70 to 277.70): E

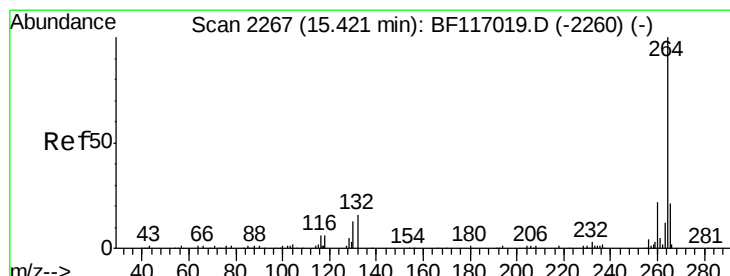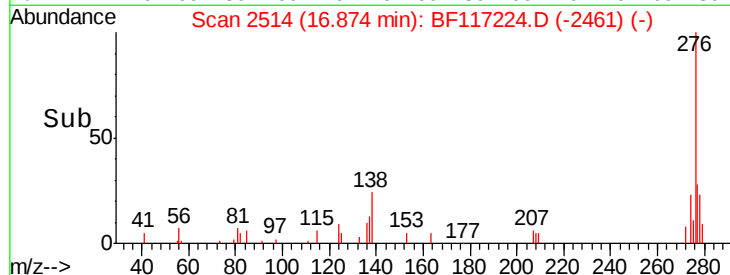
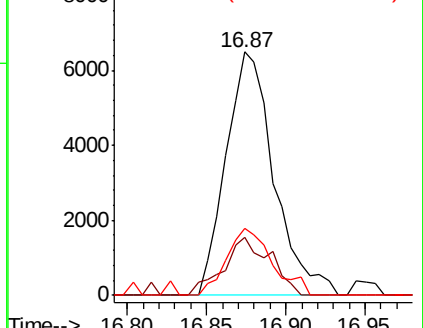



#87  
 Perylene-d12  
 Concen: 20.000 ng  
 RT: 15.43 min Scan# 2268  
 Delta R.T. 0.01 min  
 Lab File: BF117224.D  
 Acq: 24 Sep 2019 19:14

Tgt Ion:264 Resp: 70262  
 Ion Ratio Lower Upper  
 264 100  
 260 23.4 17.6 26.4  
 265 23.2 16.6 24.8

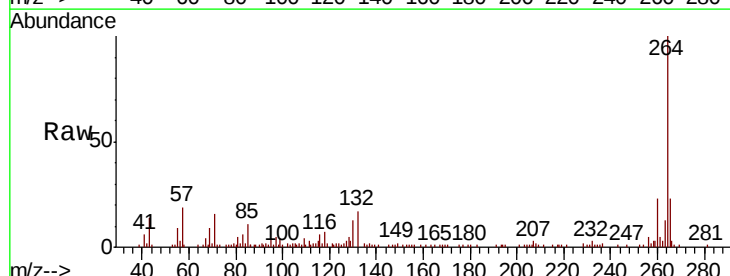

Abundance Ion 264.00 (263.70 to 264.70): E  
 Ion 260.00 (259.70 to 260.70): E  
 Ion 265.00 (264.70 to 265.70): E

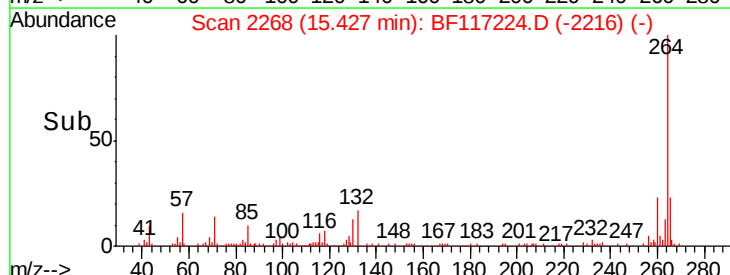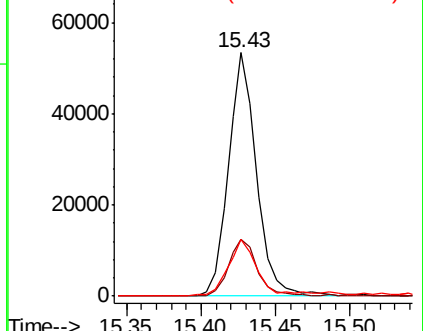


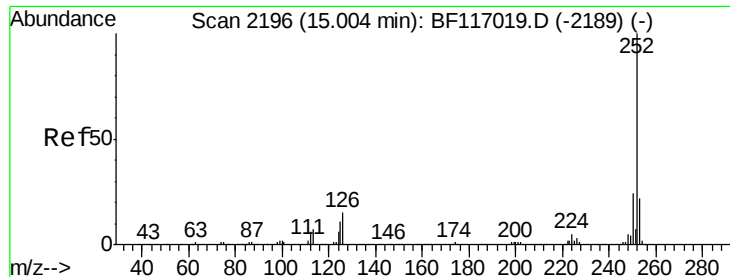

#88  
Benzo(b)fluoranthene  
Concen: 8.706 ng  
RT: 15.01 min Scan# 2197  
Delta R.T. 0.01 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

Instrument :  
BNA\_F  
ClientSampleId :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 22.6  | 17.6  | 26.4  |
| 125     | 12.0  | 8.6   | 12.8  |



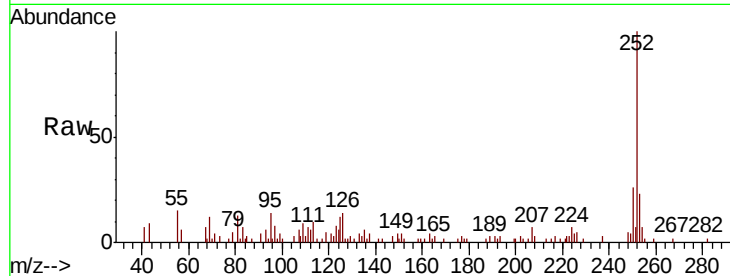


Abundance

Ion 252.00 (251.70 to 252.70): E


Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

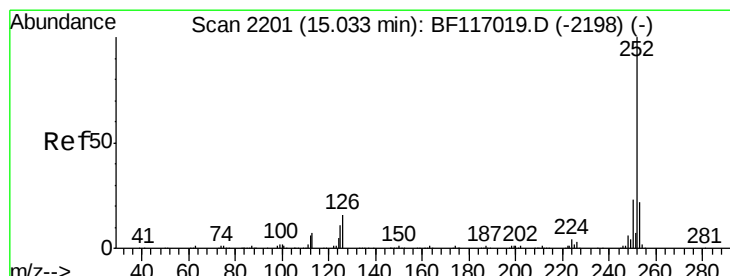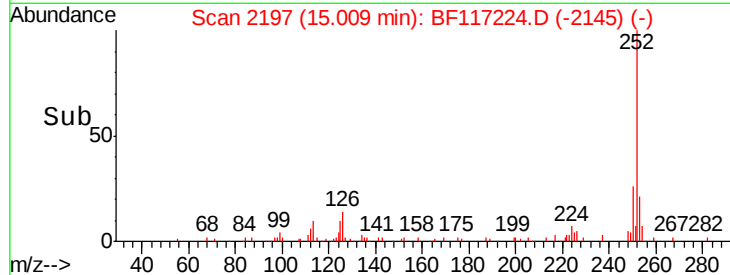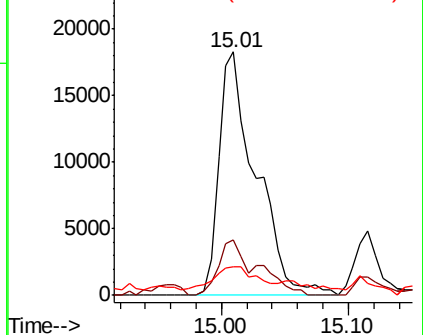

#89  
Benzo(k)fluoranthene  
Concen: 9.191 ng  
RT: 15.01 min Scan# 2197  
Delta R.T. -0.02 min  
Lab File: BF117224.D  
Acq: 24 Sep 2019 19:14

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 22.6  | 17.4  | 26.2  |
| 125     | 12.0  | 8.8   | 13.2  |


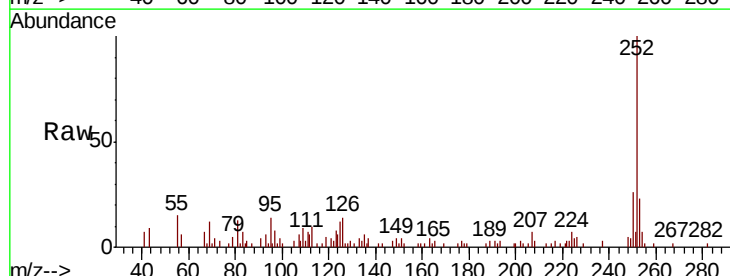



Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

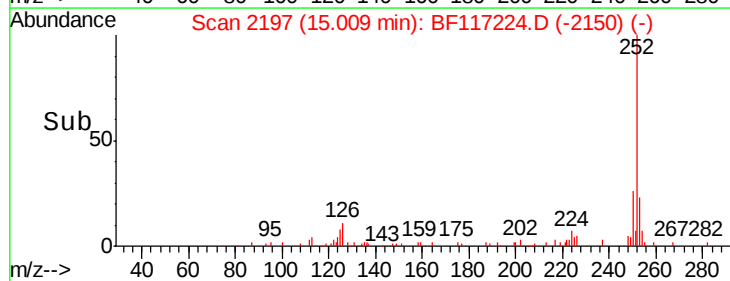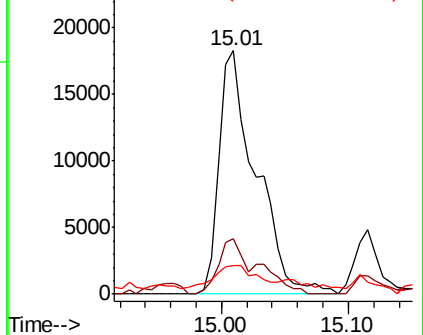



#90

Benzo(a)pyrene

Concen: 5.166 ng

RT: 15.37 min Scan# 2258

Delta R.T. 0.01 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14

Instrument :

BNA\_F

ClientSampleId :


Tot Ion:252 Resp: 19292

Ion Ratio Lower Upper

252 100

253 23.6 16.6 25.0




125 13.3 8.9 13.3

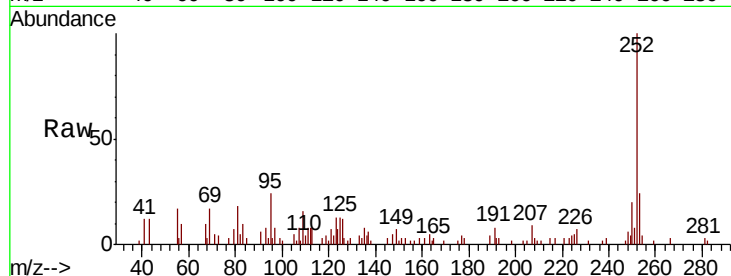

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

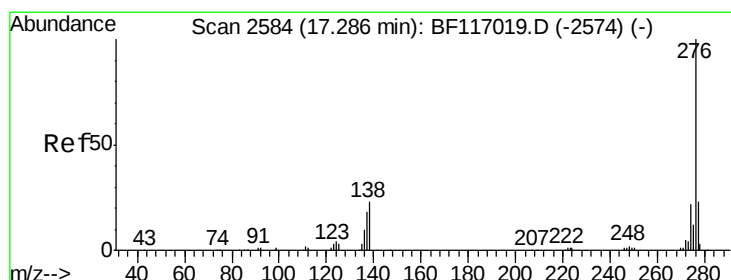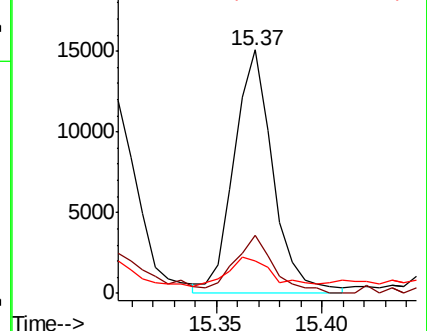

#92

Benzo(g,h,i)perylene

Concen: 4.027 ng

RT: 17.31 min Scan# 2588

Delta R.T. 0.02 min

Lab File: BF117224.D

Acq: 24 Sep 2019 19:14


Tgt Ion:276 Resp: 11939

Ion Ratio Lower Upper

276 100

277 24.0 18.6 27.8

138 20.6 18.0 27.0

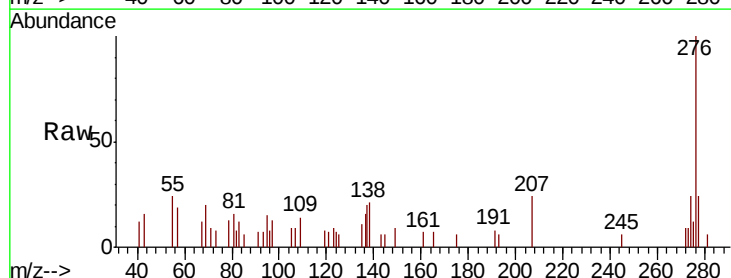

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

