
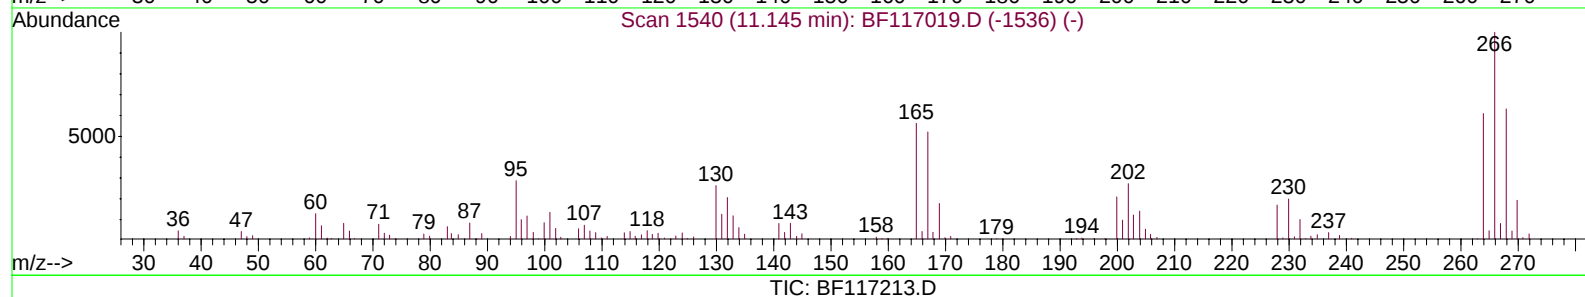
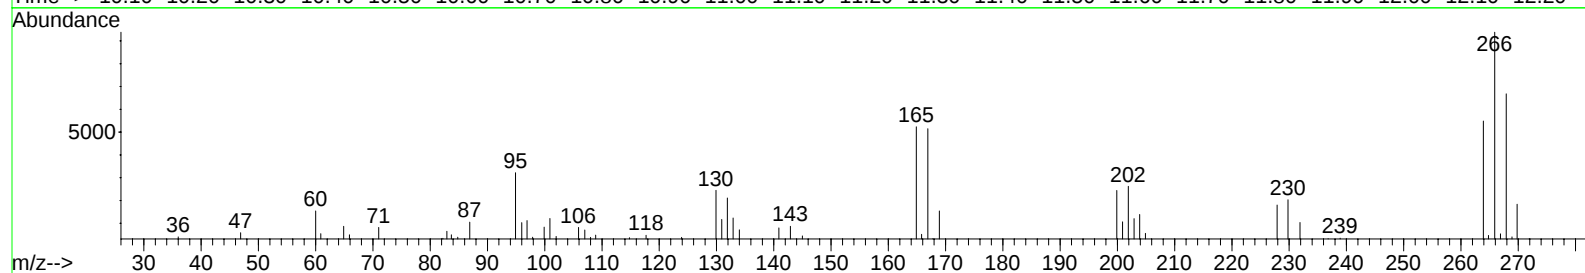


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092419\  
Data File : BF117213.D  
Acq On : 24 Sep 2019 12:47  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:17:59 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 13 16:23:17 2019  
Response via : Initial Calibration

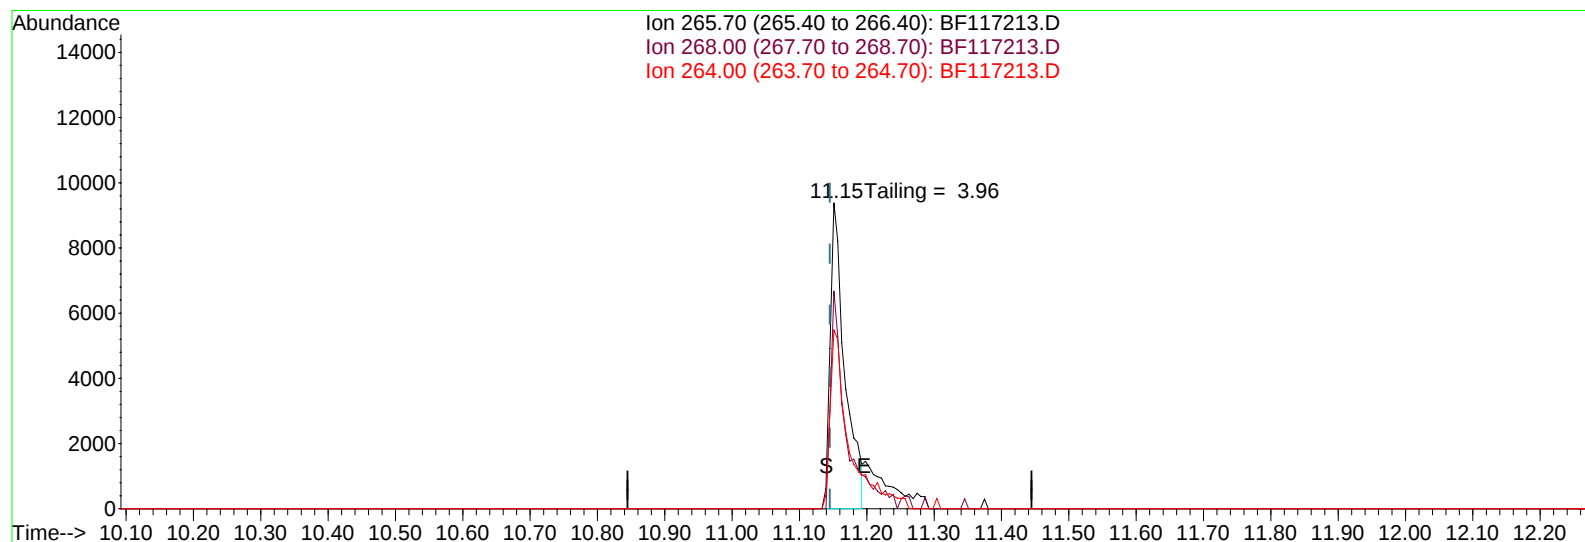

(70) Pentachlorophenol (C)




11.151min (+0.006) 0.00ng

response 17752

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.10 | 71.18 |
| 264.00 | 61.00 | 58.51 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092419\  
Data File : BF117213.D  
Acq On : 24 Sep 2019 12:47  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 24 19:17:59 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 13 16:23:17 2019  
Response via : Initial Calibration

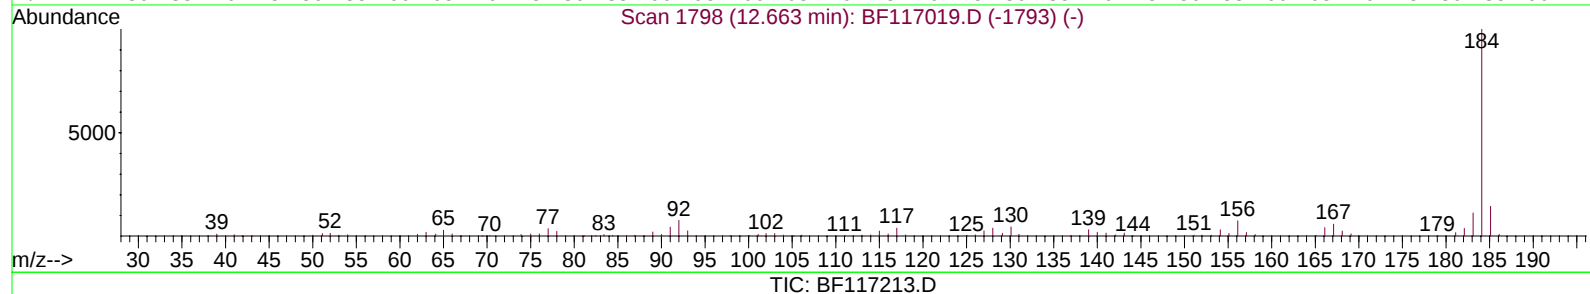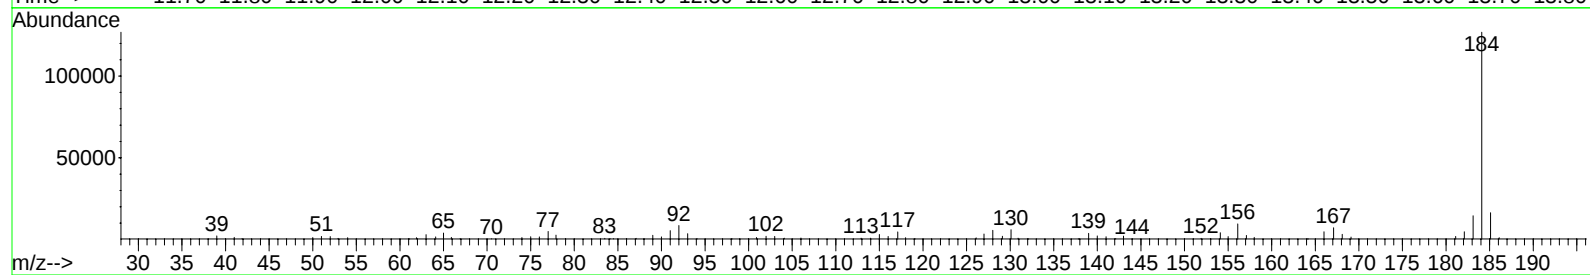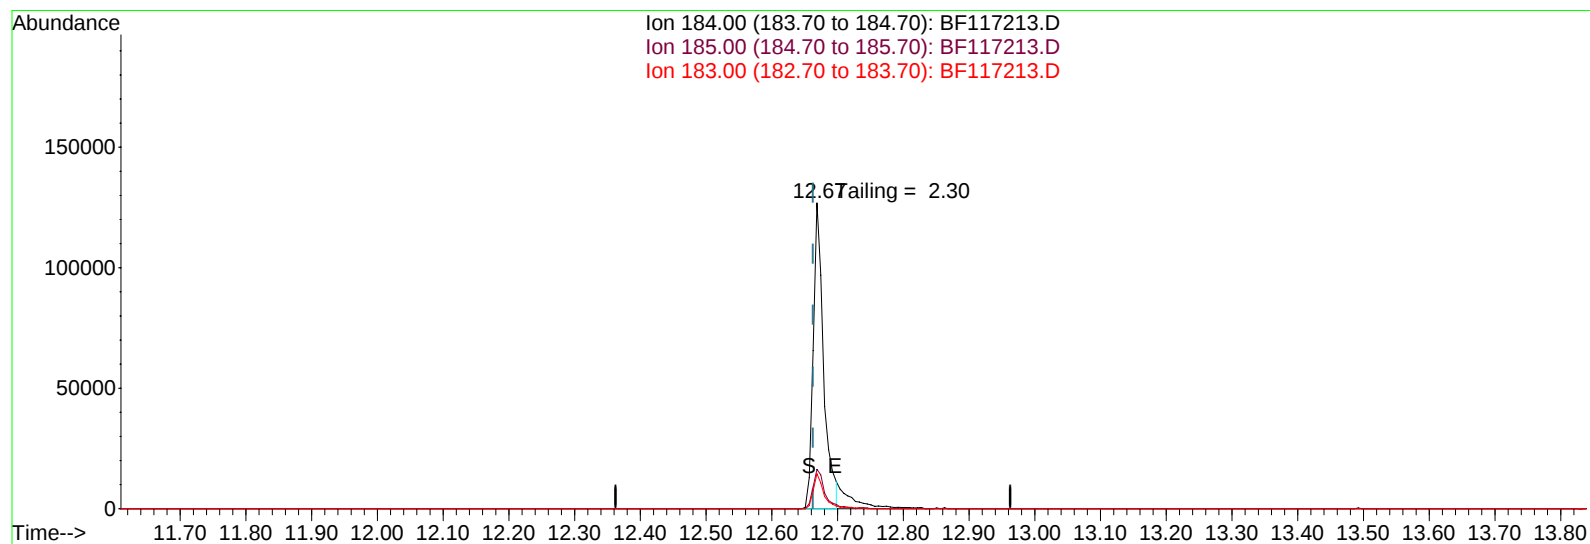

(77) Benzidine

12.669min (+0.006) 0.00ng

response 155798

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.50 | 12.90 |
| 183.00 | 11.20 | 11.47 |
| 0.00   | 0.00  | 0.00  |