


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092419\
 Data File : BF117213.D
 Acq On : 24 Sep 2019 12:47
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

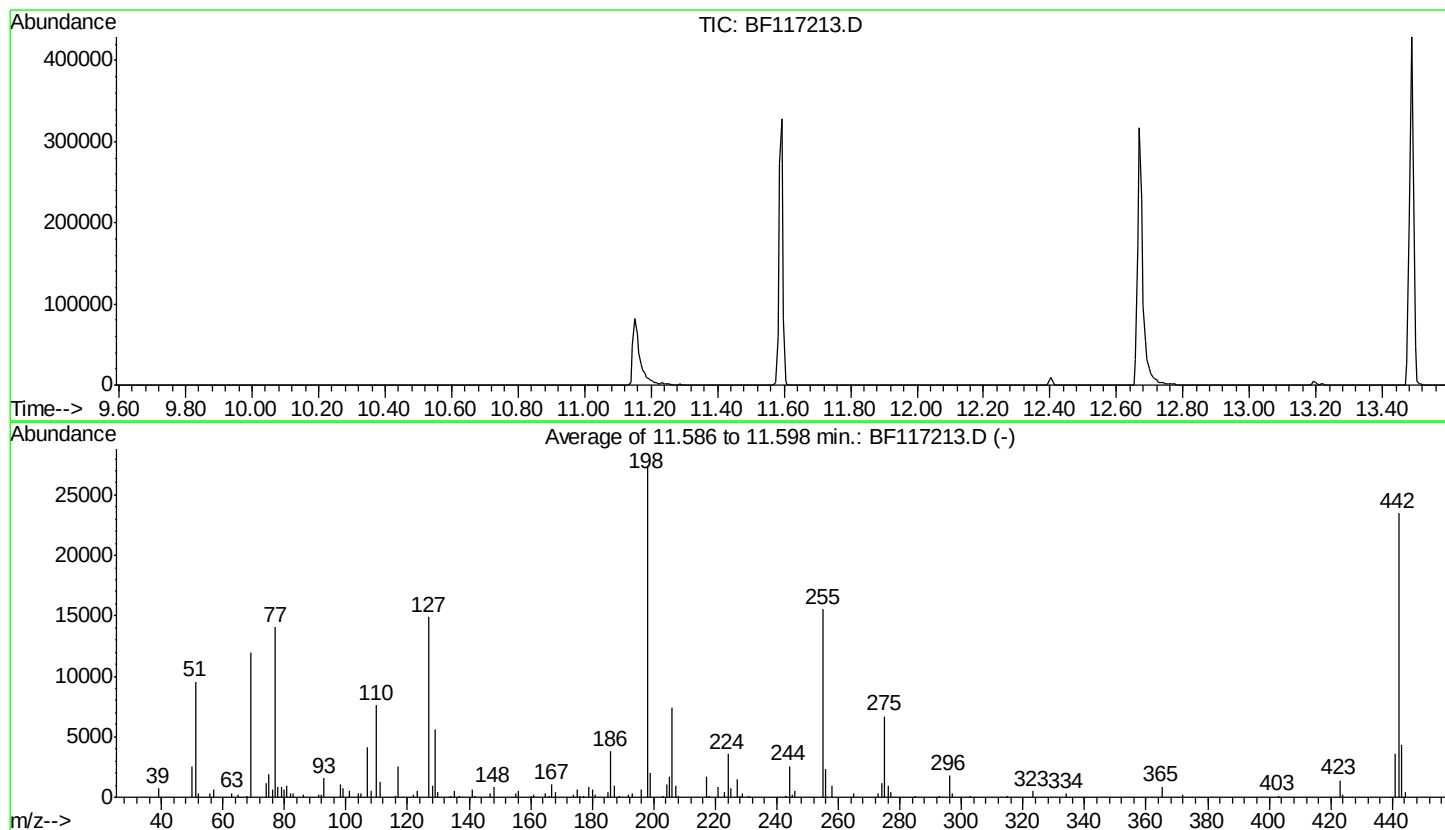

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	9529	PASS
68	69	0.00	2	1.0	125	PASS
69	198	0.00	100	43.6	11960	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.4	14908	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27426	PASS
199	198	5	9	7.2	1976	PASS
275	198	10	60	24.4	6691	PASS
365	198	1	100	3.3	895	PASS
441	198	0.01	100	13.0	3553	PASS
442	198	50	100	85.6	23466	PASS
443	442	15	24	18.6	4375	PASS