
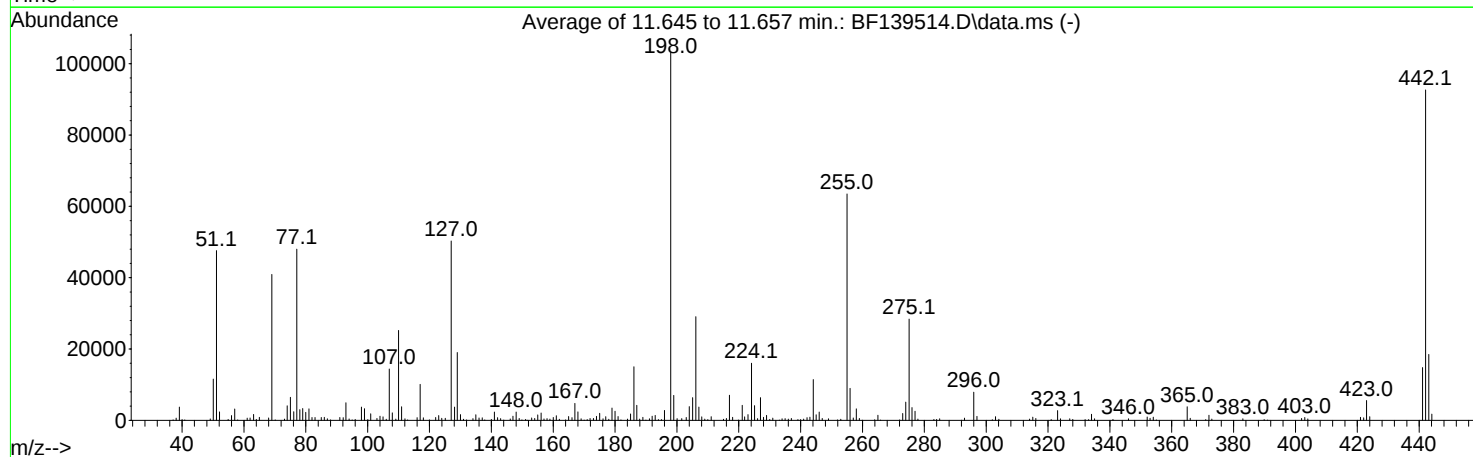


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092424\
Data File : BF139514.D
Acq On : 24 Sep 2024 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

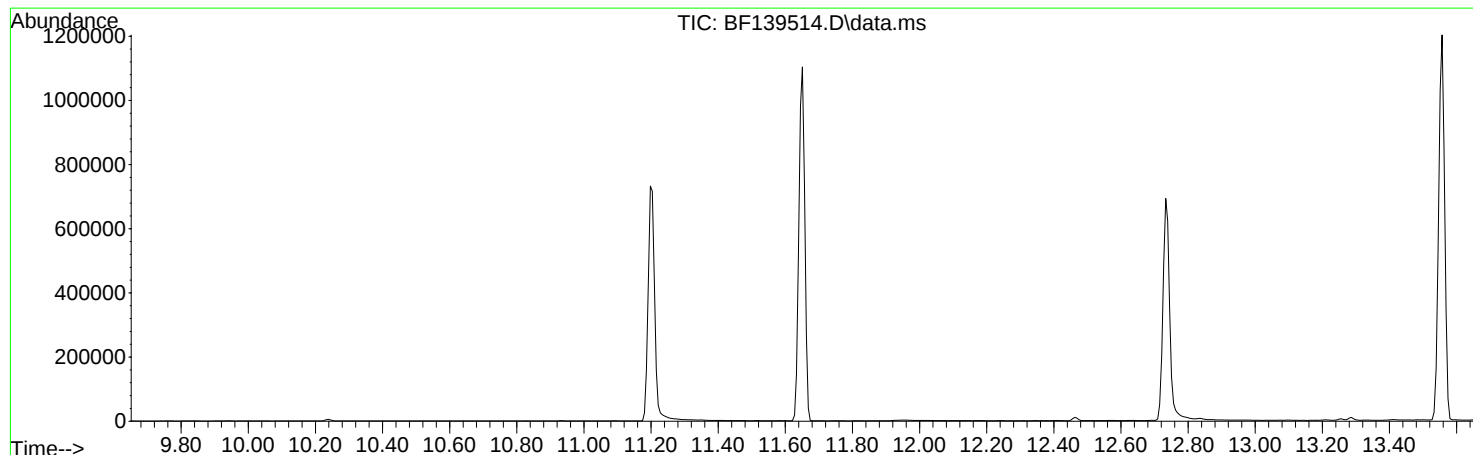

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	46.1	47581	PASS
68	69	0.00	2	1.7	699	PASS
69	198	0.00	100	39.7	40893	PASS
70	69	0.00	2	0.3	142	PASS
127	198	10	80	48.8	50285	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103133	PASS
199	198	5	9	6.8	7019	PASS
275	198	10	60	27.6	28419	PASS
365	198	1	100	3.7	3797	PASS
441	198	0.01	100	14.3	14789	PASS
442	442	50	100	100.0	92645	PASS
443	442	15	24	19.9	18464	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/24/2024	BNA_F	<u>BF139514.D</u>
Compound Name	Response	Retention Time
DDT	289110	13.557
DDD	4181	13.286
DDE	138	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4319	293429	1.47

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092424\
Data File : BF139514.D
Acq On : 24 Sep 2024 10:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 24 13:07:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

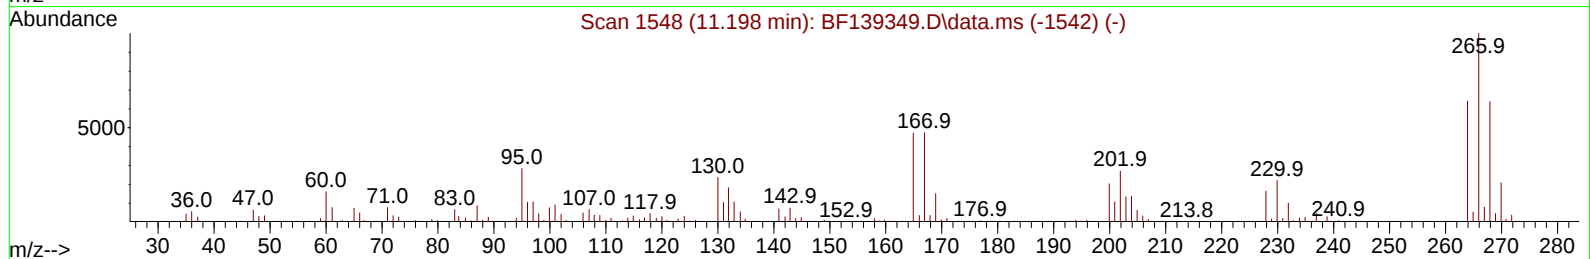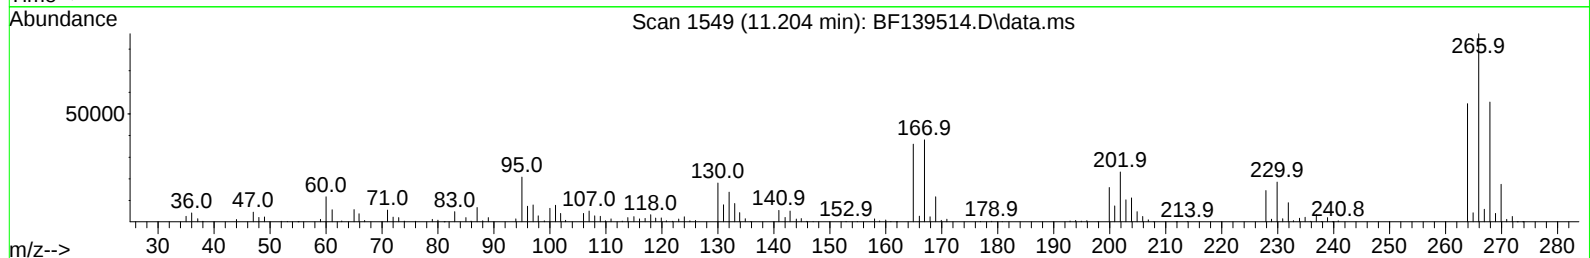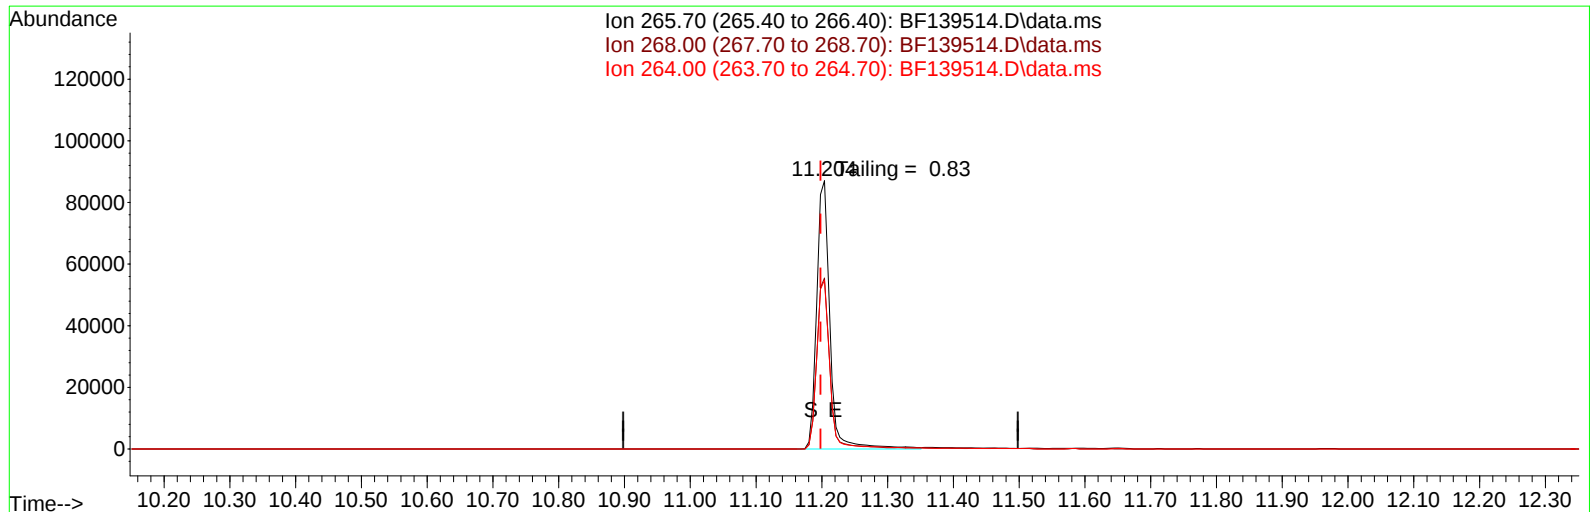

TIC: BF139514.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 36934.51 ng

response 121660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.75
264.00	64.20	62.89
0.00	0.00	0.00

