


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092519\
 Data File : BF117235.D
 Acq On : 25 Sep 2019 11:53
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

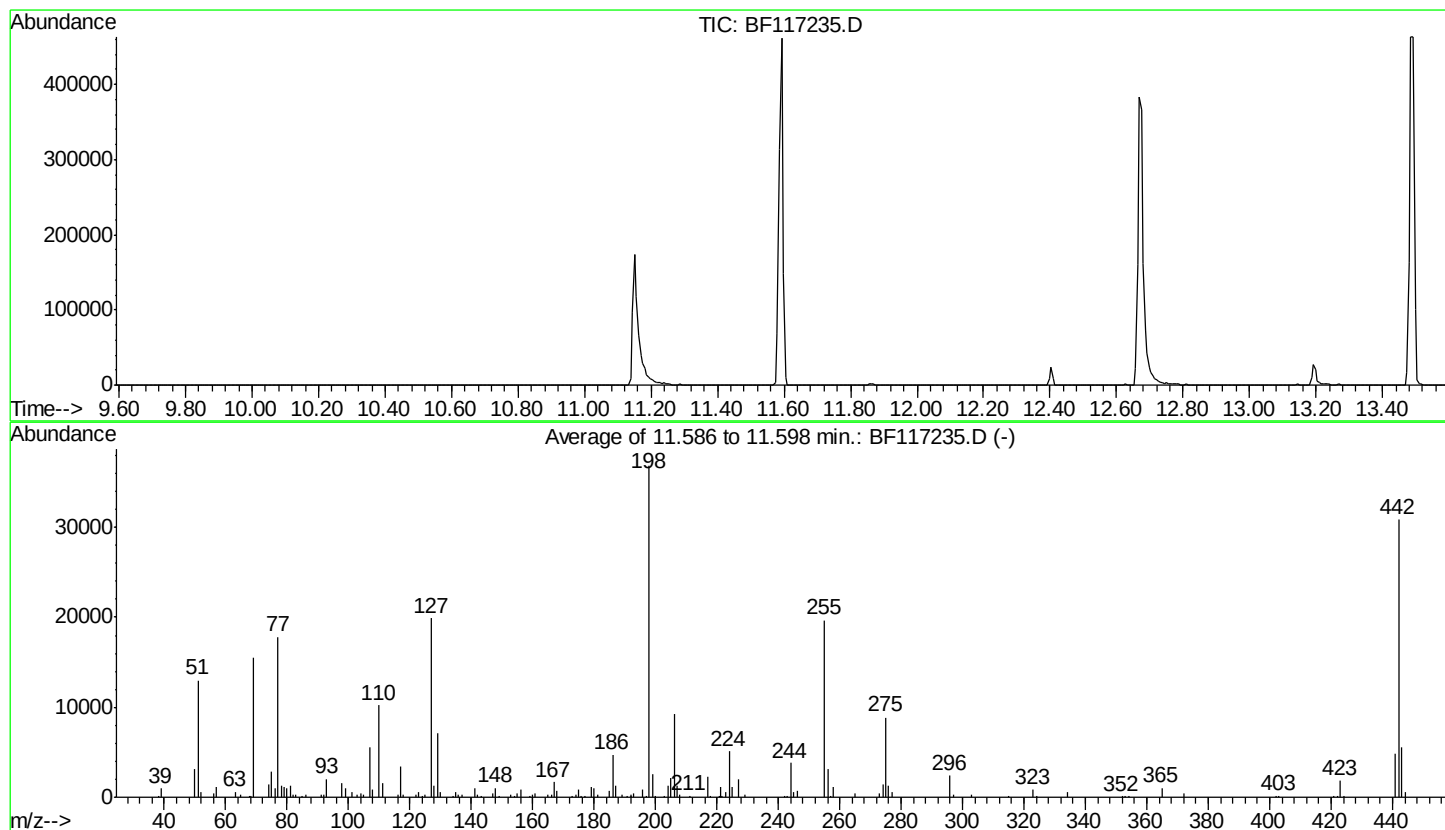

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	12988	PASS
68	69	0.00	2	1.2	181	PASS
69	198	0.00	100	42.1	15511	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.9	19866	PASS
197	198	0.00	2	0.3	108	PASS
198	198	100	100	100.0	36853	PASS
199	198	5	9	6.9	2528	PASS
275	198	10	60	24.1	8875	PASS
365	198	1	100	2.9	1066	PASS
441	198	0.01	100	13.1	4823	PASS
442	198	50	100	83.7	30840	PASS
443	442	15	24	18.1	5567	PASS