


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092519\
 Data File : BF117258.D
 Acq On : 26 Sep 2019 00:17
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

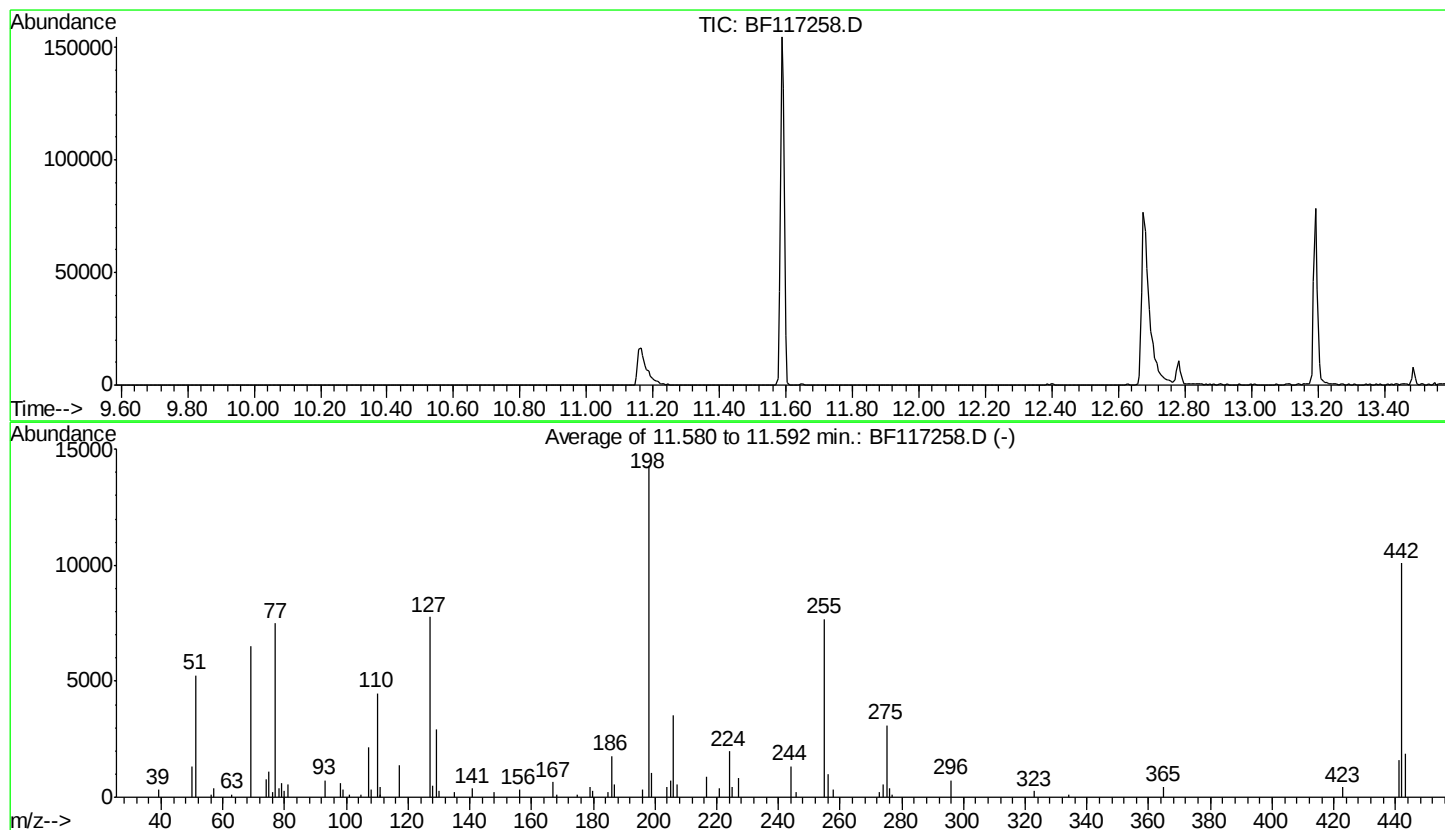

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	5258	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.4	6495	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	7761	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14297	PASS
199	198	5	9	7.2	1027	PASS
275	198	10	60	21.8	3111	PASS
365	198	1	100	3.1	449	PASS
441	198	0.01	100	11.3	1621	PASS
442	198	50	100	70.6	10095	PASS
443	442	15	24	18.8	1901	PASS