

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135422.D
Acq On : 25 Sep 2023 12:40
Operator : CG\JU
Sample : PB155762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155762BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	579	rBV	4473340	4833062	97.64%	15.407%
2	6.404	728	734	748	rBV	4170208	4839333	97.77%	15.427%
3	6.751	789	793	803	rBV	1169061	951075	19.21%	3.032%
4	7.316	884	889	892	rBV	2882137	3175928	64.16%	10.124%
5	8.028	1006	1010	1026	rBV	1212569	1238759	25.03%	3.949%
6	9.110	1188	1194	1197	rBV	4667476	4949701	100.00%	15.779%
7	9.786	1304	1309	1313	rBV	1470853	1283891	25.94%	4.093%
8	10.586	1440	1445	1448	rBV	2719513	2724787	55.05%	8.686%
9	11.280	1559	1563	1572	rBV	1537119	1297330	26.21%	4.136%
10	12.880	1830	1835	1838	rBV	4191478	4365557	88.20%	13.917%
11	13.939	2011	2015	2023	rBV	922777	900748	18.20%	2.871%
12	15.404	2259	2264	2278	rVB	590855	809217	16.35%	2.580%




Sum of corrected areas: 31369388

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135422.D
Acq On : 25 Sep 2023 12:40
Operator : CG\JU
Sample : PB155762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155762BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

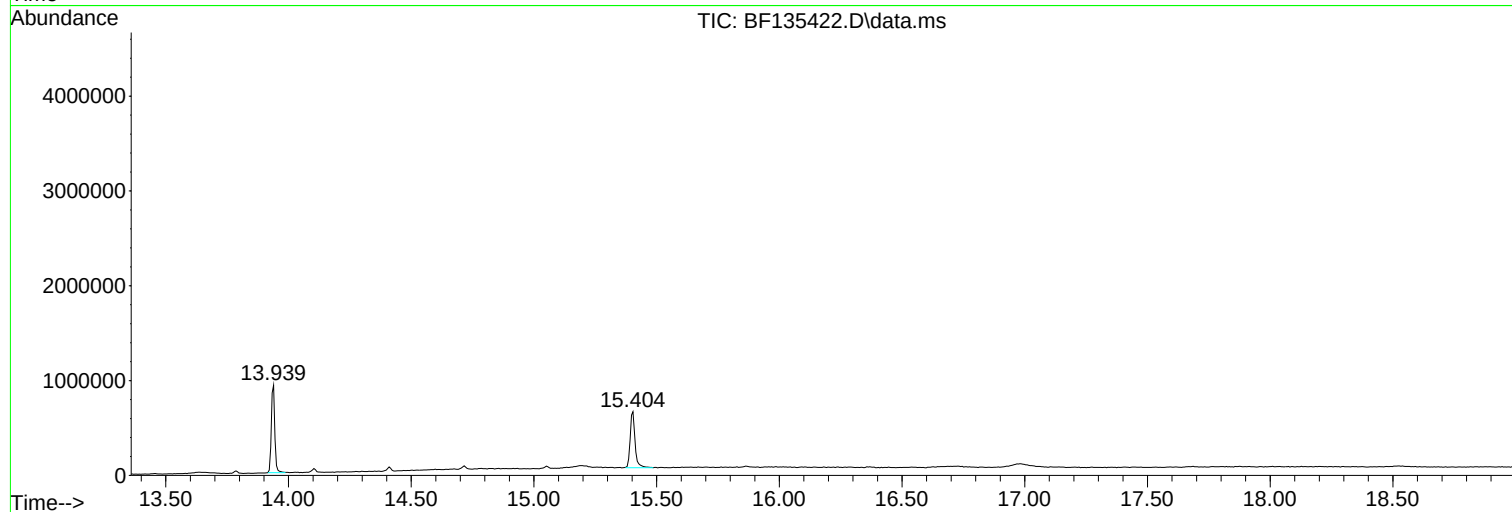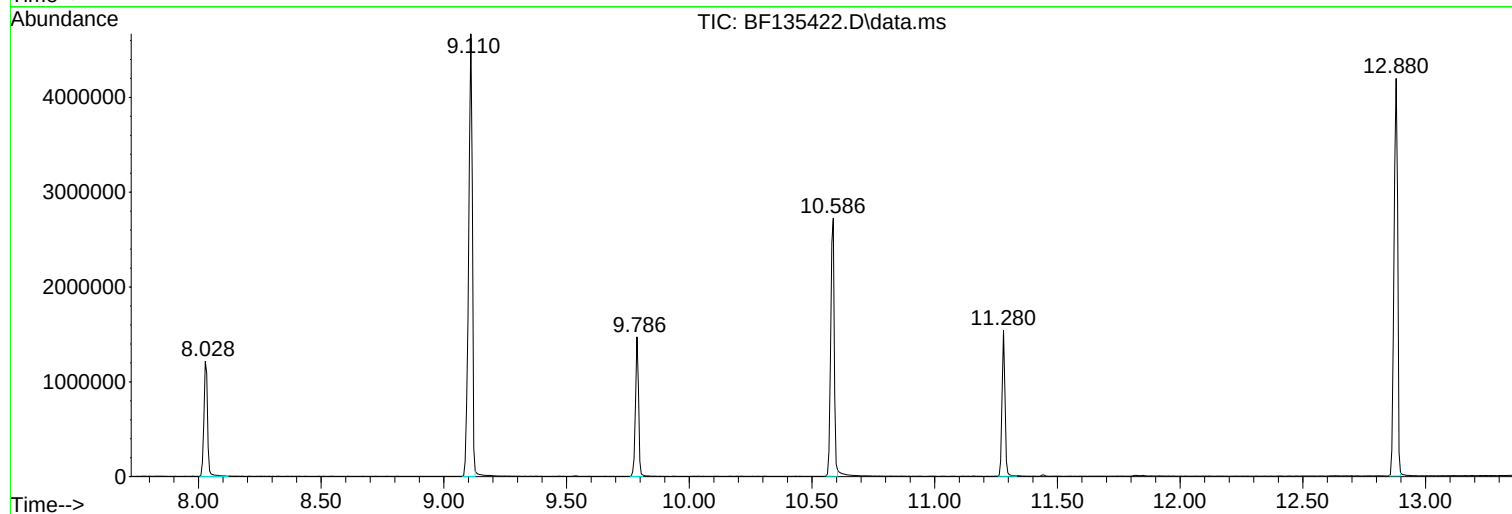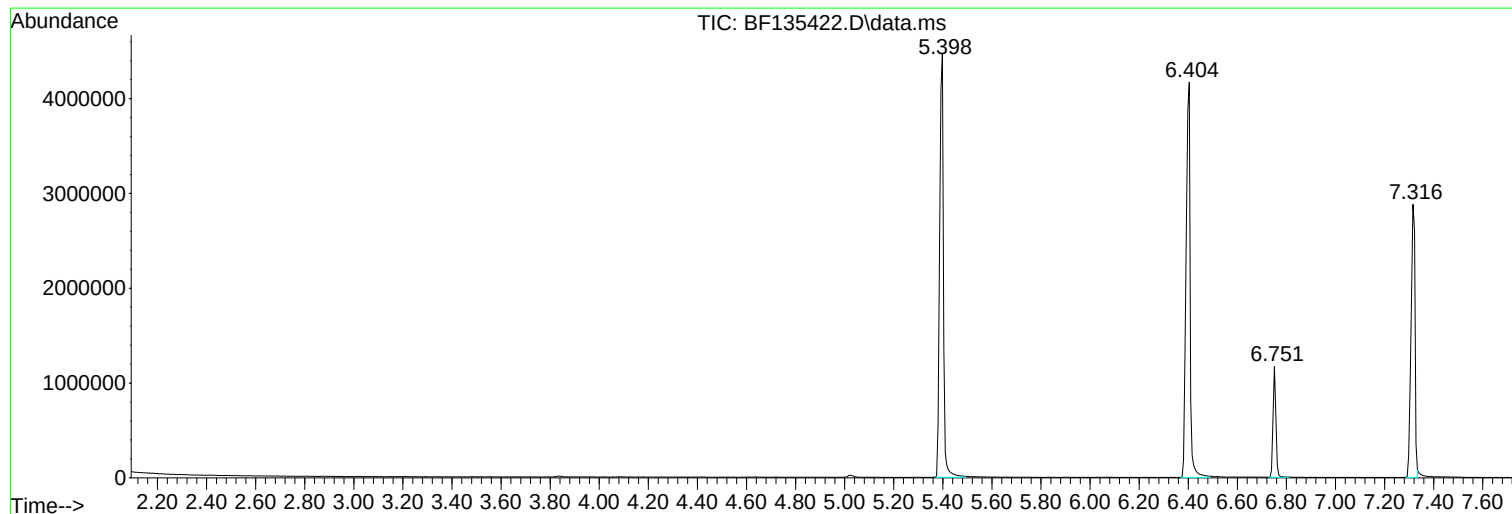

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135422.D
Acq On : 25 Sep 2023 12:40
Operator : CG\JU
Sample : PB155762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155762BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135422.D
Acq On : 25 Sep 2023 12:40
Operator : CG\JU
Sample : PB155762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155762BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------