

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135424.D
Acq On : 25 Sep 2023 13:42
Operator : CG\JU
Sample : PB155763BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155763BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	558	562	582	rBV	4370436	4692839	98.60%	15.144%
2	6.398	728	733	756	rBV	3960777	4759299	100.00%	15.358%
3	6.751	789	793	807	rBV	1290998	1044870	21.95%	3.372%
4	7.316	884	889	892	rBV	2826418	3066920	64.44%	9.897%
5	8.028	1006	1010	1026	rBV	1333624	1339924	28.15%	4.324%
6	9.110	1188	1194	1197	rBV	4613968	4757364	99.96%	15.352%
7	9.786	1304	1309	1313	rBV	1596165	1383011	29.06%	4.463%
8	10.586	1440	1445	1448	rBV	2495710	2621278	55.08%	8.459%
9	11.280	1559	1563	1571	rBV	1652009	1387412	29.15%	4.477%
10	12.880	1830	1835	1838	rBV	4225092	4135997	86.90%	13.347%
11	13.939	2011	2015	2022	rBV	920053	937913	19.71%	3.027%
12	15.404	2259	2264	2278	rVB	628225	861660	18.10%	2.781%




Sum of corrected areas: 30988487

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135424.D
Acq On : 25 Sep 2023 13:42
Operator : CG\JU
Sample : PB155763BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155763BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

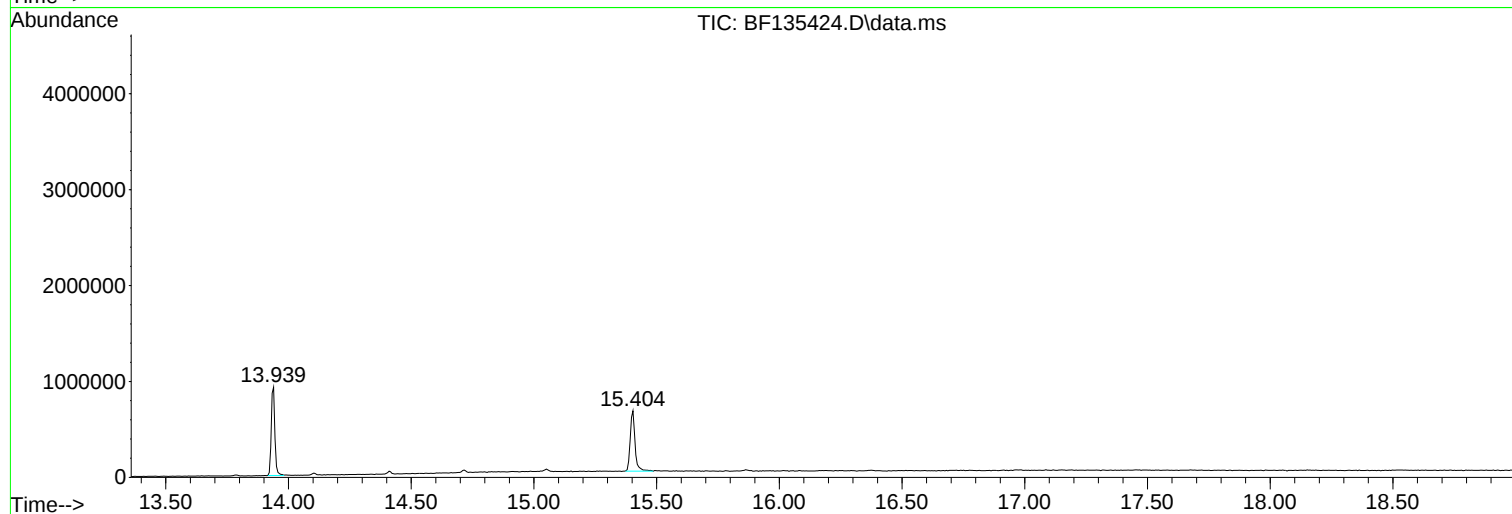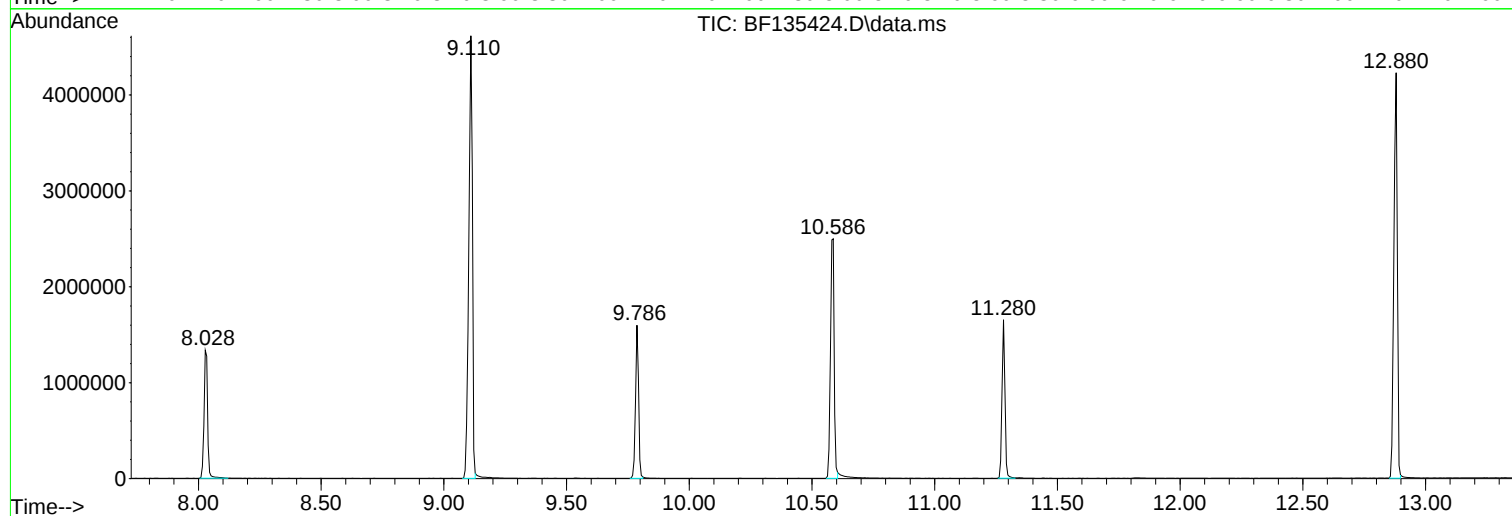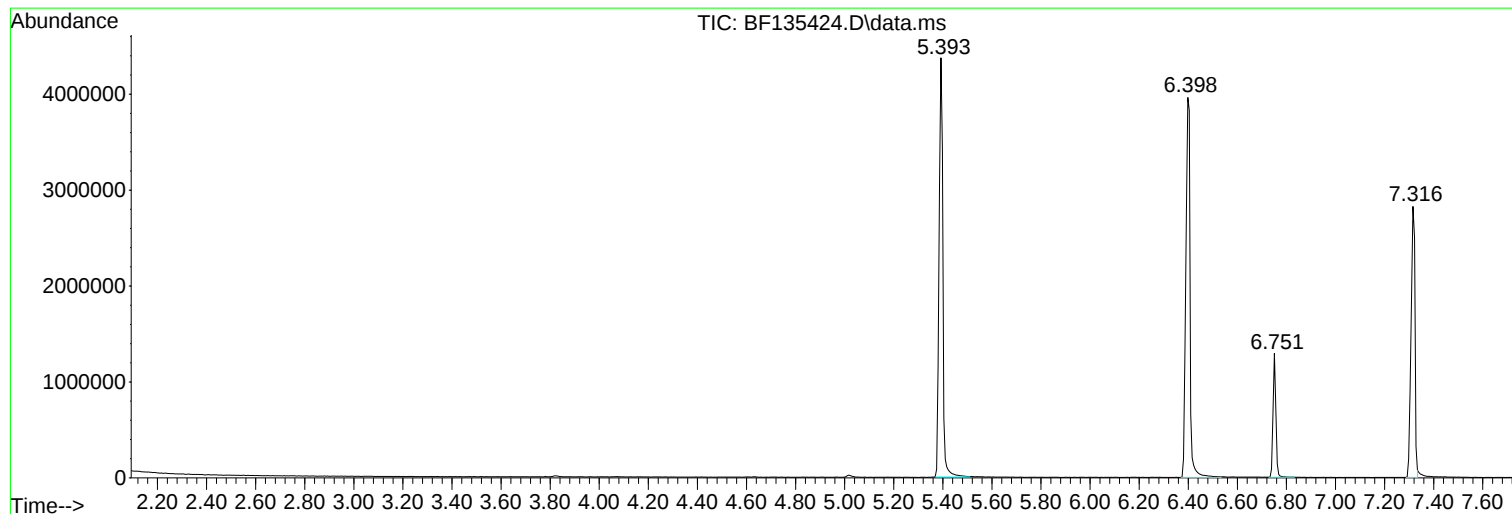

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135424.D
Acq On : 25 Sep 2023 13:42
Operator : CG\JU
Sample : PB155763BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155763BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135424.D
Acq On : 25 Sep 2023 13:42
Operator : CG\JU
Sample : PB155763BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155763BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------