

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135427.D
Acq On : 25 Sep 2023 15:15
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	584	rBV	4430990	4911881	98.54%	15.545%
2	6.398	728	733	756	rBV	4030003	4946995	99.24%	15.656%
3	6.751	789	793	809	rVB	1166783	970537	19.47%	3.072%
4	7.316	884	889	903	rBV	2825442	3314125	66.48%	10.488%
5	8.028	1006	1010	1018	rBV	1254082	1246218	25.00%	3.944%
6	9.110	1188	1194	1197	rBV	4807013	4984857	100.00%	15.776%
7	9.786	1304	1309	1319	rBV	1481253	1307400	26.23%	4.138%
8	10.580	1440	1444	1458	rBV	2665348	2747689	55.12%	8.696%
9	11.280	1559	1563	1572	rBV	1522052	1290618	25.89%	4.085%
10	12.880	1830	1835	1838	rBV	4198791	4238513	85.03%	13.414%
11	13.939	2011	2015	2022	rBV	845974	852486	17.10%	2.698%
12	15.404	2259	2264	2275	rBV	556131	786415	15.78%	2.489%




Sum of corrected areas: 31597734

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135427.D
Acq On : 25 Sep 2023 15:15
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

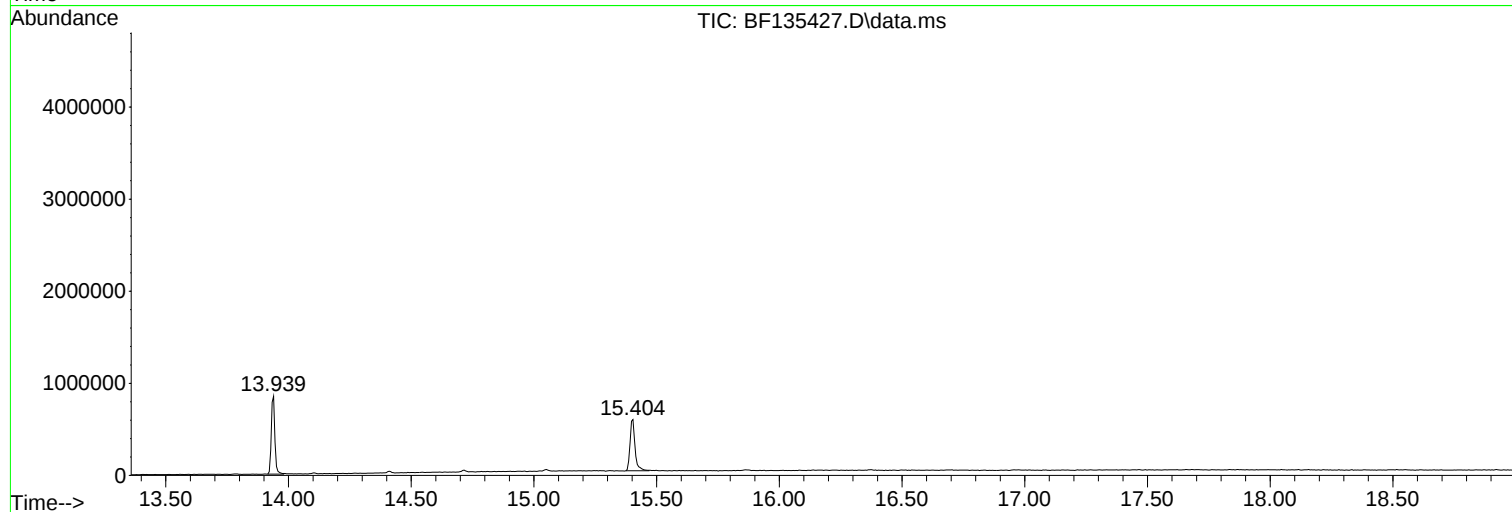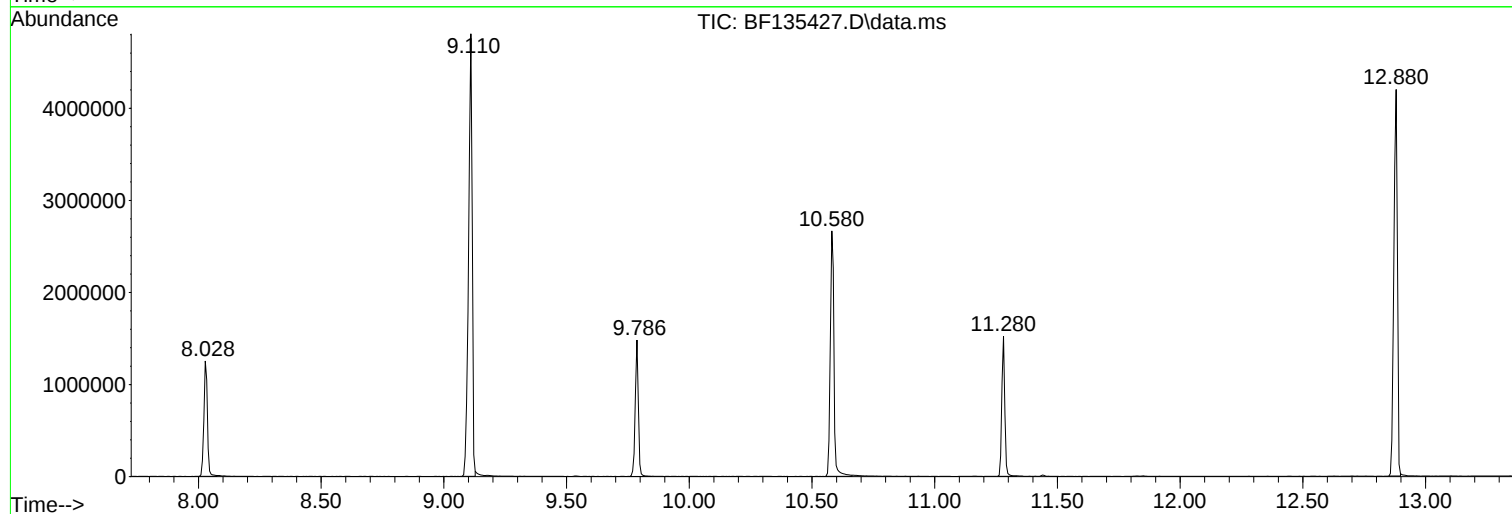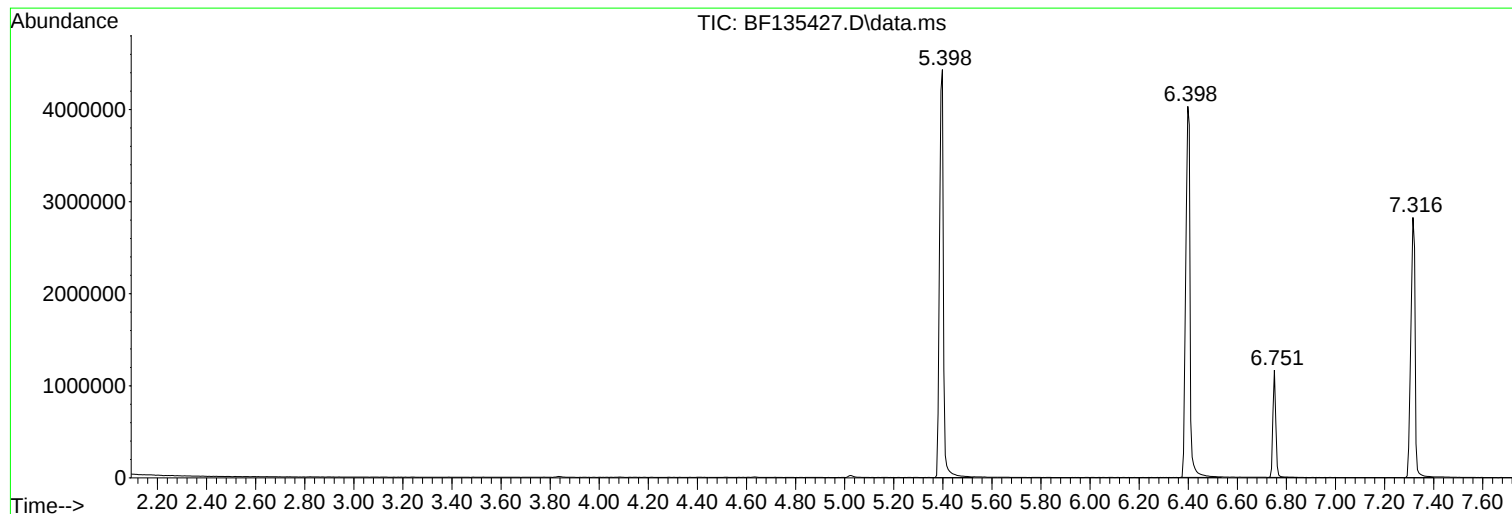

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135427.D
Acq On : 25 Sep 2023 15:15
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135427.D
Acq On : 25 Sep 2023 15:15
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------