
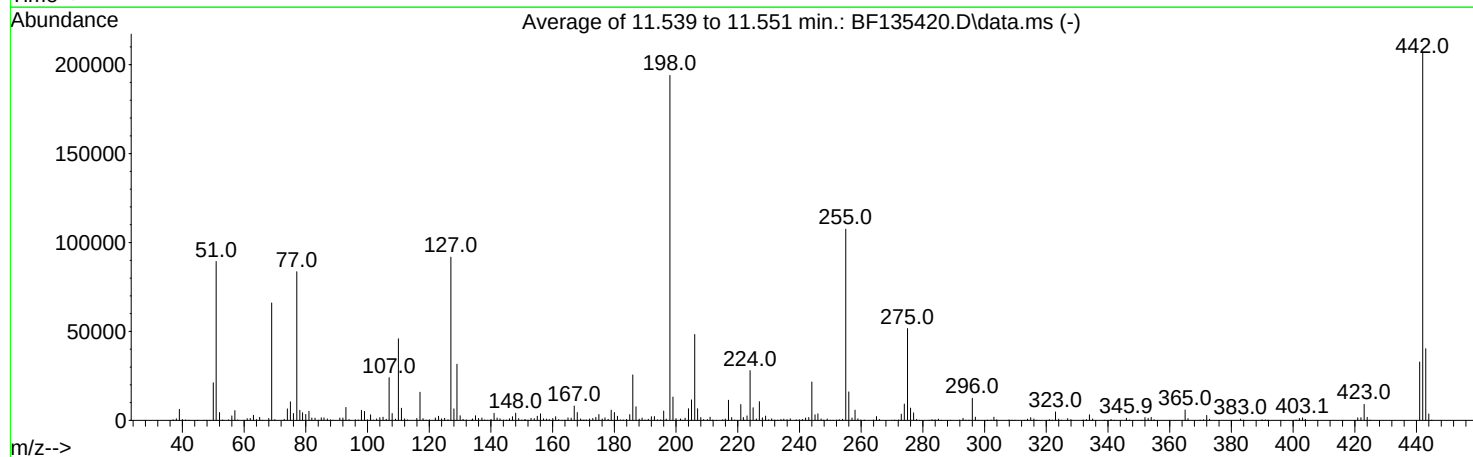


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
 Data File : BF135420.D
 Acq On : 25 Sep 2023 11:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 26 01:36:36 2023

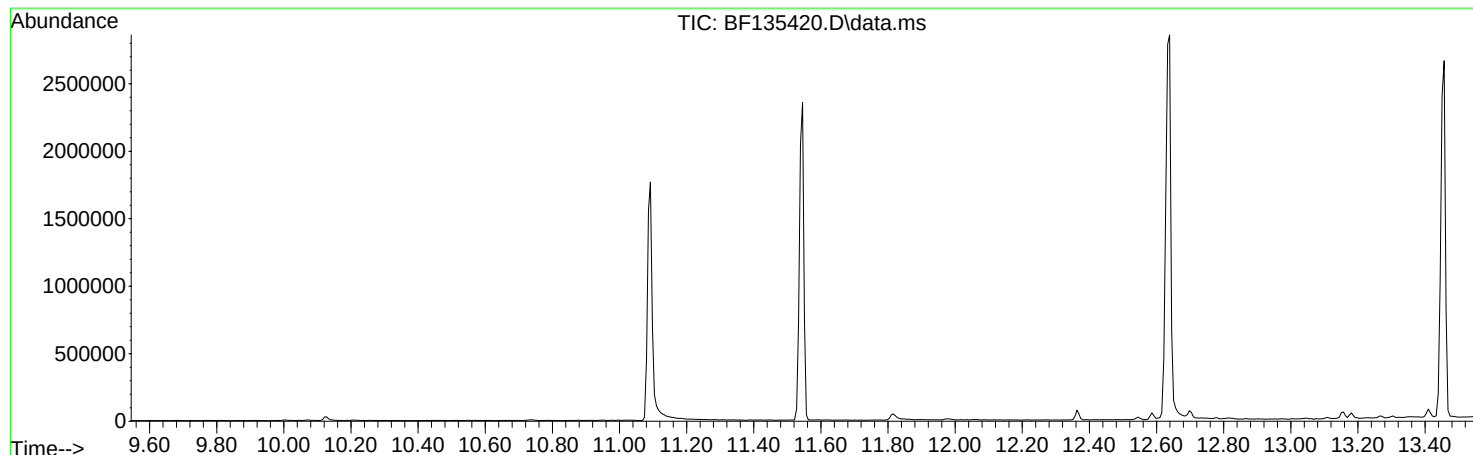




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	89323	PASS
68	69	0.00	2	1.7	1109	PASS
69	198	0.00	100	34.0	66029	PASS
70	69	0.00	2	0.7	457	PASS
127	198	10	80	47.3	91776	PASS
197	198	0.00	2	0.4	743	PASS
198	198	100	100	100.0	194005	PASS
199	198	5	9	6.8	13101	PASS
275	198	10	60	26.6	51627	PASS
365	198	1	100	3.0	5878	PASS
441	198	0.01	100	16.9	32856	PASS
442	442	50	100	100.0	206848	PASS
443	442	15	24	19.5	40357	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
Data File : BF135420.D
Acq On : 25 Sep 2023 11:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 26 03:57:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration

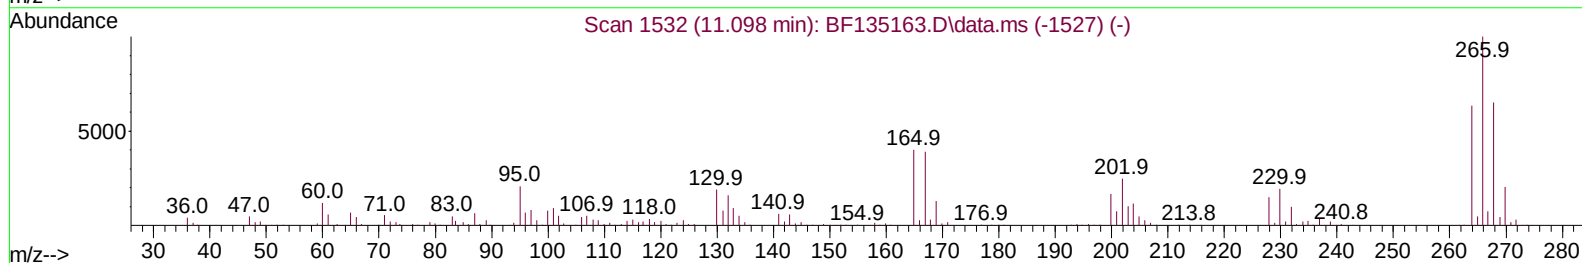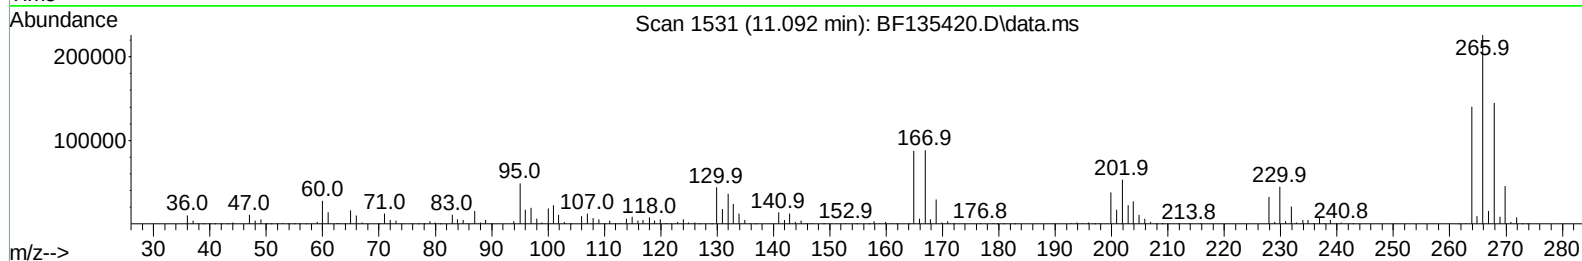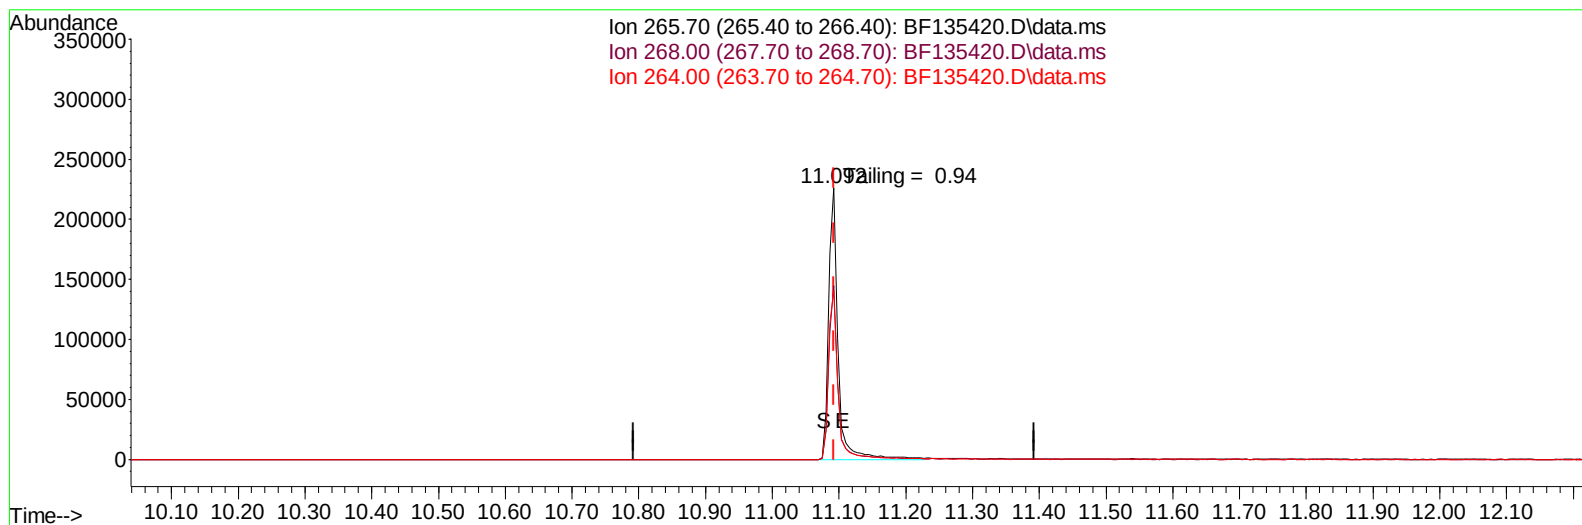

TIC: BF135420.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.000) 630342.16 ng




response 225455

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.95
264.00	63.50	62.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092523\
 Data File : BF135420.D
 Acq On : 25 Sep 2023 11:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 26 03:57:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 26 01:36:36 2023
 Response via : Initial Calibration

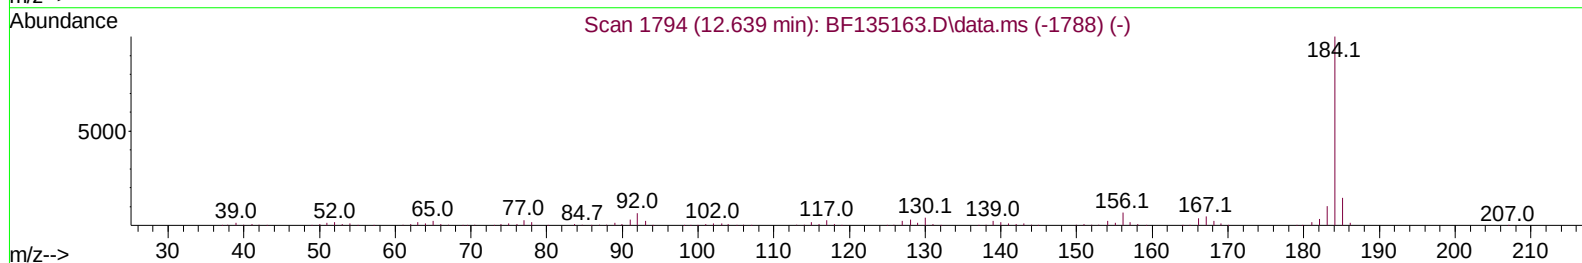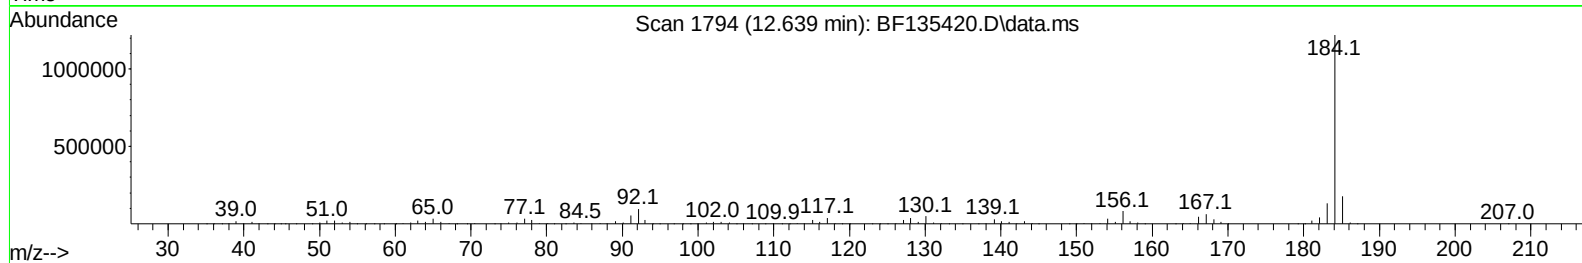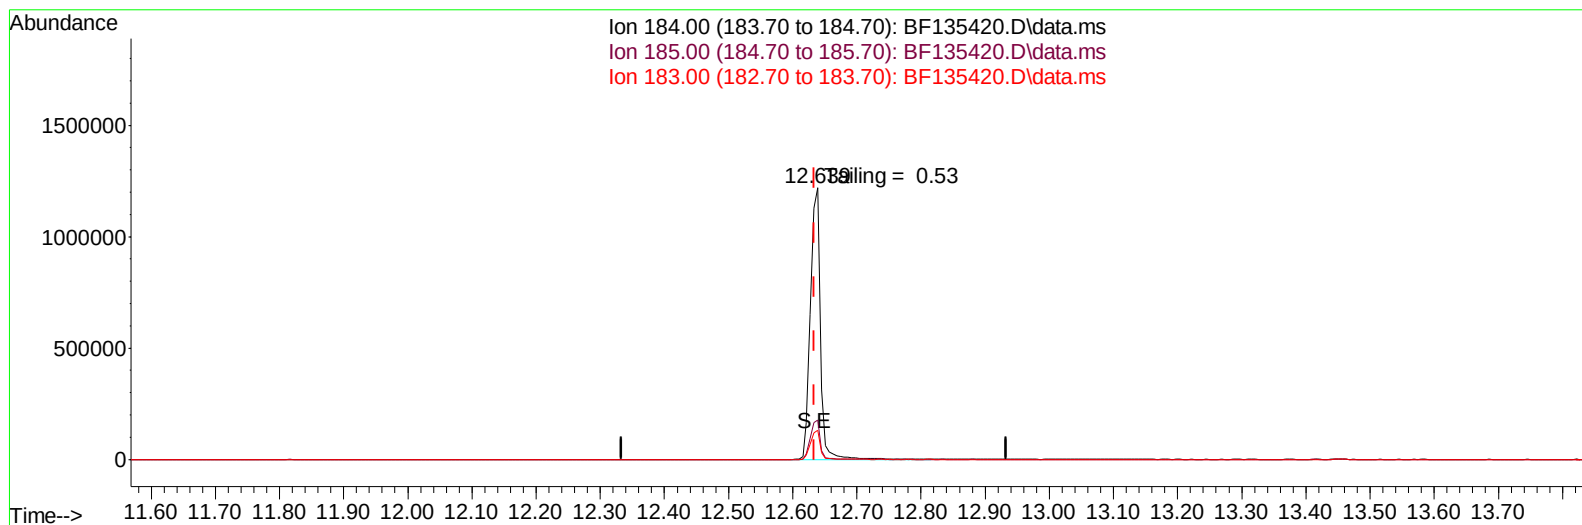

TIC: BF135420.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 157840.94 ng

response 1316100

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.50
183.00	10.30	10.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2023	BNA_F	<u>BF135420.D</u>
Compound Name	Response	Retention Time
DDT	505855	13.457
DDD	15712	13.157
DDE	899	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16611	522466	3.18

Instrument :
BNA_F
ClientSampleId :
DFTPP