
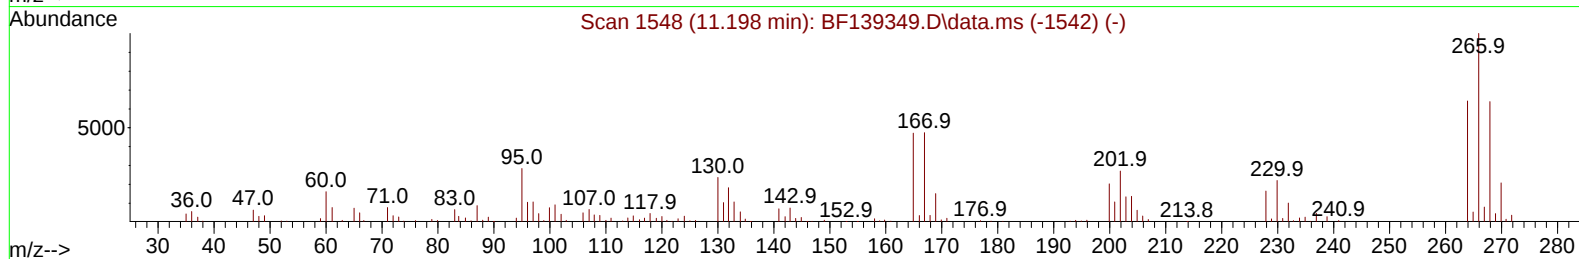
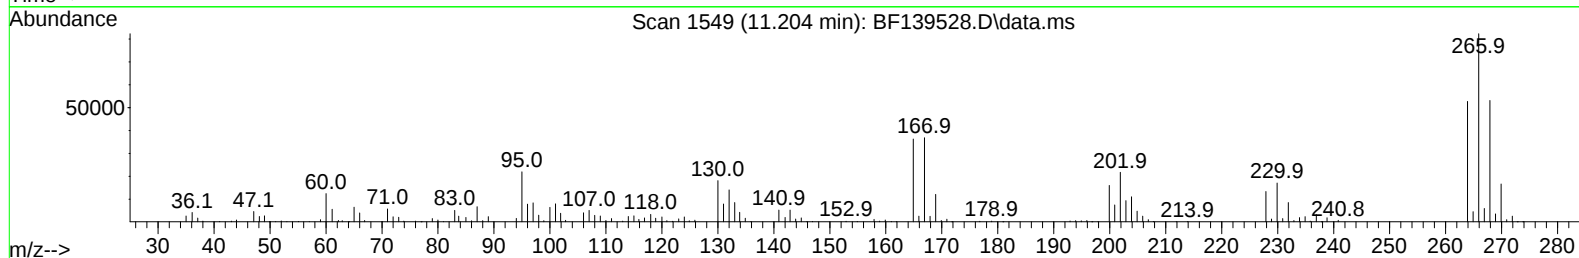


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092524\
Data File : BF139528.D
Acq On : 25 Sep 2024 14:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 15:16:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

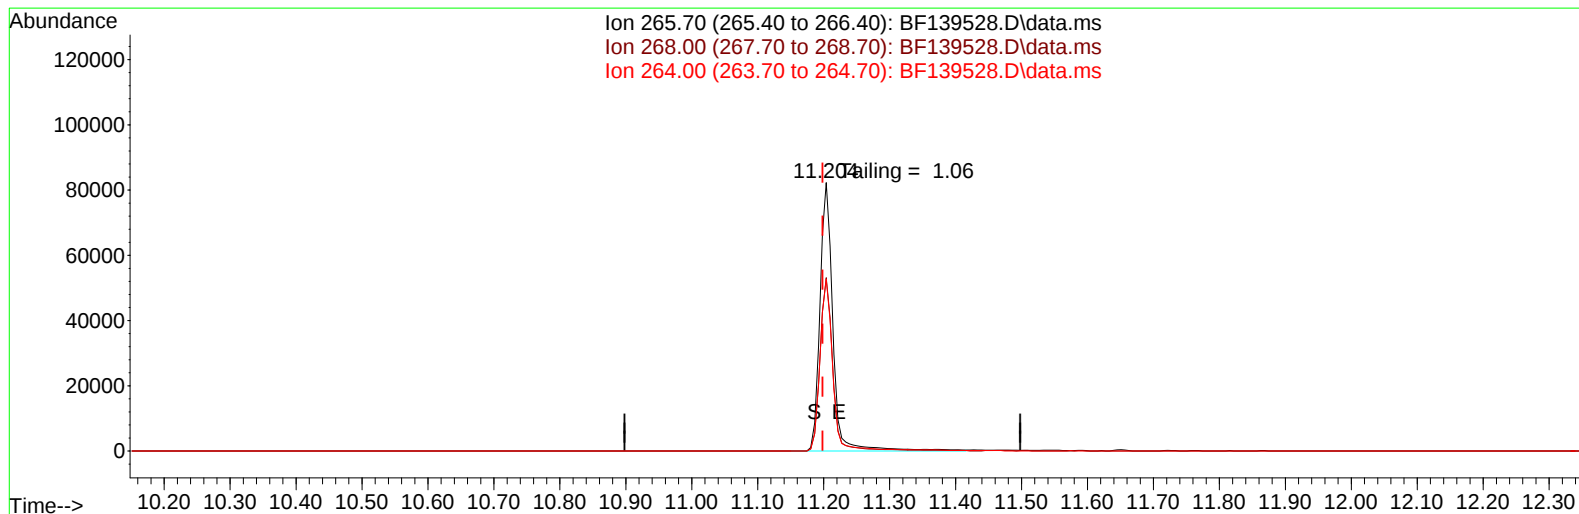

TIC: BF139528.D\data.ms

(70) Pentachlorophenol (C)




11.204min (+ 0.006) 34972.97 ng

response 112270

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.60
264.00	64.20	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092524\
Data File : BF139528.D
Acq On : 25 Sep 2024 14:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 15:16:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

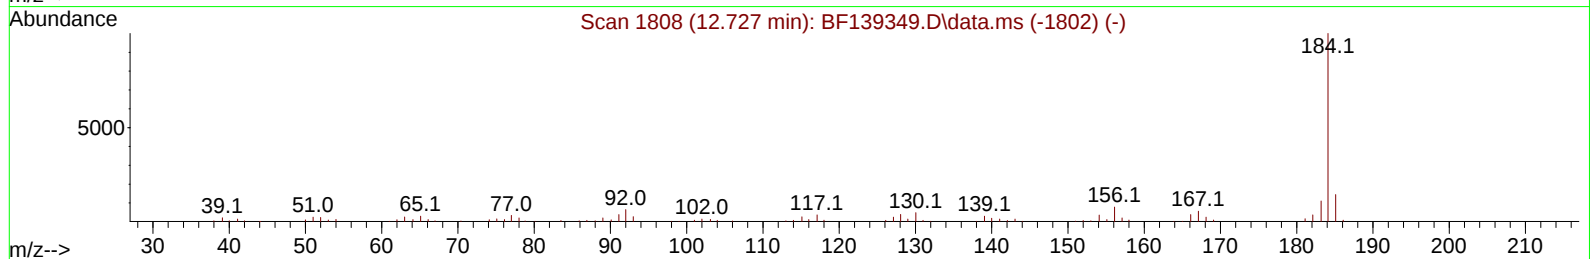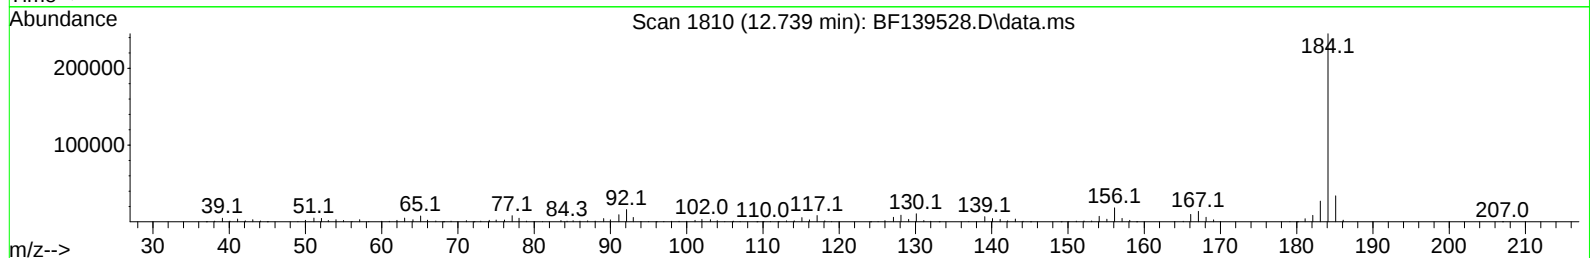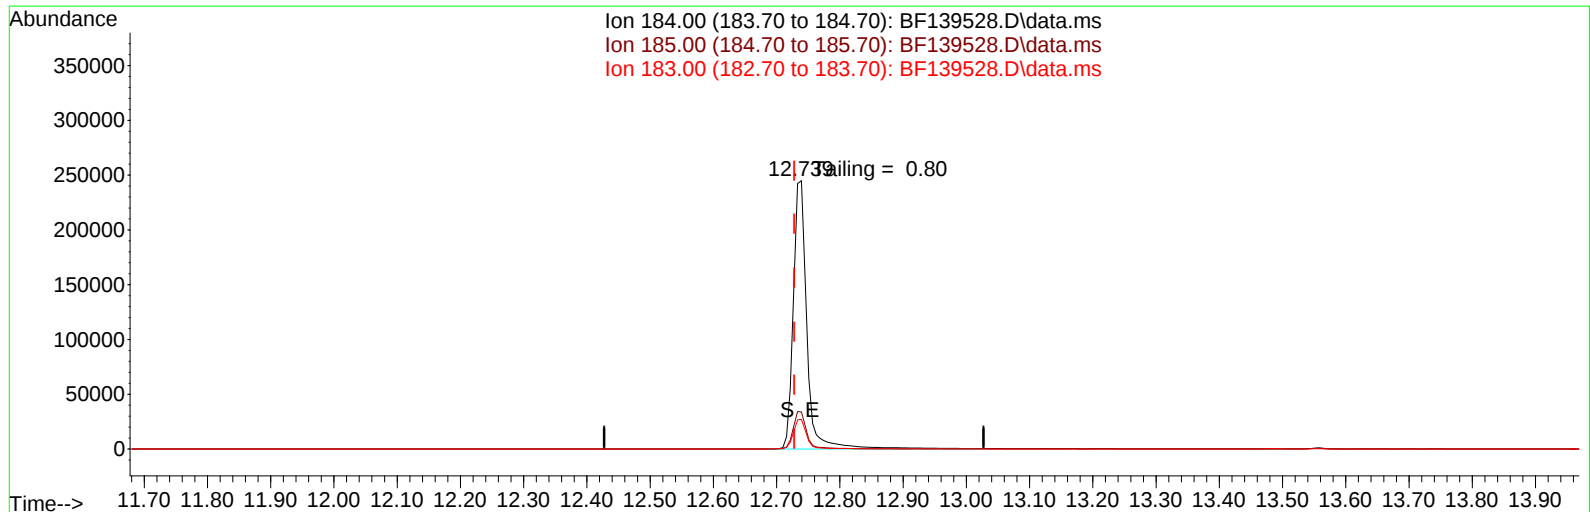

TIC: BF139528.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 0.00 ng

response 367549

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	11.10	11.04
0.00	0.00	0.00