


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092524\
Data File : BF139528.D
Acq On : 25 Sep 2024 14:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

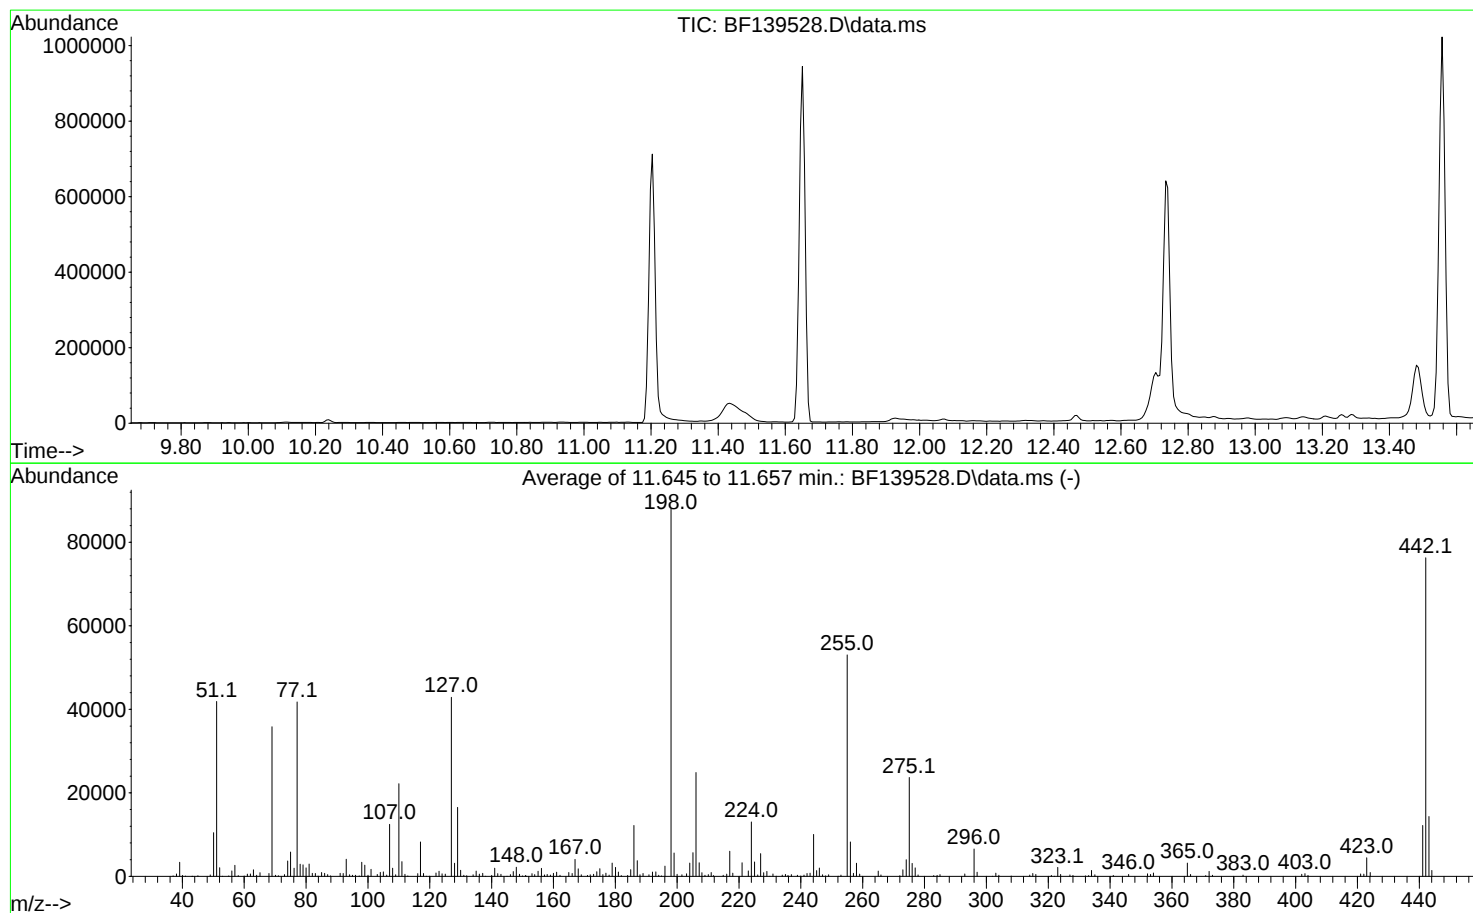




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	41893	PASS
68	69	0.00	2	1.9	692	PASS
69	198	0.00	100	40.7	35827	PASS
70	69	0.00	2	0.7	266	PASS
127	198	10	80	48.7	42891	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88096	PASS
199	198	5	9	6.3	5594	PASS
275	198	10	60	26.9	23677	PASS
365	198	1	100	3.6	3173	PASS
441	198	0.01	100	13.8	12192	PASS
442	442	50	100	100.0	76291	PASS
443	442	15	24	18.8	14337	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092524\
Data File : BF139528.D
Acq On : 25 Sep 2024 14:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 25 15:16:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

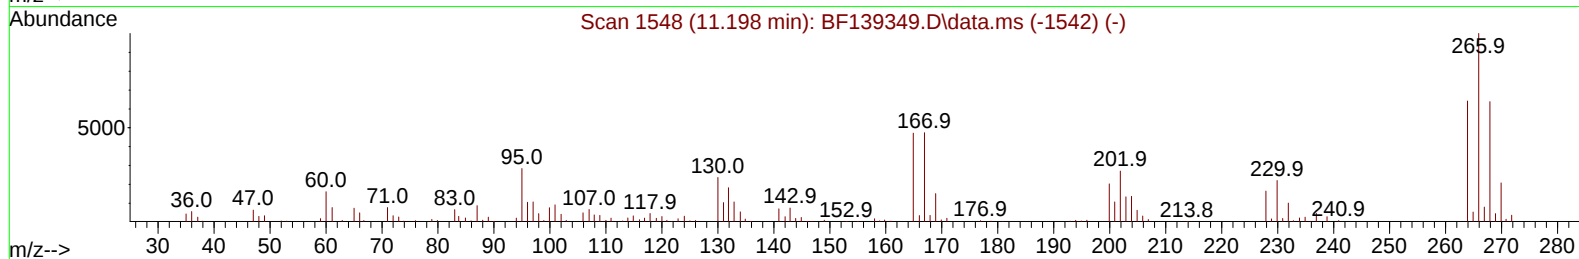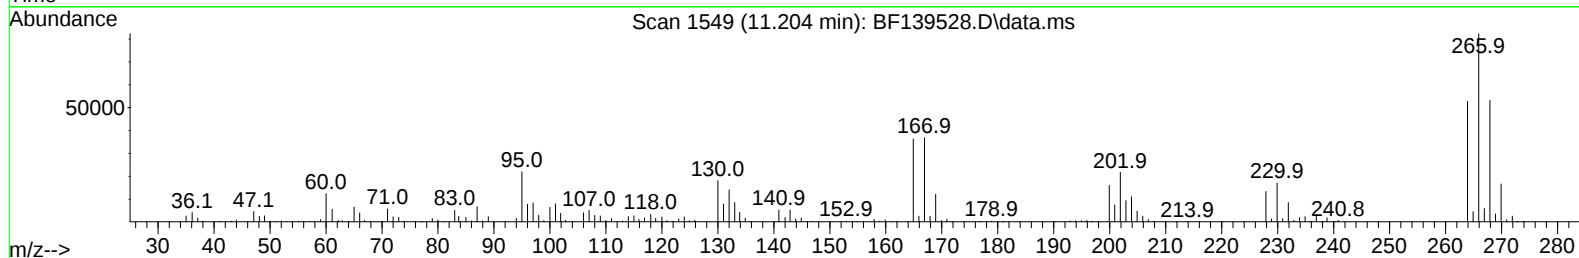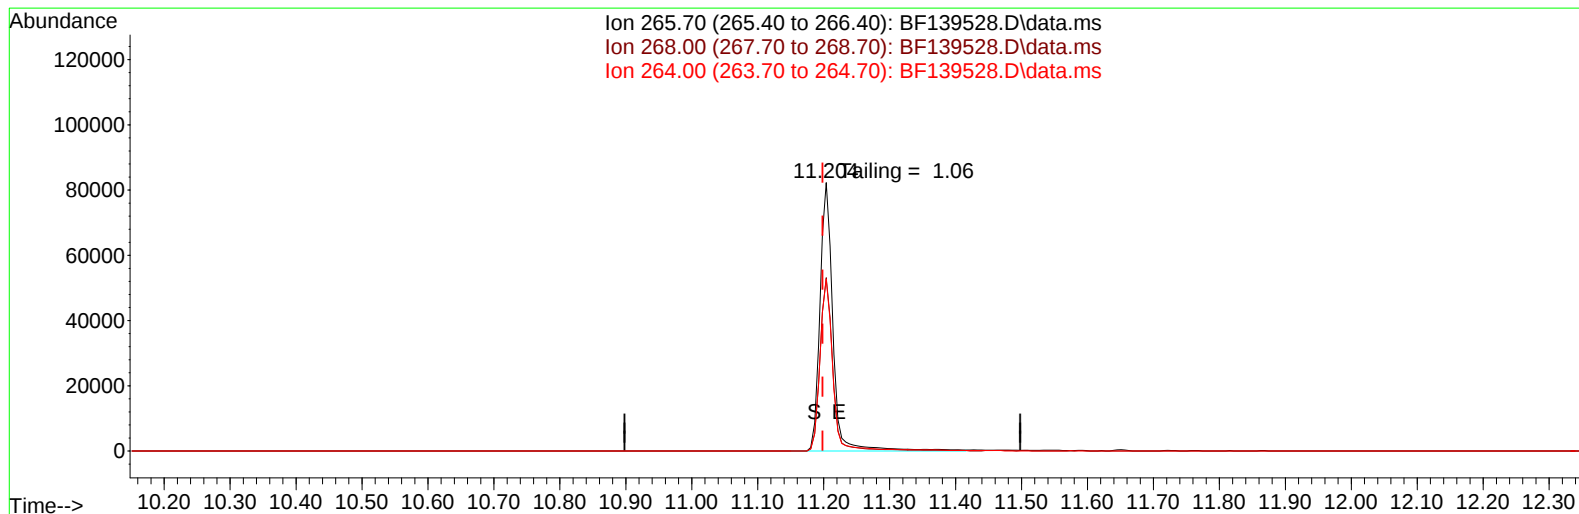

TIC: BF139528.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 34972.97 ng




response 112270

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.60
264.00	64.20	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092524\
Data File : BF139528.D
Acq On : 25 Sep 2024 14:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 25 15:16:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

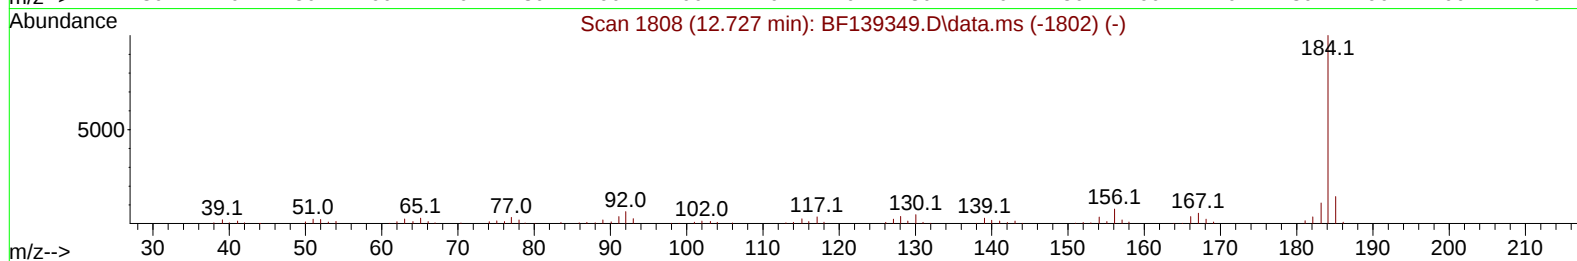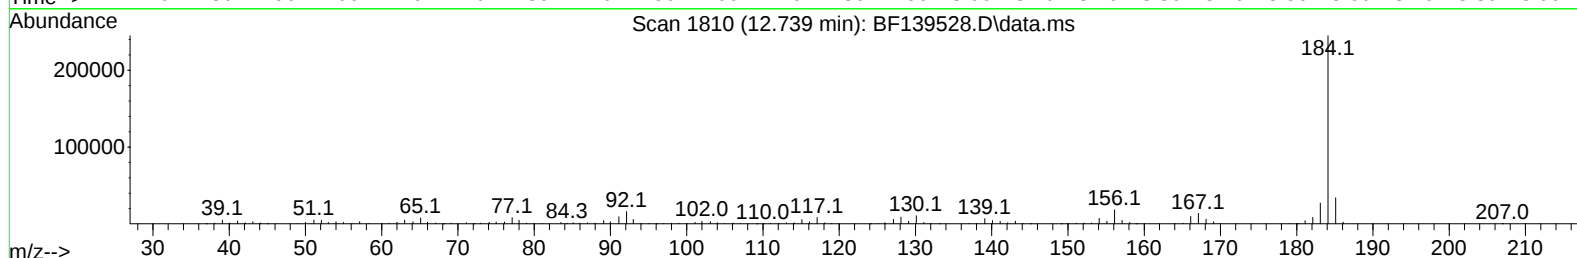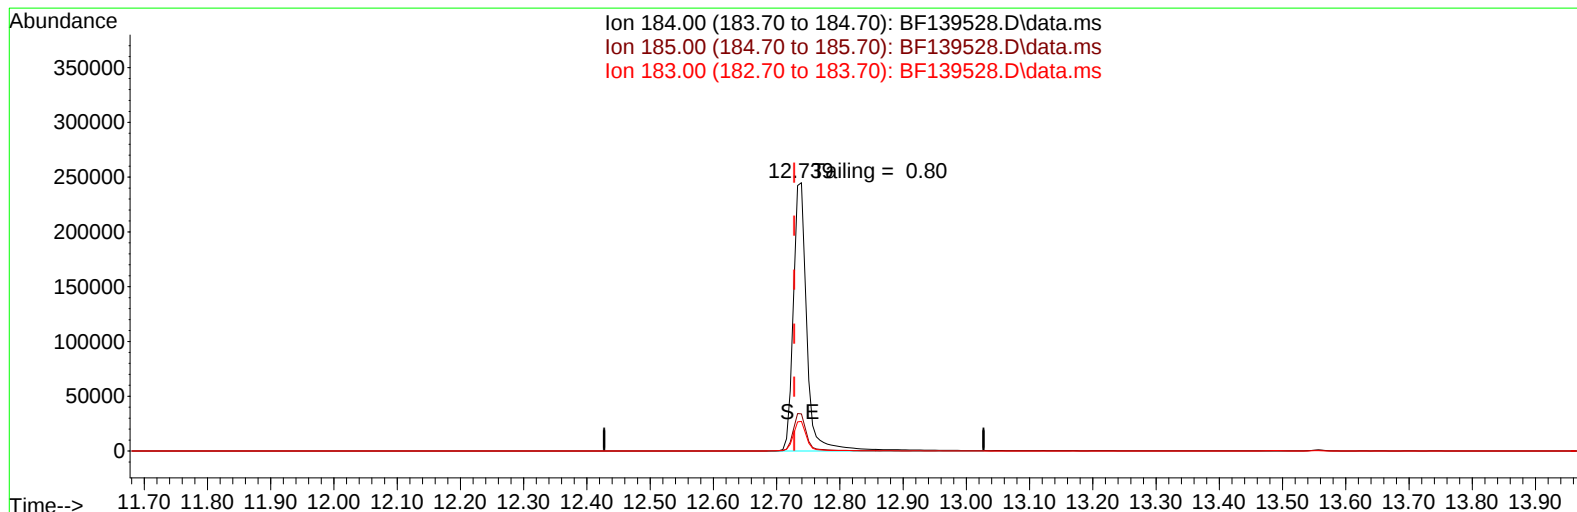

TIC: BF139528.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 0.00 ng

response 367549

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.87
183.00	11.10	11.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/25/2024	BNA_F	<u>BF139528.D</u>
Compound Name	Response	Retention Time
DDT	236587	13.557
DDD	6226	13.257
DDE	208	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6434	243021	2.65

Instrument :
BNA_F
ClientSampleId :
DFTPP