
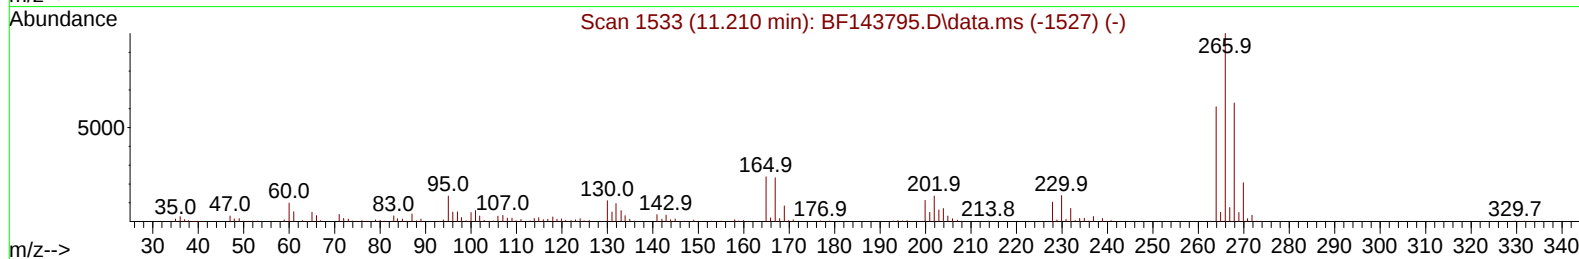
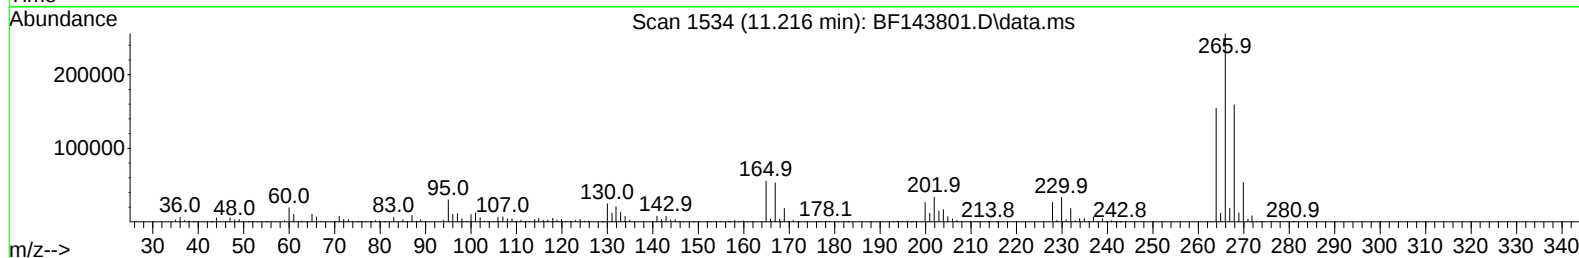


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092525\
Data File : BF143801.D
Acq On : 25 Sep 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 12:28:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 05:00:00 2025
Response via : Initial Calibration

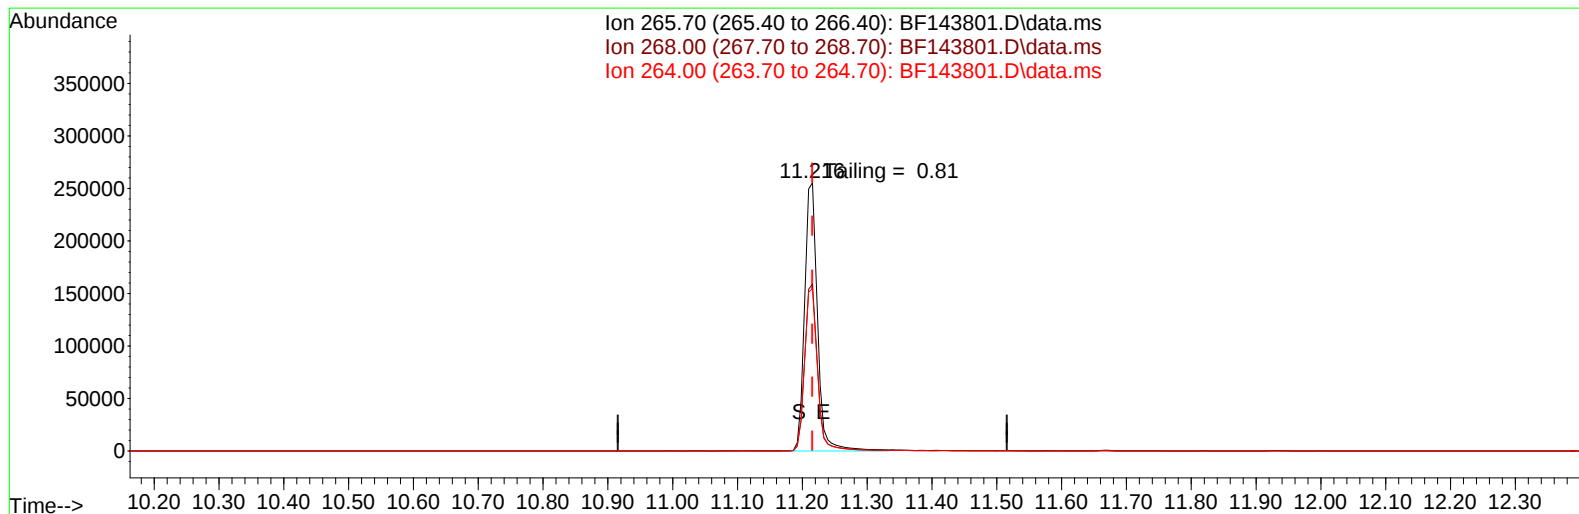

TIC: BF143801.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.000) 38670.72 ng

response 355330

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.16
264.00	61.00	60.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092525\
Data File : BF143801.D
Acq On : 25 Sep 2025 12:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 25 12:28:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 24 05:00:00 2025
Response via : Initial Calibration

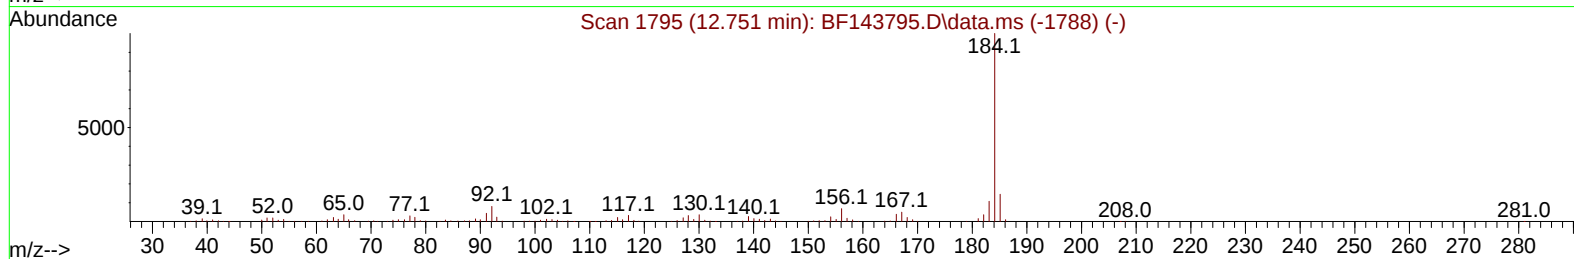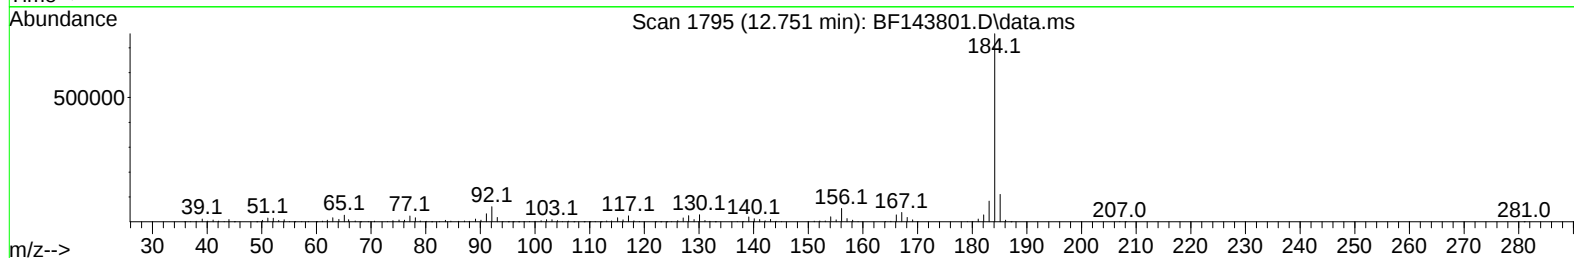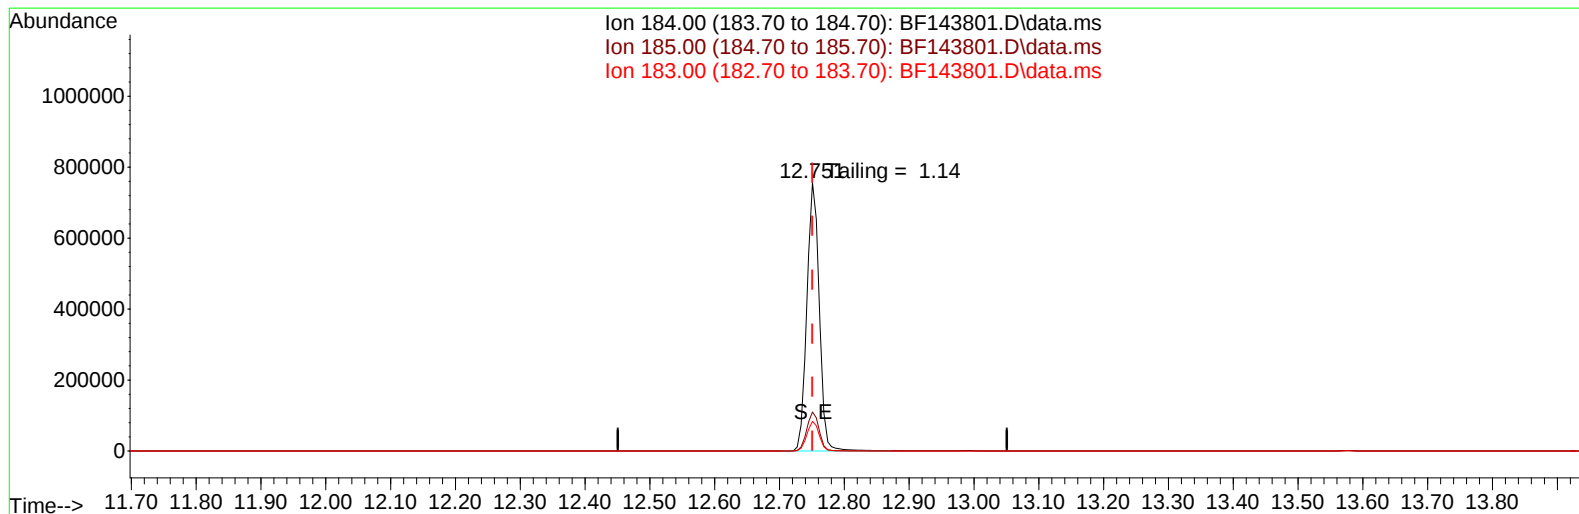

TIC: BF143801.D\data.ms

(77) Benzidine

12.751min (0.000) 5496.52 ng

response 1007617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.54
183.00	10.80	11.02
0.00	0.00	0.00