


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092525\  
Data File : BF143801.D  
Acq On : 25 Sep 2025 12:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF092325.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Sep 24 05:00:00 2025

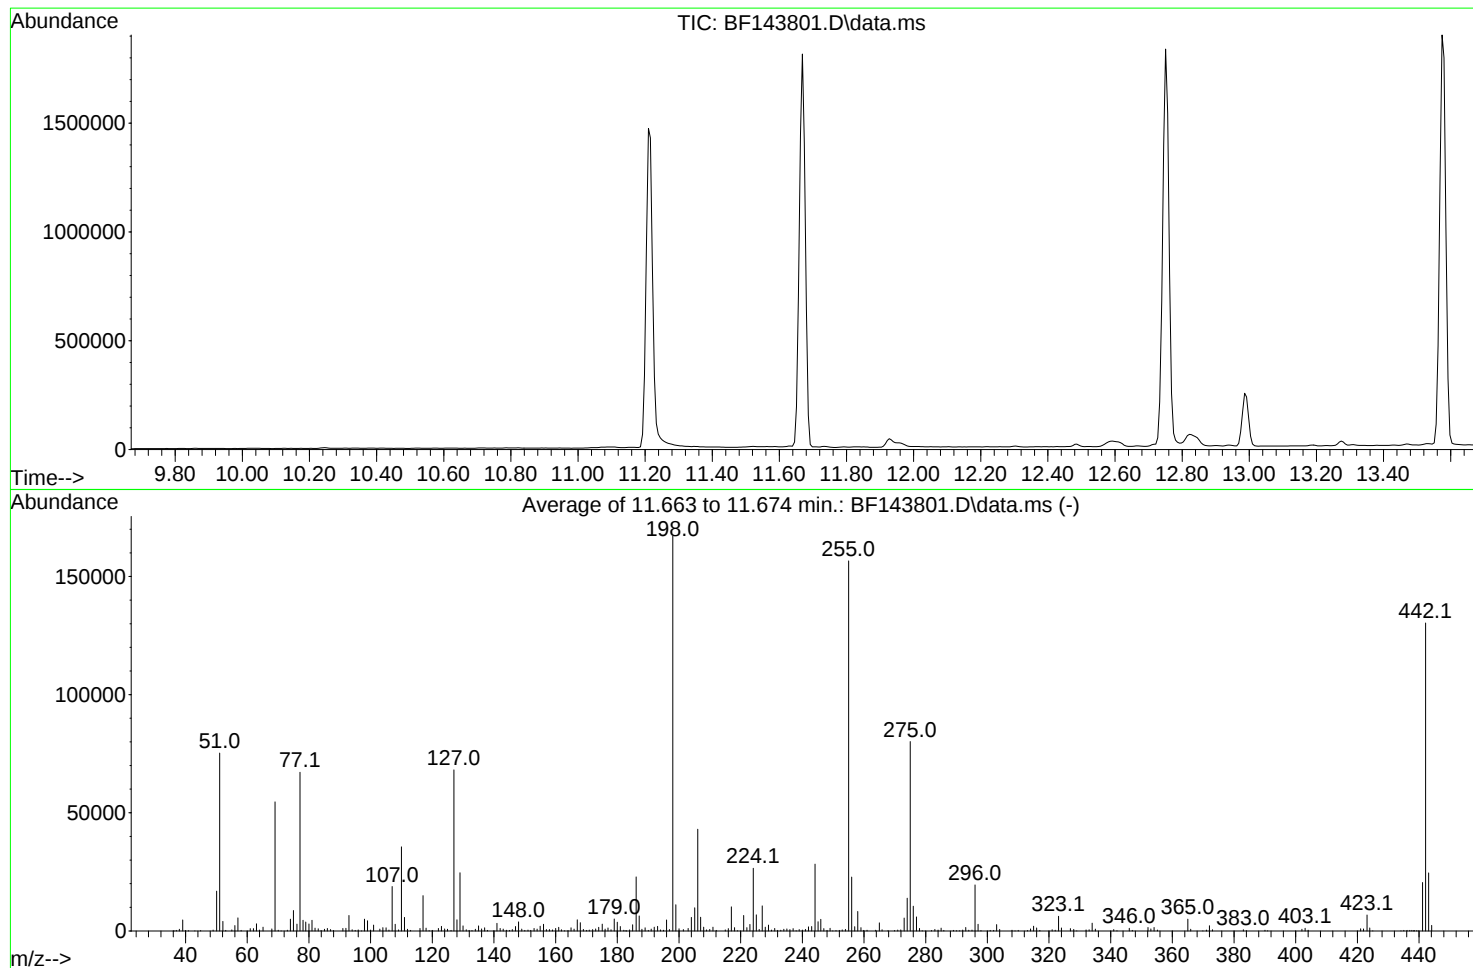




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.5   | 818    | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 54649  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.5   | 280    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.3   | 572    | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 167104 | PASS      |
| 199    | 198     | 5      | 9      | 6.6   | 11091  | PASS      |
| 365    | 198     | 1      | 100    | 3.0   | 4982   | PASS      |
| 441    | 443     | 0.01   | 150    | 83.4  | 20469  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 130317 | PASS      |
| 443    | 442     | 15     | 24     | 18.8  | 24531  | PASS      |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092525\  
Data File : BF143801.D  
Acq On : 25 Sep 2025 12:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 25 12:28:08 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF092325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 24 05:00:00 2025  
Response via : Initial Calibration

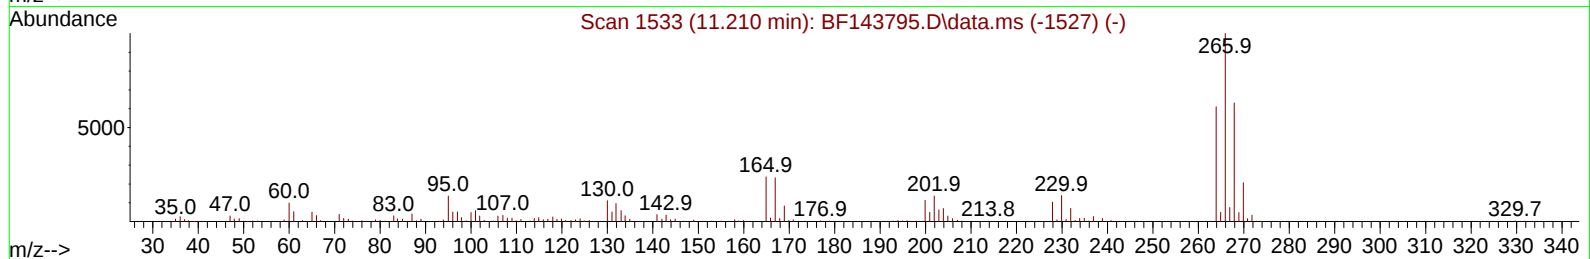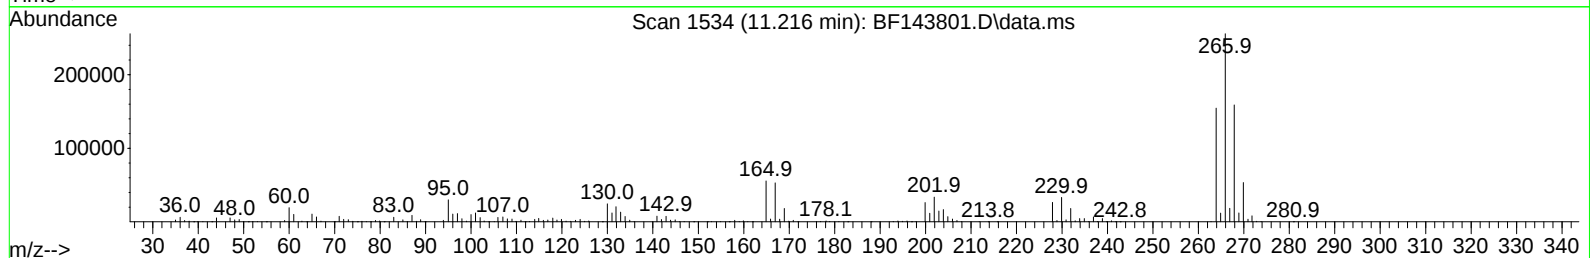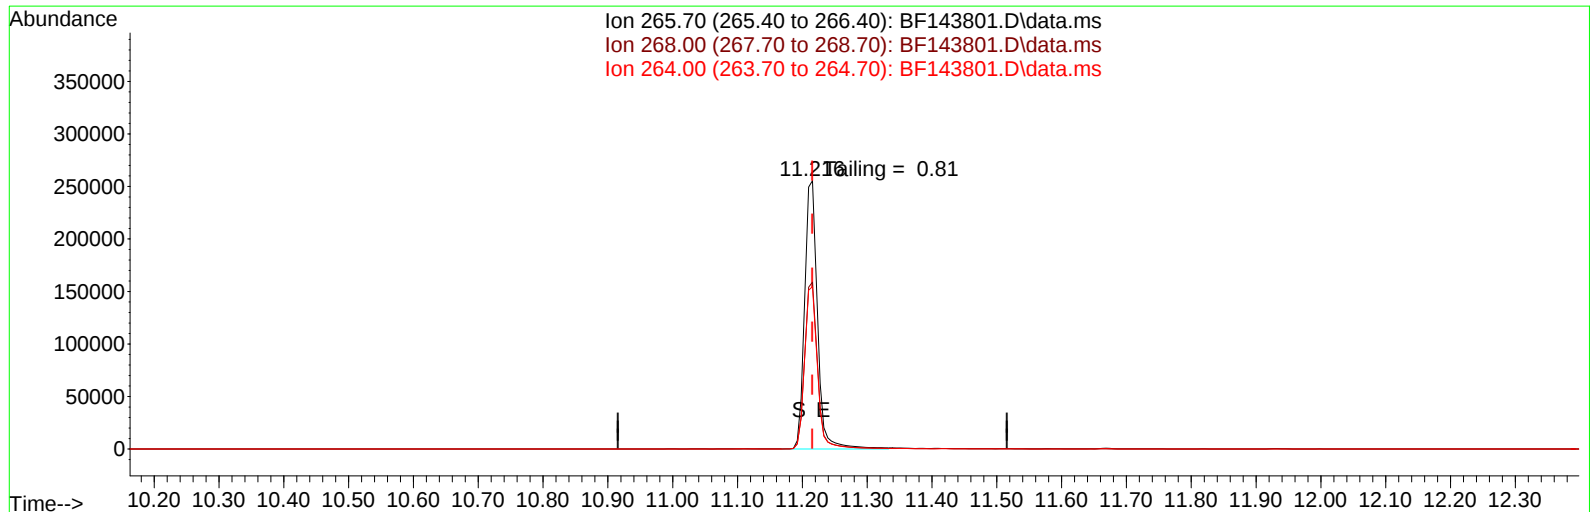

TIC: BF143801.D\data.ms

**(70) Pentachlorophenol (C)**

**11.216min (-0.000) 38670.72 ng**




**response 355330**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 62.16  |
| 264.00 | 61.00  | 60.46  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092525\  
Data File : BF143801.D  
Acq On : 25 Sep 2025 12:03  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 25 12:28:08 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF092325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 24 05:00:00 2025  
Response via : Initial Calibration

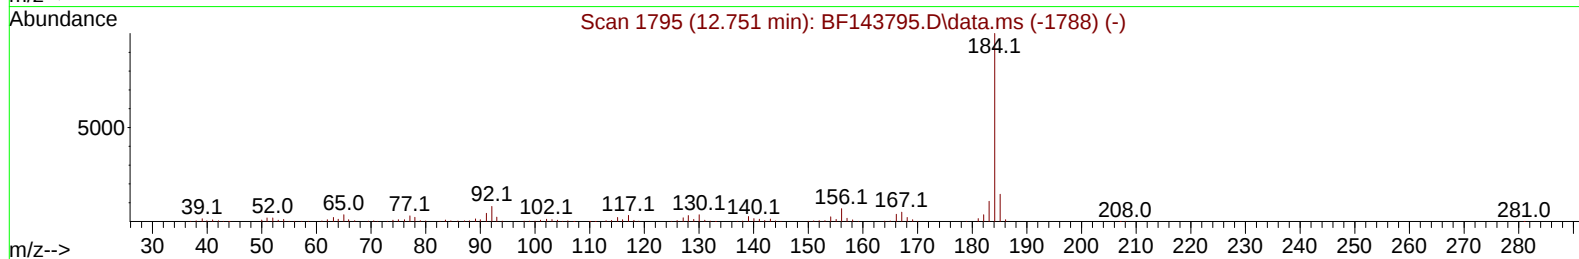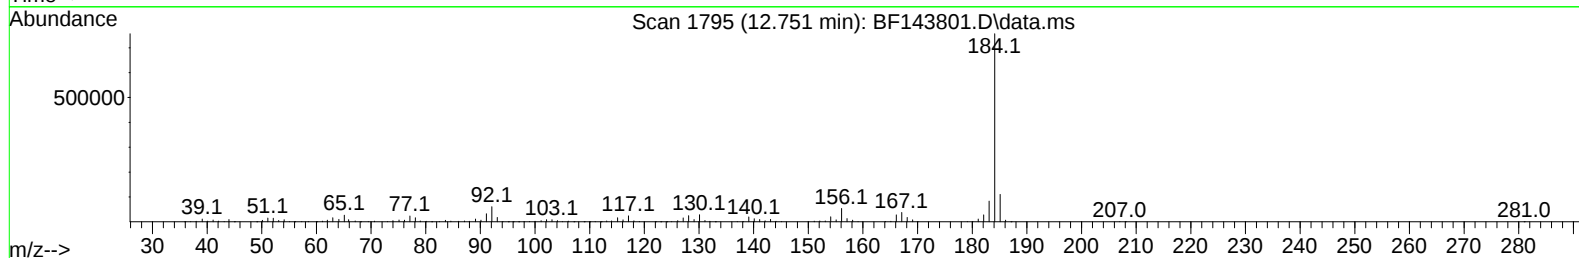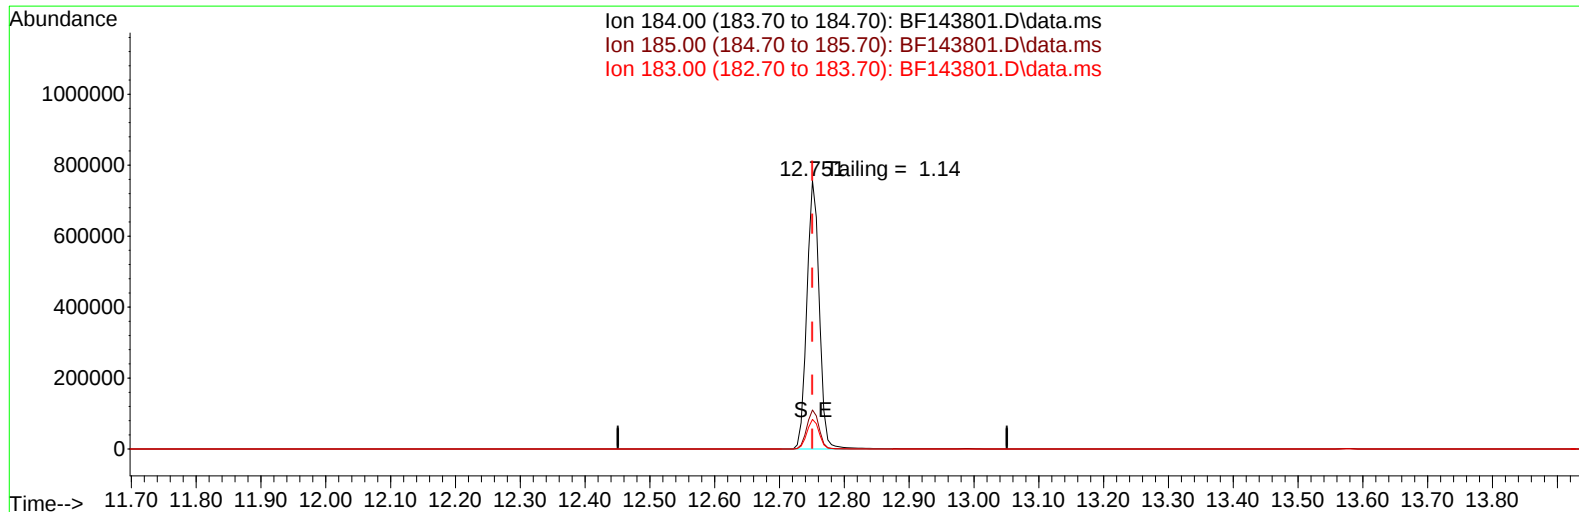

TIC: BF143801.D\data.ms

(77) Benzidine

12.751min ( 0.000) 5496.52 ng

response 1007617

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 14.54  |
| 183.00 | 10.80  | 11.02  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/25/2025     | BNA_F            | <u>BF143801.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 502047           | 13.574             |
| DDD           | 7723             | 13.274             |
| DDE           | 1204             | 12.939             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 8927          | 510974           | 1.75               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP