
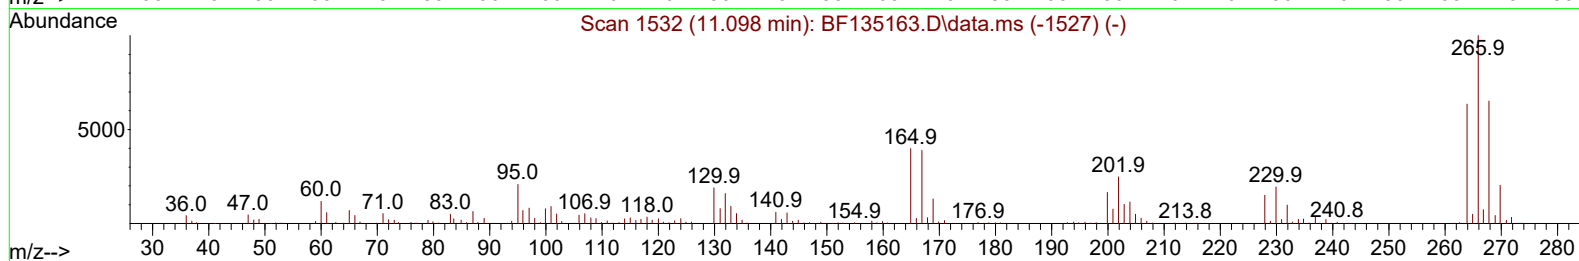
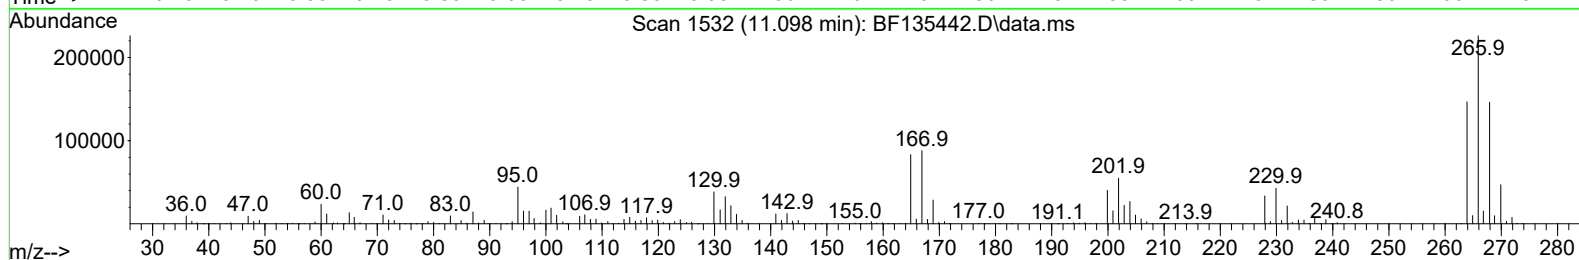


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135442.D
Acq On : 26 Sep 2023 09:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 12:39:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration

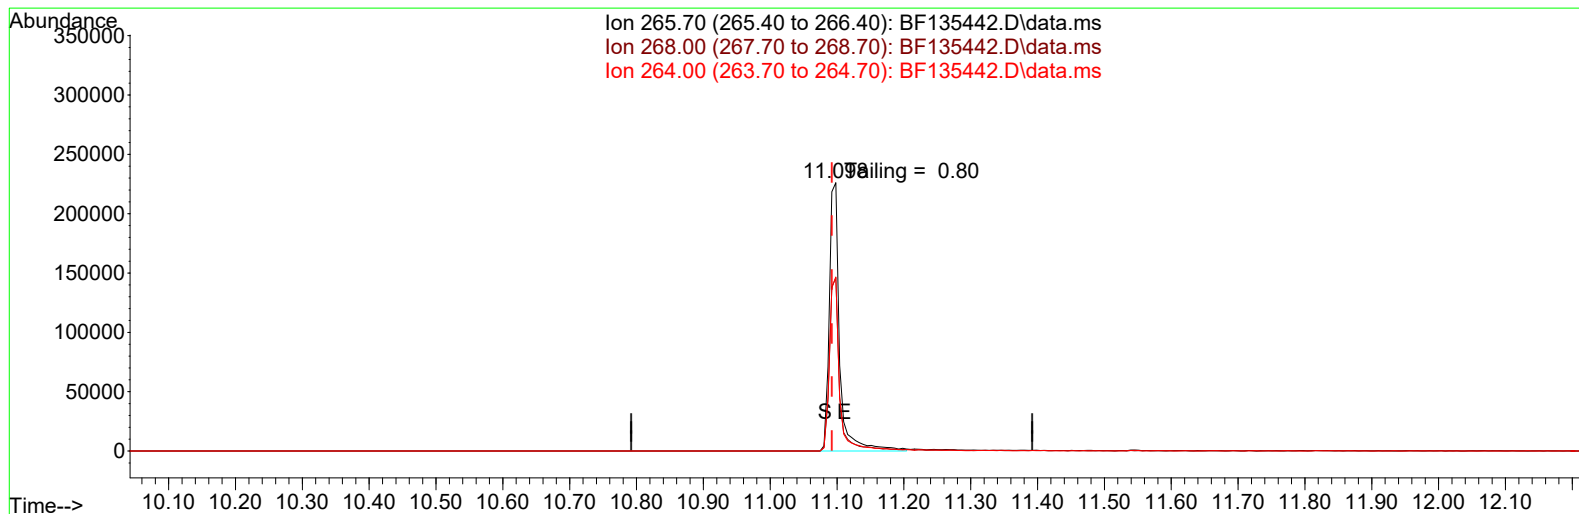

TIC: BF135442.D\data.ms

(70) Pentachlorophenol (C)




11.098min (+ 0.006) 39240.00 ng

response 246683

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.60
264.00	63.50	64.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
 Data File : BF135442.D
 Acq On : 26 Sep 2023 09:42
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 12:39:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 26 01:36:36 2023
 Response via : Initial Calibration

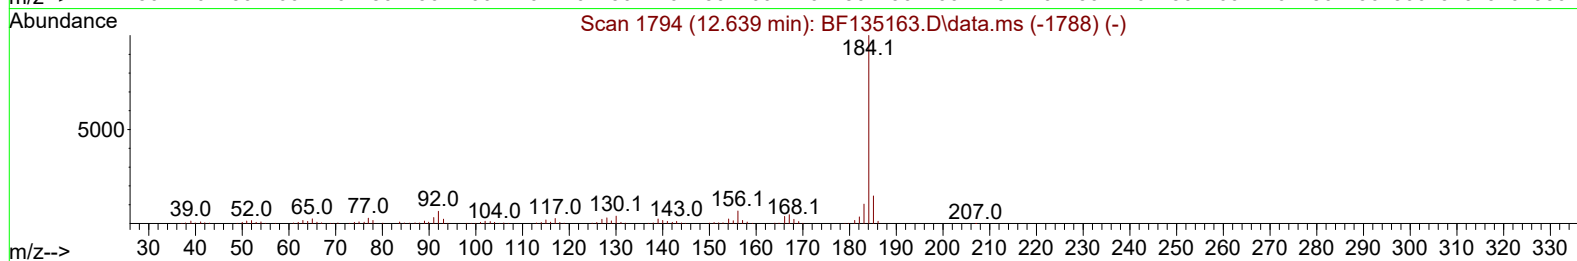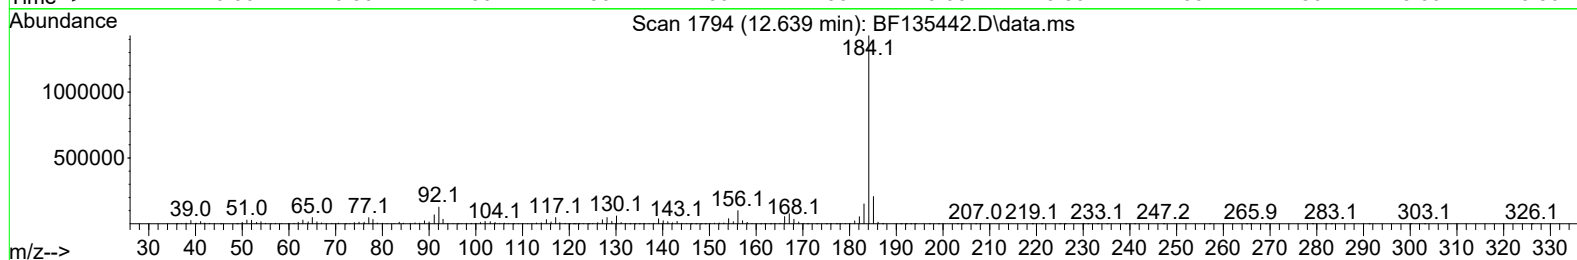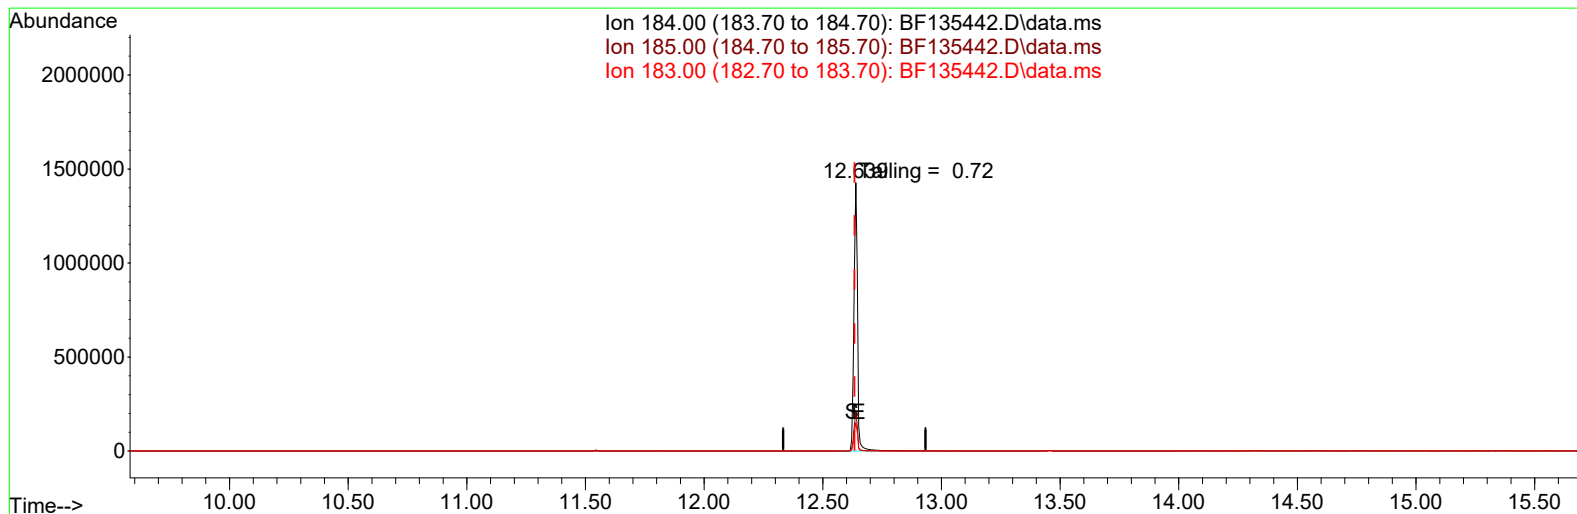

TIC: BF135442.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 133266.40 ng m

response 1427898

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.50
183.00	10.30	10.56
0.00	0.00	0.00