

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
 Data File : BF135457.D
 Acq On : 26 Sep 2023 17:26
 Operator : CG\JU
 Sample : 04531-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-BCD

Quant Time: Sep 27 02:47:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 26 01:36:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.757	152	164122	20.000	ng	0.00
21) Naphthalene-d8	8.034	136	611744	20.000	ng	0.00
39) Acenaphthene-d10	9.786	164	282573	20.000	ng	0.00
64) Phenanthrene-d10	11.280	188	429732	20.000	ng	# 0.00
76) Chrysene-d12	13.939	240	297967	20.000	ng	0.00
86) Perylene-d12	15.404	264	330151	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.404	112	1214678	120.374	ng	0.02
7) Phenol-d6	6.404	99	1490284	116.146	ng	0.00
23) Nitrobenzene-d5	7.322	82	1001168	88.914	ng	0.00
42) 2,4,6-Tribromophenol	10.586	330	302105	107.584	ng	0.00
45) 2-Fluorobiphenyl	9.110	172	1631611	87.115	ng	0.00
79) Terphenyl-d14	12.880	244	1264032	65.762	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135457.D
Acq On : 26 Sep 2023 17:26
Operator : CG\JU
Sample : 04531-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-BCD

Quant Time: Sep 27 02:47:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration




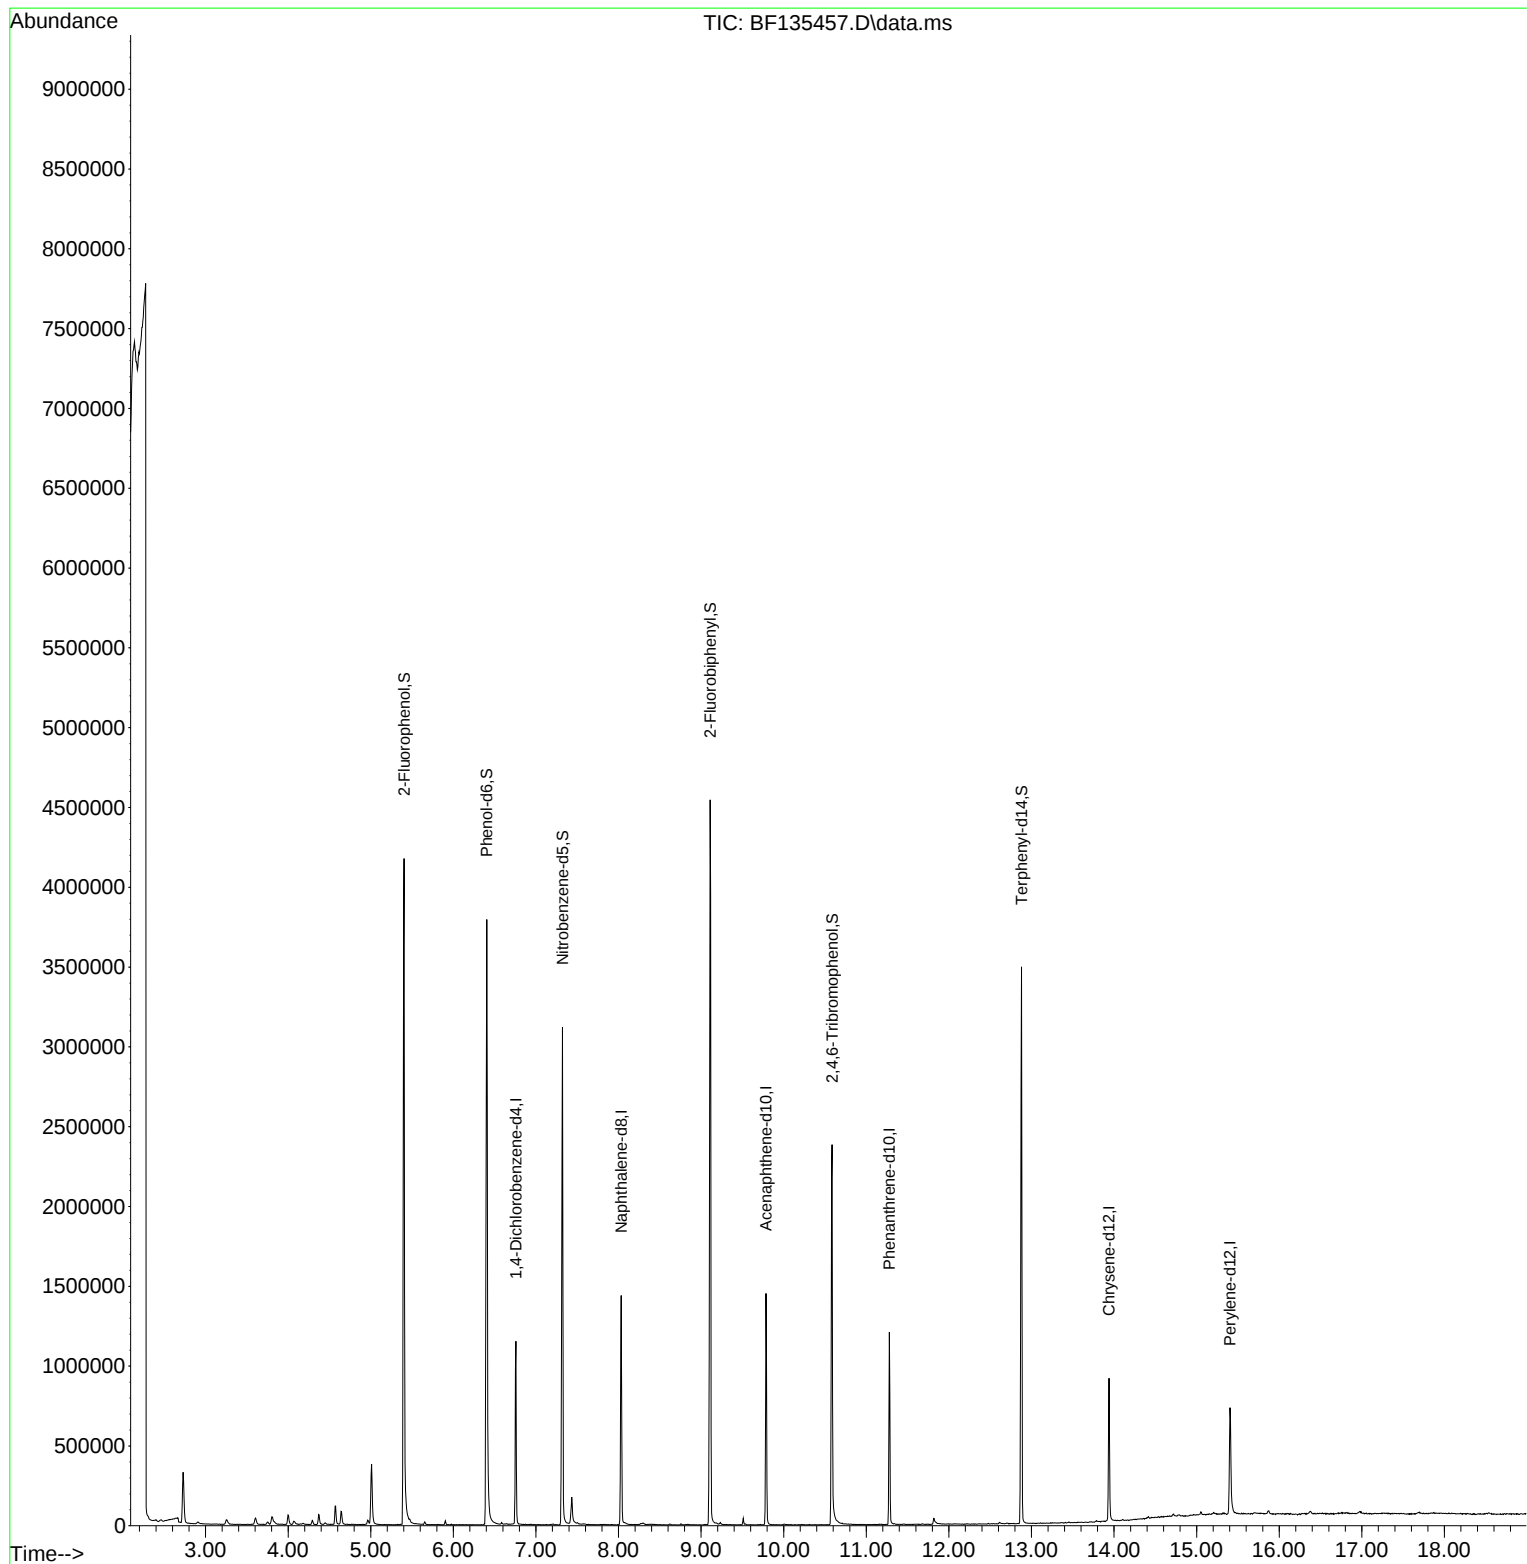




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.757 min Scan# 795
Delta R.T. 0.006 min
Lab File: BF135457.D
Acq: 26 Sep 2023 17:26




Instrument :
BNA_F
ClientSampleId :
TP-BCD


Tgt Ion:152 Resp: 164122
Ion Ratio Lower Upper
152 100
150 151.4 127.8 191.6
115 57.5 49.8 74.8

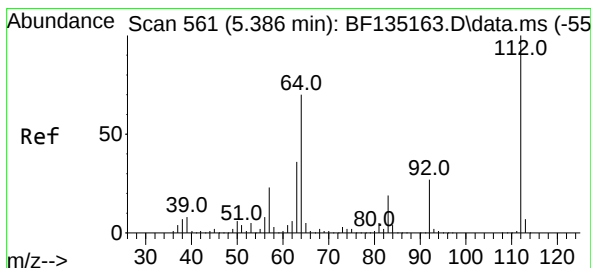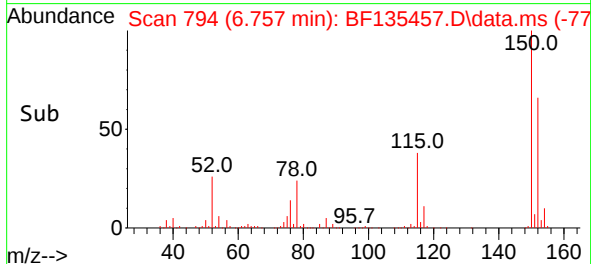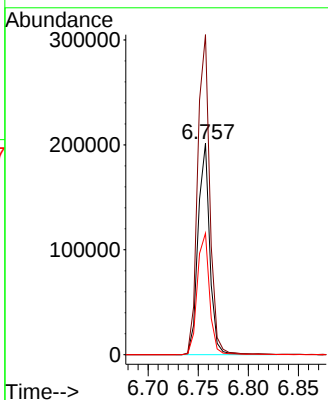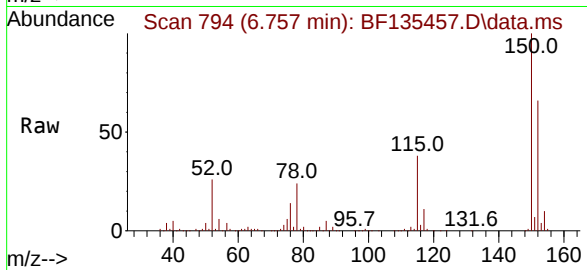

#5
2-Fluorophenol
Concen: 120.374 ng
RT: 5.404 min Scan# 564
Delta R.T. 0.023 min
Lab File: BF135457.D
Acq: 26 Sep 2023 17:26

Tgt Ion:112 Resp: 1214678
Ion Ratio Lower Upper
112 100
64 65.6 55.9 83.9
63 33.6 29.0 43.6

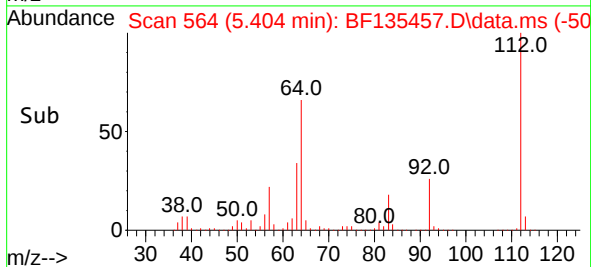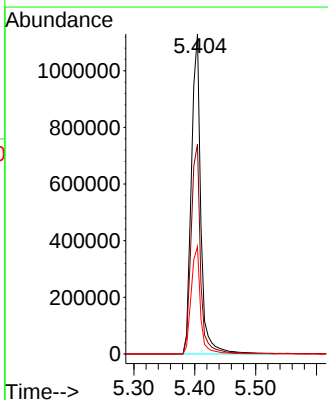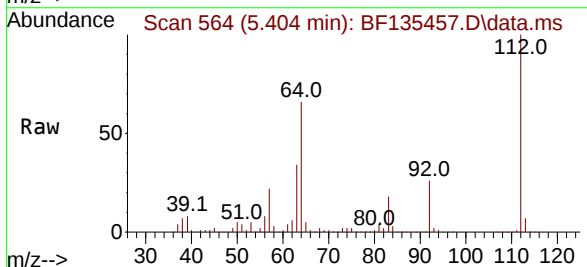




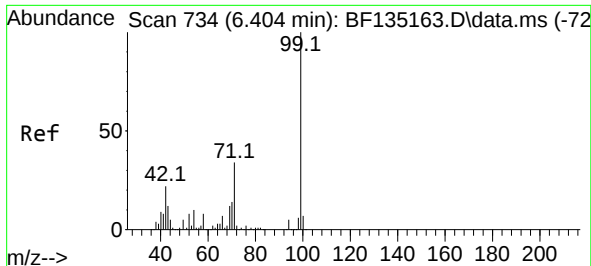


#7
Phenol-d6
Concen: 116.146 ng
RT: 6.404 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF135457.D
Acq: 26 Sep 2023 17:26

Instrument :
BNA_F
ClientSampleId :
TP-BCD

Tgt Ion: 99 Resp: 1490284




Ion	Ratio	Lower	Upper
99	100		
42	22.9	17.9	26.9
71	32.0	27.0	40.6

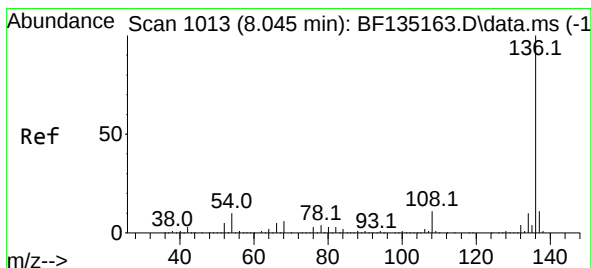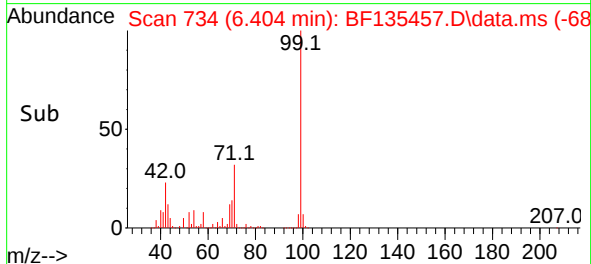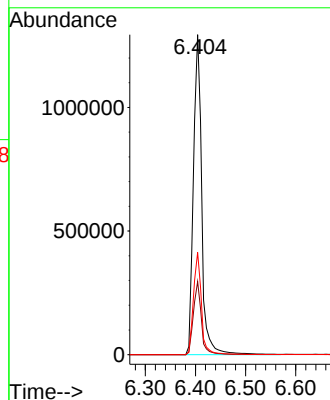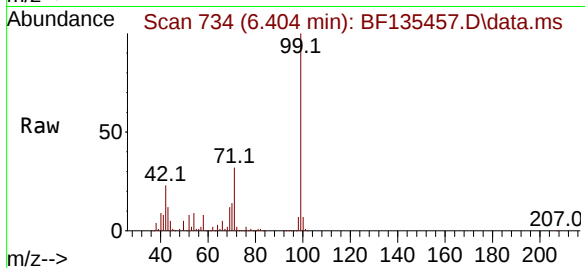

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.034 min Scan# 1011
Delta R.T. -0.000 min
Lab File: BF135457.D
Acq: 26 Sep 2023 17:26

Tgt Ion: 136 Resp: 611744

Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.8	13.2
54	9.8	7.7	11.5
68	6.8	4.6	6.8

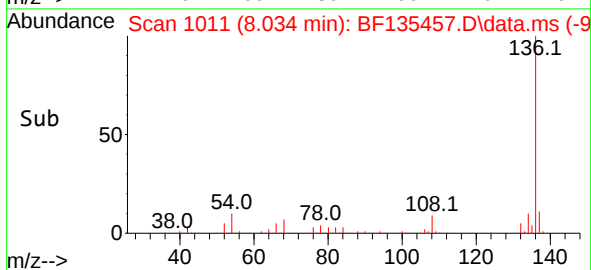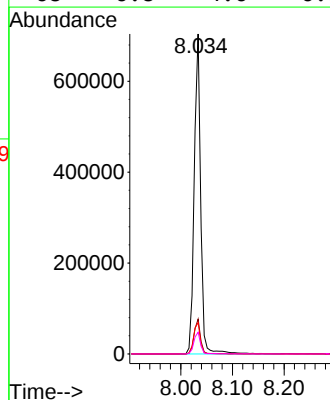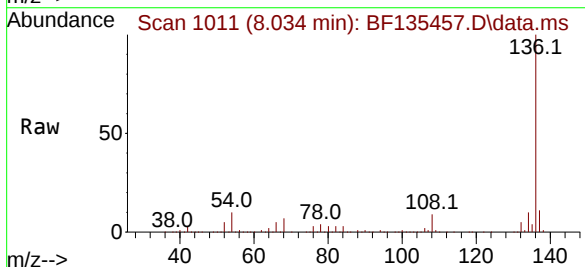



#23

Nitrobenzene-d5

Concen: 88.914 ng

RT: 7.322 min Scan# 89

Delta R.T. -0.000 min

Lab File: BF135457.D

Acq: 26 Sep 2023 17:26

Instrument :

BNA_F

ClientSampleId :

TP-BCD





Tgt Ion: 82 Resp: 1001168

Ion Ratio Lower Upper

82 100

128 45.3 35.8 53.6

54 64.8 50.6 76.0

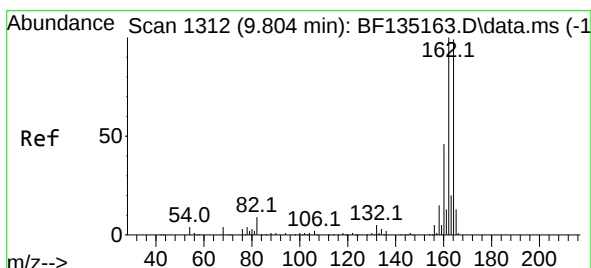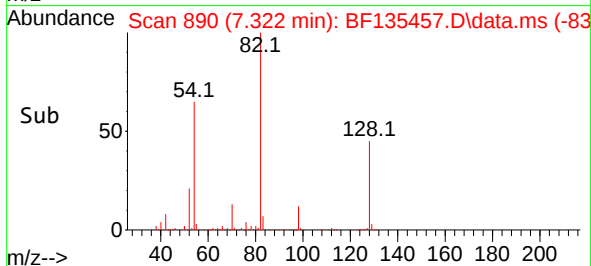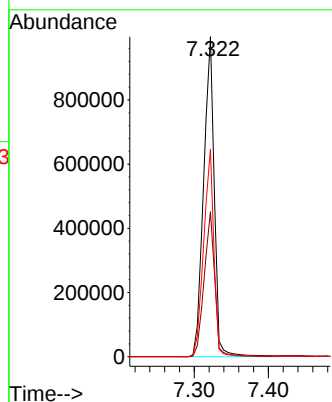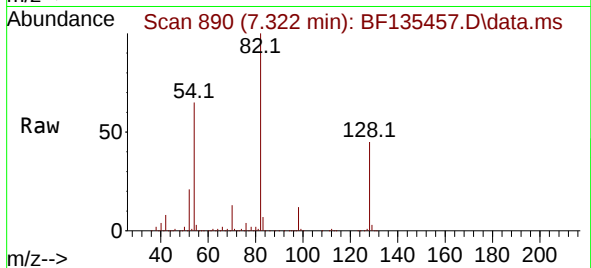

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.786 min Scan# 1309

Delta R.T. -0.006 min

Lab File: BF135457.D

Acq: 26 Sep 2023 17:26




Tgt Ion: 164 Resp: 282573

Ion Ratio Lower Upper

164 100

162 100.8 81.0 121.4

160 45.3 37.0 55.4

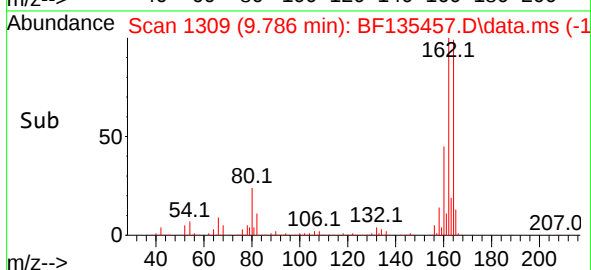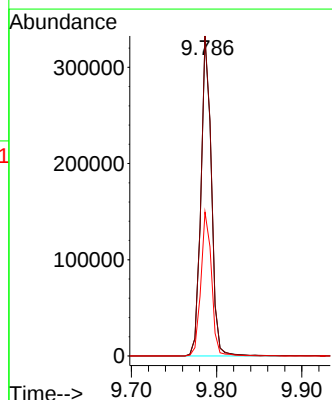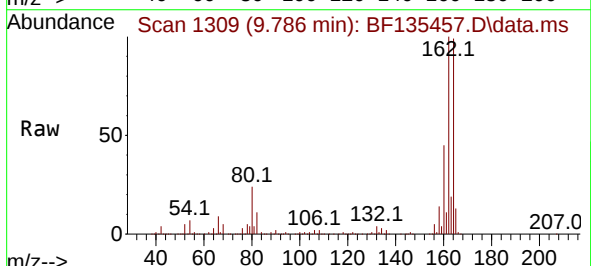



#42

2,4,6-Tribromophenol

Concen: 107.584 ng

RT: 10.586 min Scan# 1445

Delta R.T. -0.000 min

Lab File: BF135457.D

Acq: 26 Sep 2023 17:26

Instrument :

BNA_F

ClientSampleId :

TP-BCD





Tgt Ion:330 Resp: 302105

Ion Ratio Lower Upper

330 100

332 95.1 77.3 115.9

141 34.4 25.8 38.8

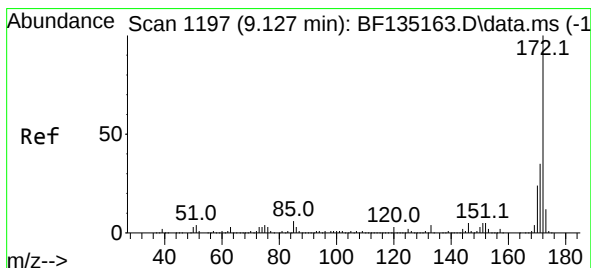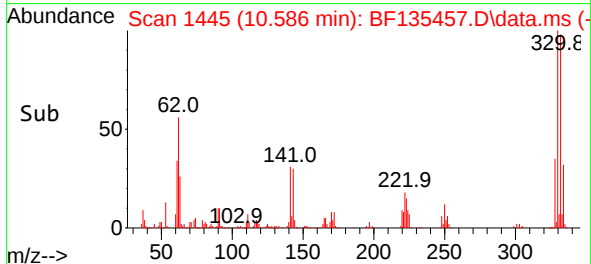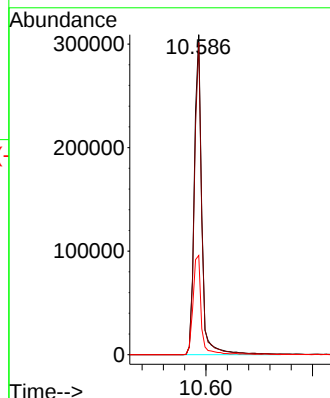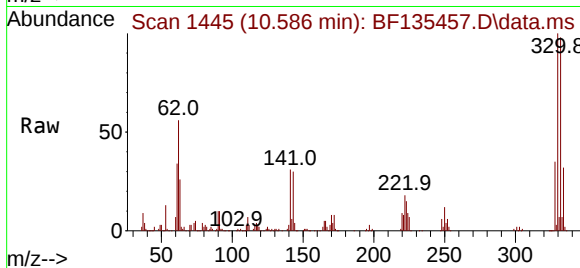

#45

2-Fluorobiphenyl

Concen: 87.115 ng

RT: 9.110 min Scan# 1194

Delta R.T. -0.006 min

Lab File: BF135457.D

Acq: 26 Sep 2023 17:26




Tgt Ion:172 Resp: 1631611

Ion Ratio Lower Upper

172 100

171 35.6 28.4 42.6

170 24.0 19.0 28.4

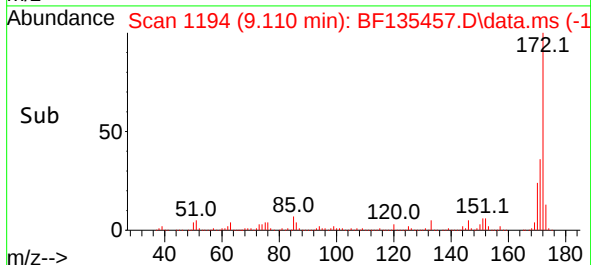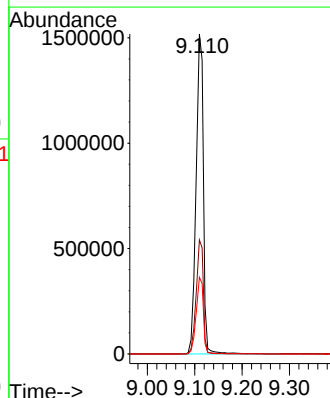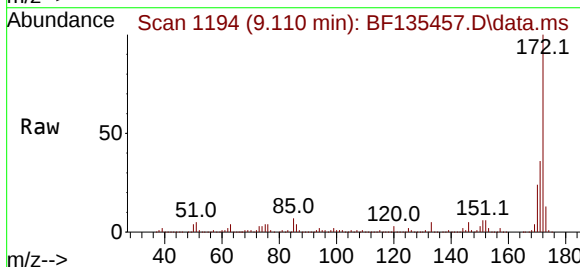



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.280 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF135457.D

Acq: 26 Sep 2023 17:26

Instrument :

BNA_F

ClientSampleId :

TP-BCD





Tgt Ion:188 Resp: 429732

Ion Ratio Lower Upper

188 100

94 10.8 7.0 10.6#

80 11.6 7.5 11.3#

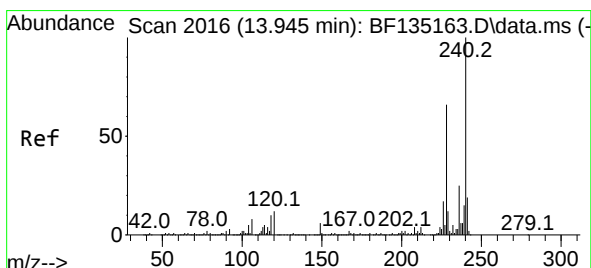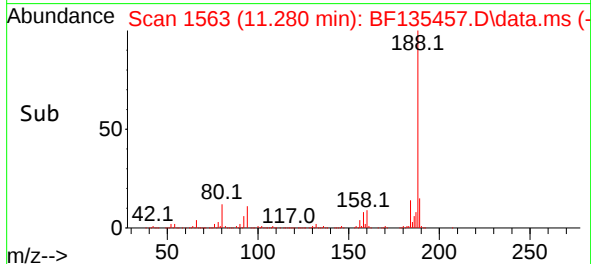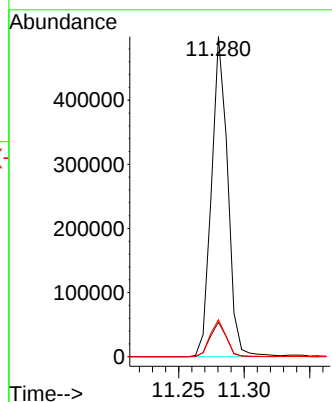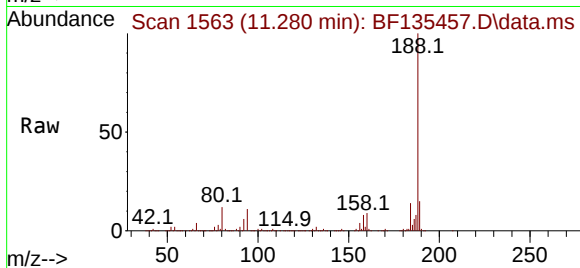

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.939 min Scan# 2015

Delta R.T. -0.006 min

Lab File: BF135457.D

Acq: 26 Sep 2023 17:26




Tgt Ion:240 Resp: 297967

Ion Ratio Lower Upper

240 100

120 12.8 9.4 14.2


236 24.8 19.8 29.8

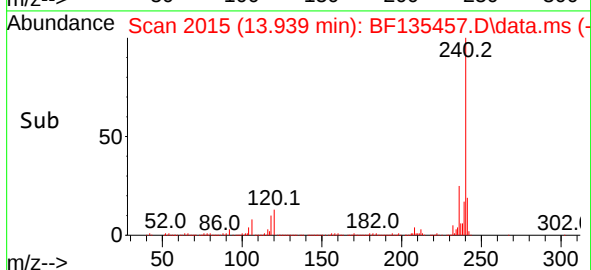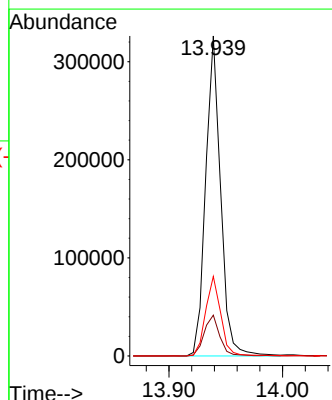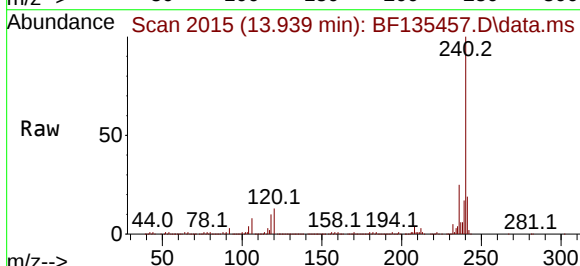






#79
 Terphenyl-d14
 Concen: 65.762 ng
 RT: 12.880 min Scan# 1835
 Delta R.T. -0.000 min
 Lab File: BF135457.D
 Acq: 26 Sep 2023 17:26

Instrument :
 BNA_F
 ClientSampleId :
 TP-BCD

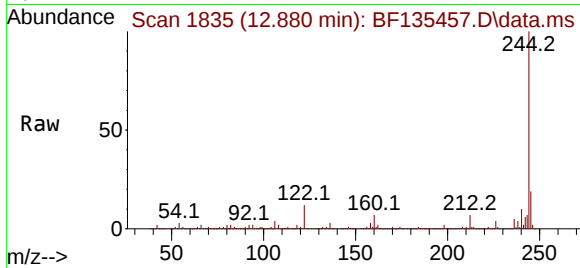

Tgt Ion:244 Resp: 1264032
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.1 7.7
 122 12.1 7.9 11.9#

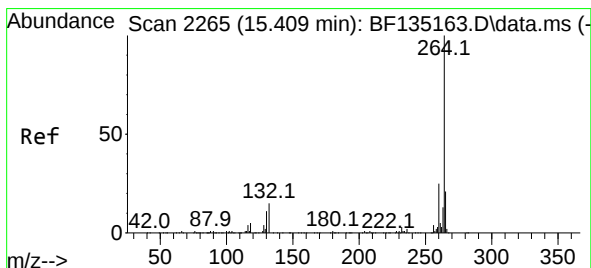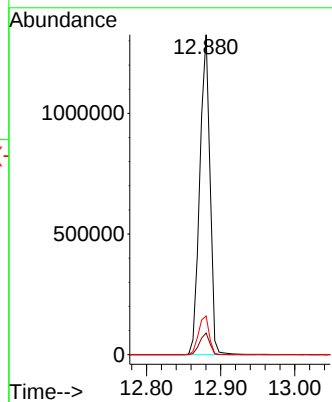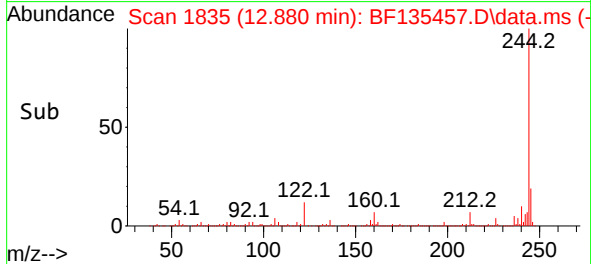

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.404 min Scan# 2264
 Delta R.T. -0.000 min
 Lab File: BF135457.D
 Acq: 26 Sep 2023 17:26

Tgt Ion:264 Resp: 330151
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.8 29.6
 265 21.3 17.0 25.4

