

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
 Data File : BF135444.D
 Acq On : 26 Sep 2023 10:43
 Operator : CG\JU
 Sample : PB155591TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155591TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	583	rBV	4508075	4674504	93.54%	14.320%
2	6.404	729	734	755	rBV	4141594	4716770	94.38%	14.450%
3	6.751	790	793	802	rBV	1322775	1097619	21.96%	3.363%
4	7.316	884	889	893	rBV	2688403	3113354	62.30%	9.538%
5	8.034	1006	1011	1026	rBV	1446309	1466370	29.34%	4.492%
6	9.110	1188	1194	1197	rBV	4505828	4997483	100.00%	15.310%
7	9.786	1304	1309	1313	rBV	1626232	1568489	31.39%	4.805%
8	10.586	1440	1445	1448	rBV	2868190	2848004	56.99%	8.725%
9	11.280	1559	1563	1567	rBV	1835261	1641783	32.85%	5.030%
10	12.880	1830	1835	1839	rBV	4124756	4469732	89.44%	13.693%
11	13.939	2011	2015	2023	rBV	1191954	1094877	21.91%	3.354%
12	15.410	2260	2265	2277	rVB	677237	953914	19.09%	2.922%




Sum of corrected areas: 32642899

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135444.D
Acq On : 26 Sep 2023 10:43
Operator : CG\JU
Sample : PB155591TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155591TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

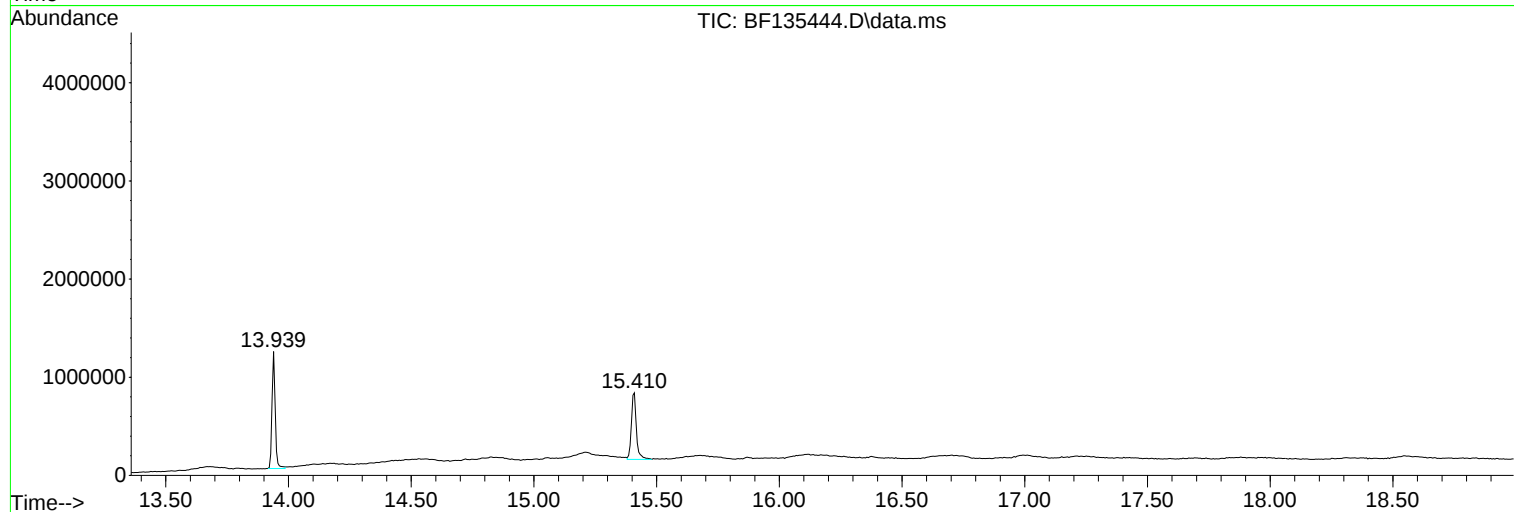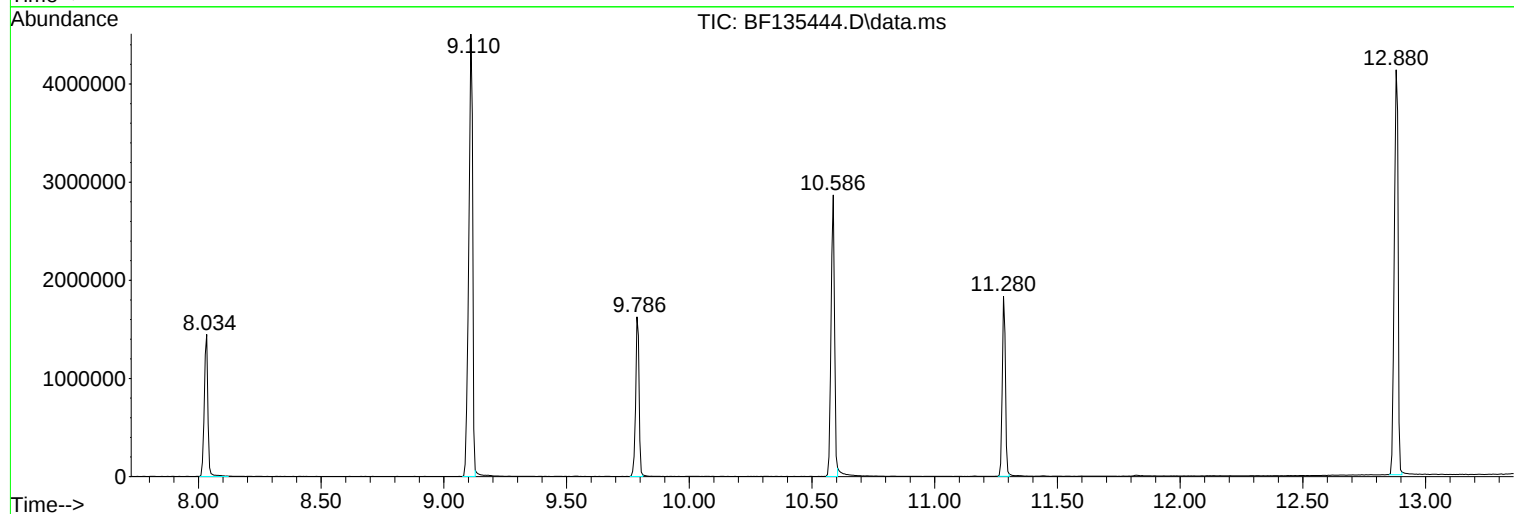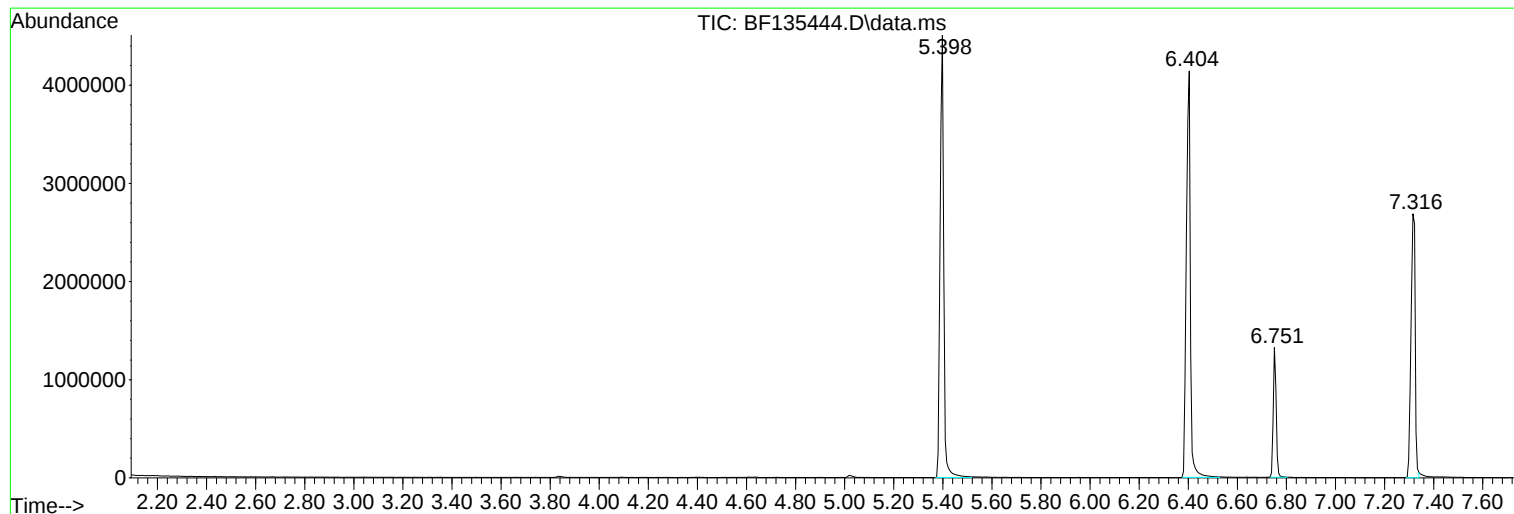

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135444.D
Acq On : 26 Sep 2023 10:43
Operator : CG\JU
Sample : PB155591TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155591TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135444.D
Acq On : 26 Sep 2023 10:43
Operator : CG\JU
Sample : PB155591TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155591TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------