

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
 Data File : BF135445.D
 Acq On : 26 Sep 2023 11:13
 Operator : CG\JU
 Sample : PB155781BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155781BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	495	498	508	rBV	67499	103622	1.91%	0.305%
2	5.399	558	563	566	rBV	4781783	4963082	91.58%	14.598%
3	6.404	729	734	737	rBV	4383374	5046110	93.11%	14.842%
4	6.751	790	793	801	rBV	1248080	1047543	19.33%	3.081%
5	7.322	884	890	893	rBV	3165552	3470965	64.05%	10.209%
6	8.034	1006	1011	1028	rBV	1406621	1401945	25.87%	4.123%
7	9.110	1188	1194	1198	rBV	4656524	5419402	100.00%	15.940%
8	9.786	1304	1309	1313	rBV	1556312	1464832	27.03%	4.308%
9	10.586	1440	1445	1448	rBV	3004434	2969414	54.79%	8.734%
10	11.280	1559	1563	1571	rBV	1690152	1548214	28.57%	4.554%
11	12.886	1830	1836	1839	rBV	4227542	4736700	87.40%	13.932%
12	13.939	2011	2015	2024	rBV	1026699	973967	17.97%	2.865%
13	15.410	2260	2265	2273	rBV	590963	853474	15.75%	2.510%




Sum of corrected areas: 33999270

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135445.D
Acq On : 26 Sep 2023 11:13
Operator : CG\JU
Sample : PB155781BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155781BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

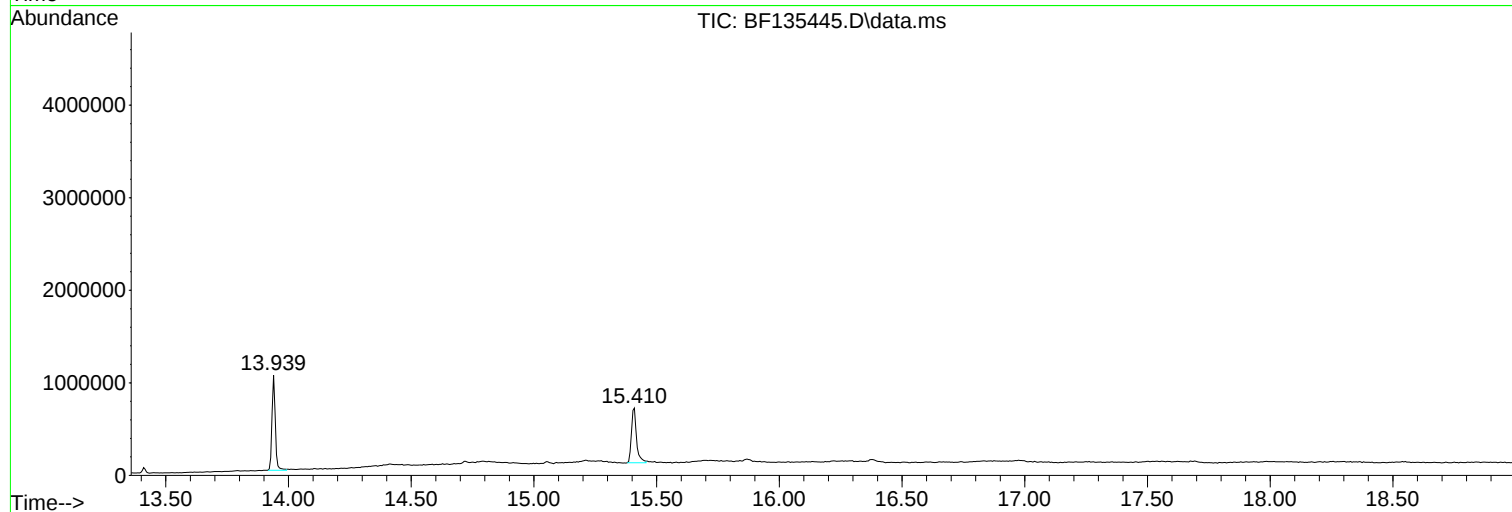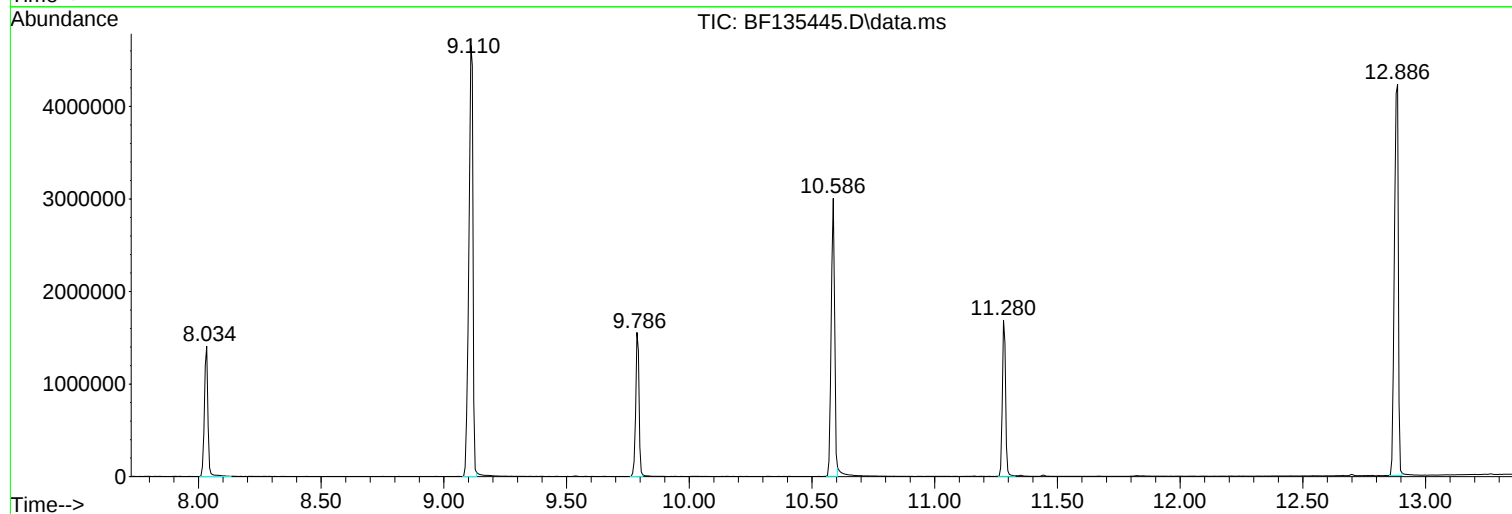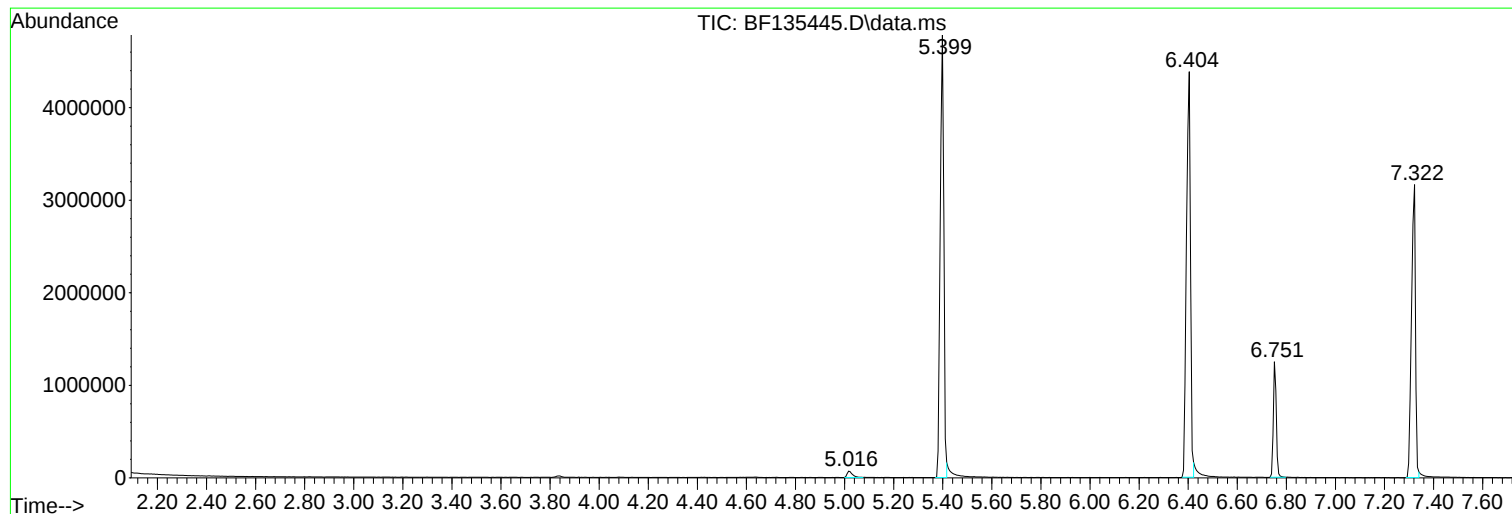

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135445.D
Acq On : 26 Sep 2023 11:13
Operator : CG\JU
Sample : PB155781BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155781BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135445.D
Acq On : 26 Sep 2023 11:13
Operator : CG\JU
Sample : PB155781BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155781BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------