

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
 Data File : BF135448.D
 Acq On : 26 Sep 2023 12:44
 Operator : CG\JU
 Sample : PB155659TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155659TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	558	563	566	rBV	4728919	4807353	91.61%	14.434%
2	6.404	729	734	737	rBV	4298917	4891604	93.22%	14.687%
3	6.751	790	793	804	rBV	1263008	1069779	20.39%	3.212%
4	7.322	884	890	893	rBV	2996418	3338206	63.62%	10.023%
5	8.034	1006	1011	1028	rBV	1407994	1416074	26.99%	4.252%
6	9.110	1188	1194	1198	rBV	4534878	5247381	100.00%	15.756%
7	9.786	1304	1309	1313	rBV	1612176	1499898	28.58%	4.504%
8	10.586	1440	1445	1448	rBV	2926017	2889215	55.06%	8.675%
9	11.280	1559	1563	1572	rBV	1739143	1547270	29.49%	4.646%
10	12.880	1830	1835	1839	rBV	4202162	4647416	88.57%	13.954%
11	13.939	2011	2015	2024	rBV	1080140	1024311	19.52%	3.076%
12	15.404	2260	2264	2277	rBV	680406	926519	17.66%	2.782%




Sum of corrected areas: 33305026

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135448.D
Acq On : 26 Sep 2023 12:44
Operator : CG\JU
Sample : PB155659TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155659TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

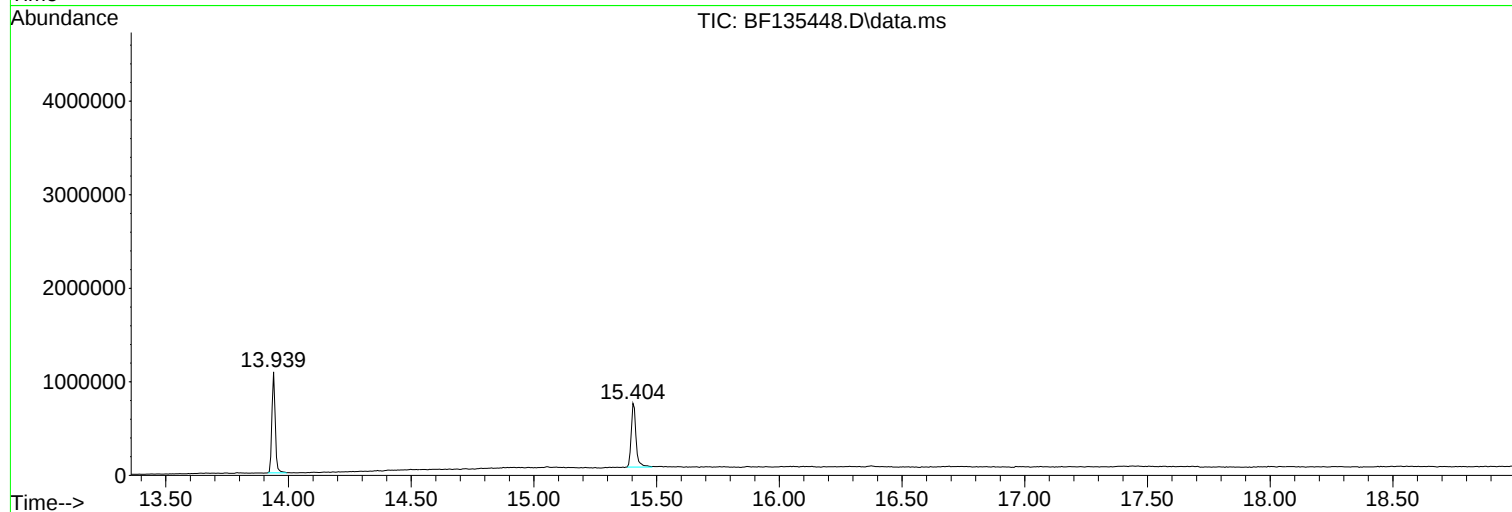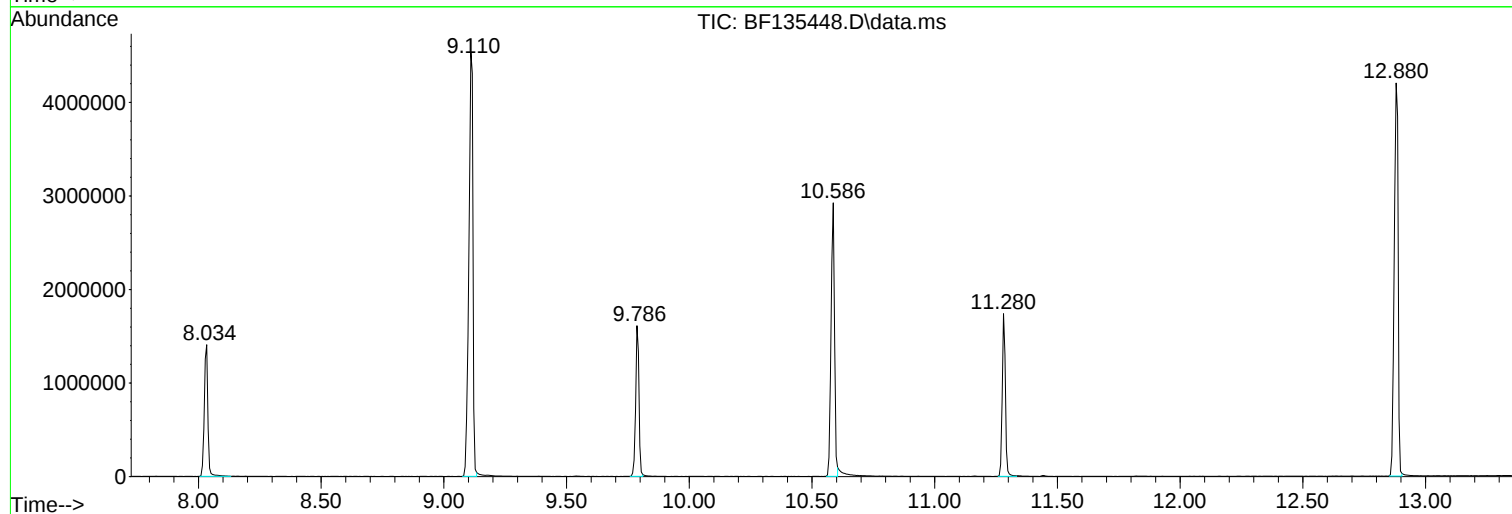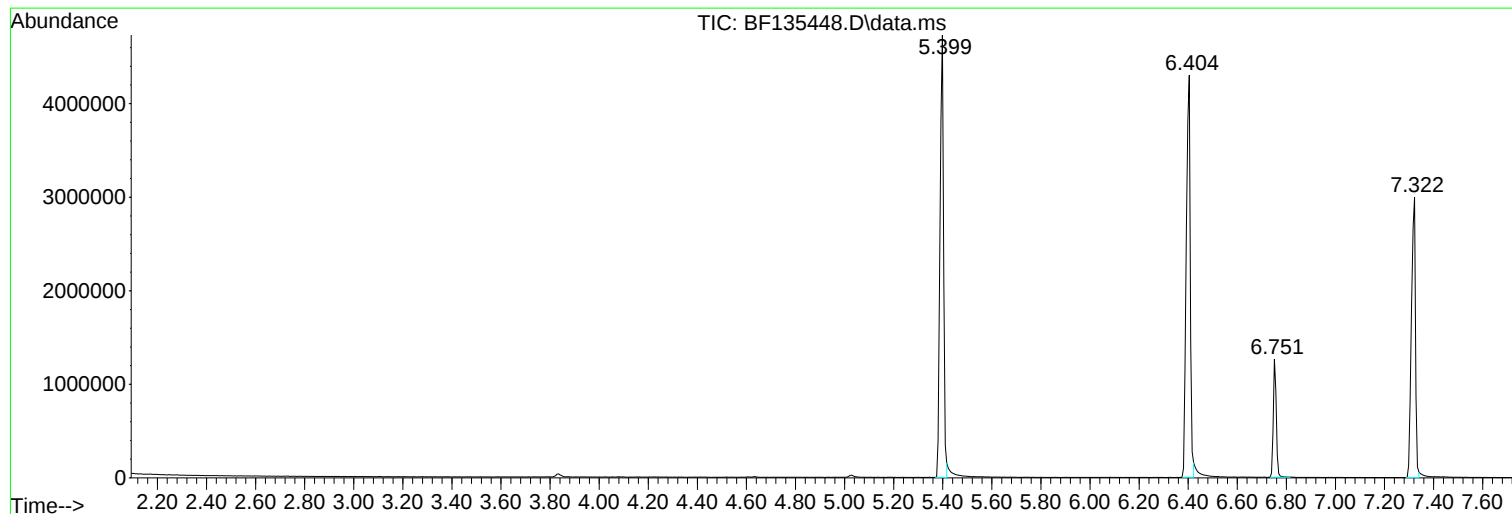

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135448.D
Acq On : 26 Sep 2023 12:44
Operator : CG\JU
Sample : PB155659TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155659TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135448.D
Acq On : 26 Sep 2023 12:44
Operator : CG\JU
Sample : PB155659TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155659TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------