

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
 Data File : BF135449.D
 Acq On : 26 Sep 2023 13:14
 Operator : CG\JU
 Sample : PB155781BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155781BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	566	rBV	4679520	4828649	91.42%	14.453%
2	6.404	729	734	737	rBV	4312655	4852211	91.86%	14.524%
3	6.751	790	793	804	rVB	1212159	1056711	20.01%	3.163%
4	7.322	884	890	893	rBV	2976651	3346274	63.35%	10.016%
5	8.033	1006	1011	1029	rBV	1314676	1400516	26.51%	4.192%
6	9.110	1188	1194	1198	rBV	4567638	5282028	100.00%	15.810%
7	9.786	1304	1309	1313	rBV	1548248	1482255	28.06%	4.437%
8	10.586	1439	1445	1448	rBV	2917536	2899157	54.89%	8.678%
9	11.280	1559	1563	1571	rBV	1770060	1530067	28.97%	4.580%
10	12.880	1830	1835	1839	rBV	4282305	4662140	88.26%	13.955%
11	13.939	2011	2015	2026	rBV	1183537	1097007	20.77%	3.284%
12	15.404	2259	2264	2275	rBV	717730	971361	18.39%	2.908%




Sum of corrected areas: 33408376

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135449.D
Acq On : 26 Sep 2023 13:14
Operator : CG\JU
Sample : PB155781BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155781BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

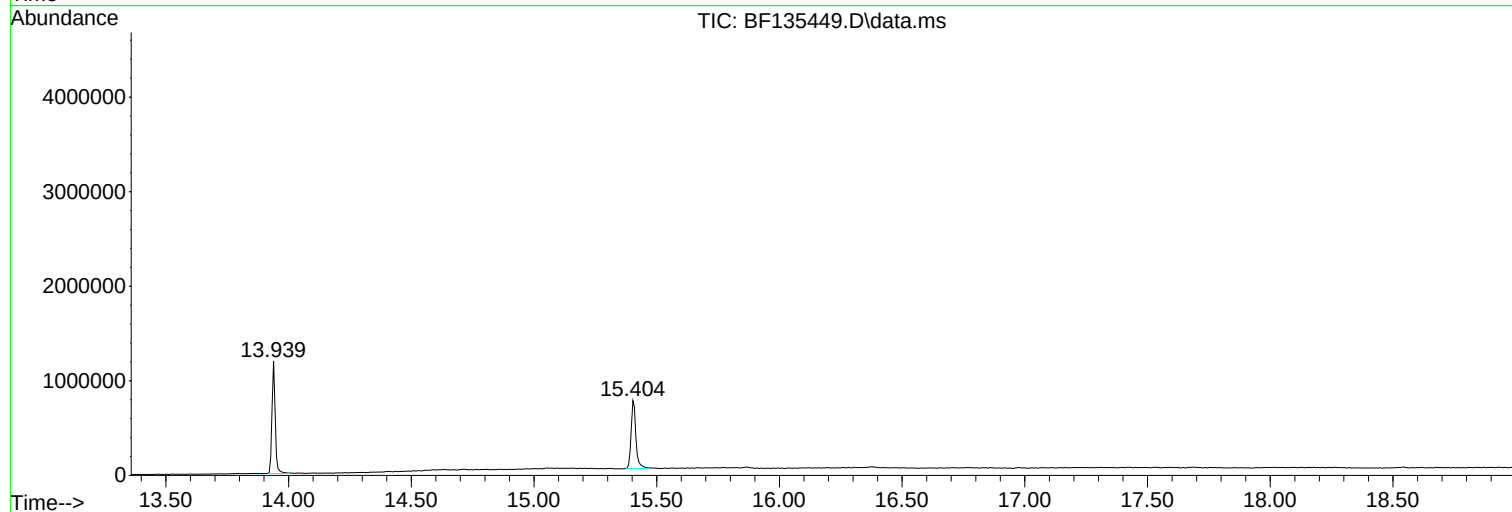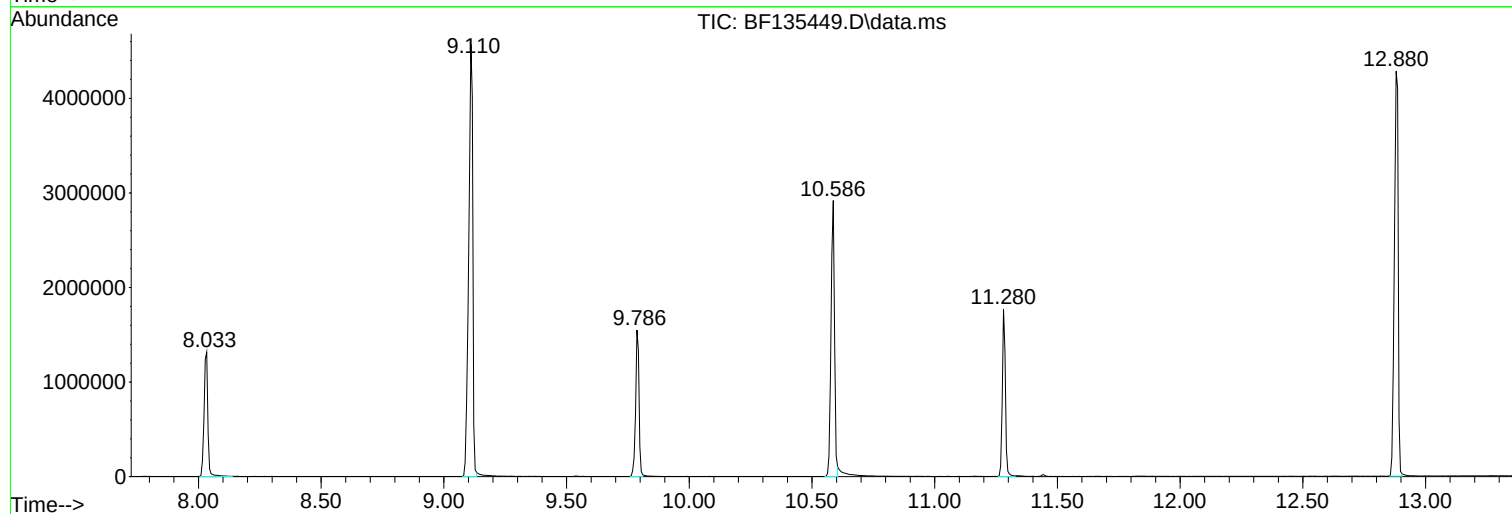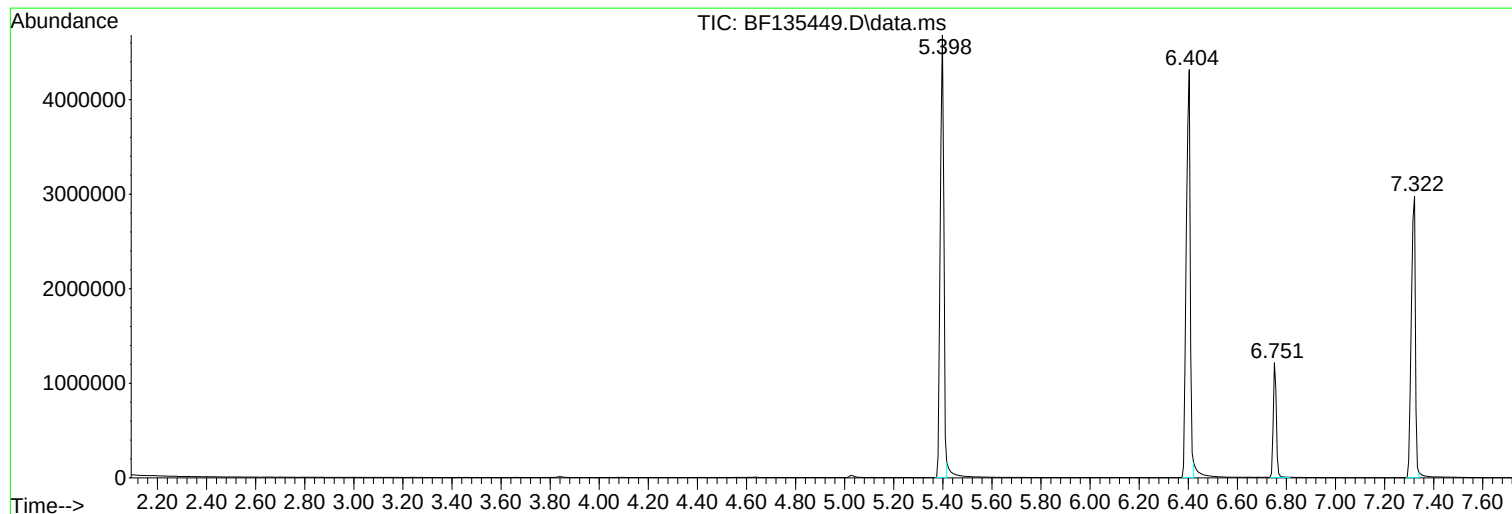

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135449.D
Acq On : 26 Sep 2023 13:14
Operator : CG\JU
Sample : PB155781BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155781BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135449.D
Acq On : 26 Sep 2023 13:14
Operator : CG\JU
Sample : PB155781BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155781BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------