


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135442.D
Acq On : 26 Sep 2023 09:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 26 01:36:36 2023

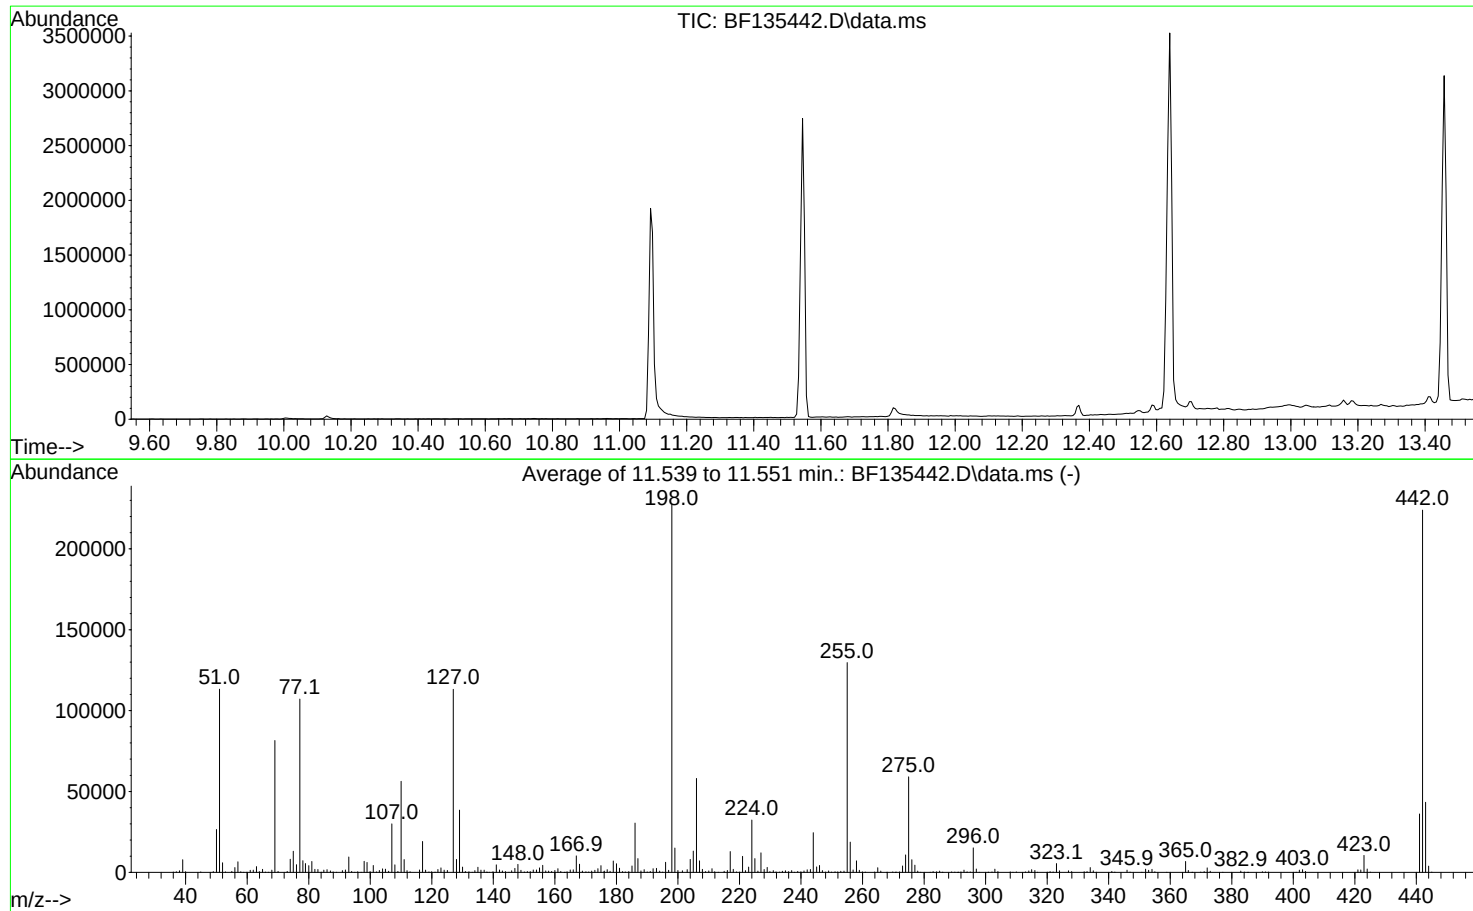




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.8	113309	PASS
68	69	0.00	2	1.7	1347	PASS
69	198	0.00	100	35.8	81525	PASS
70	69	0.00	2	0.8	614	PASS
127	198	10	80	49.8	113187	PASS
197	198	0.00	2	0.5	1248	PASS
198	198	100	100	100.0	227456	PASS
199	198	5	9	6.6	15031	PASS
275	198	10	60	25.9	59024	PASS
365	198	1	100	3.0	6740	PASS
441	198	0.01	100	15.9	36080	PASS
442	442	50	100	100.0	223957	PASS
443	442	15	24	19.4	43355	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135442.D
Acq On : 26 Sep 2023 09:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 26 12:39:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration

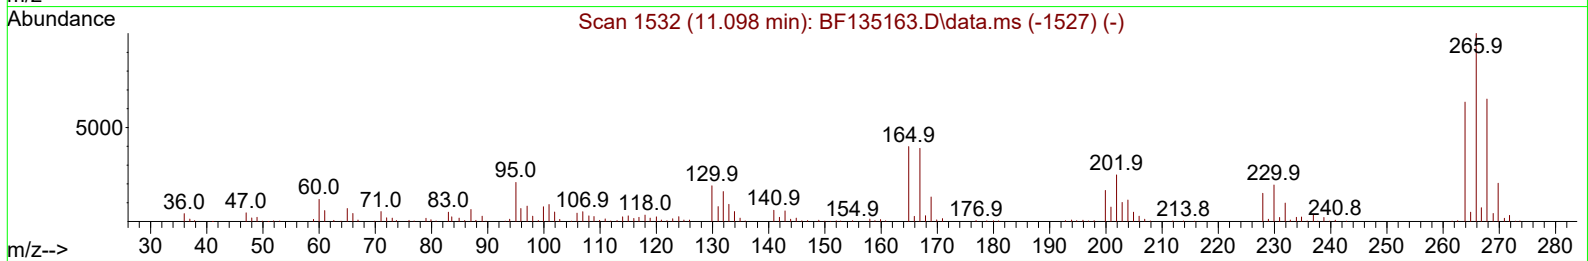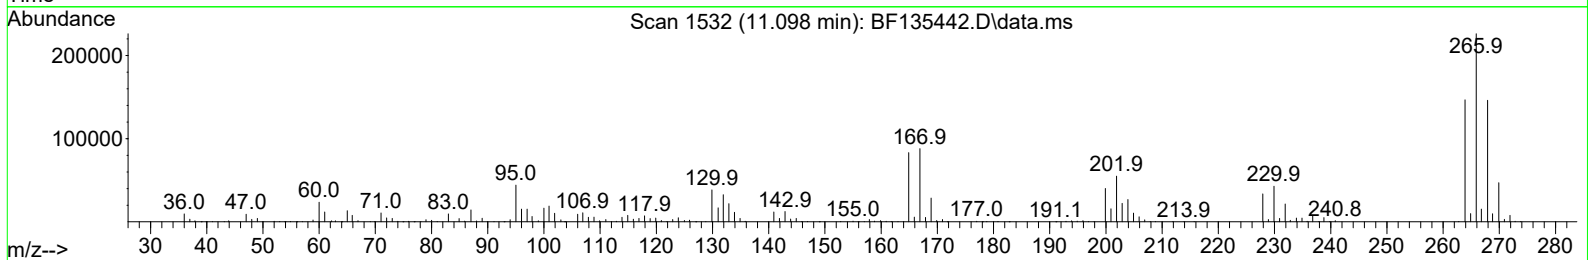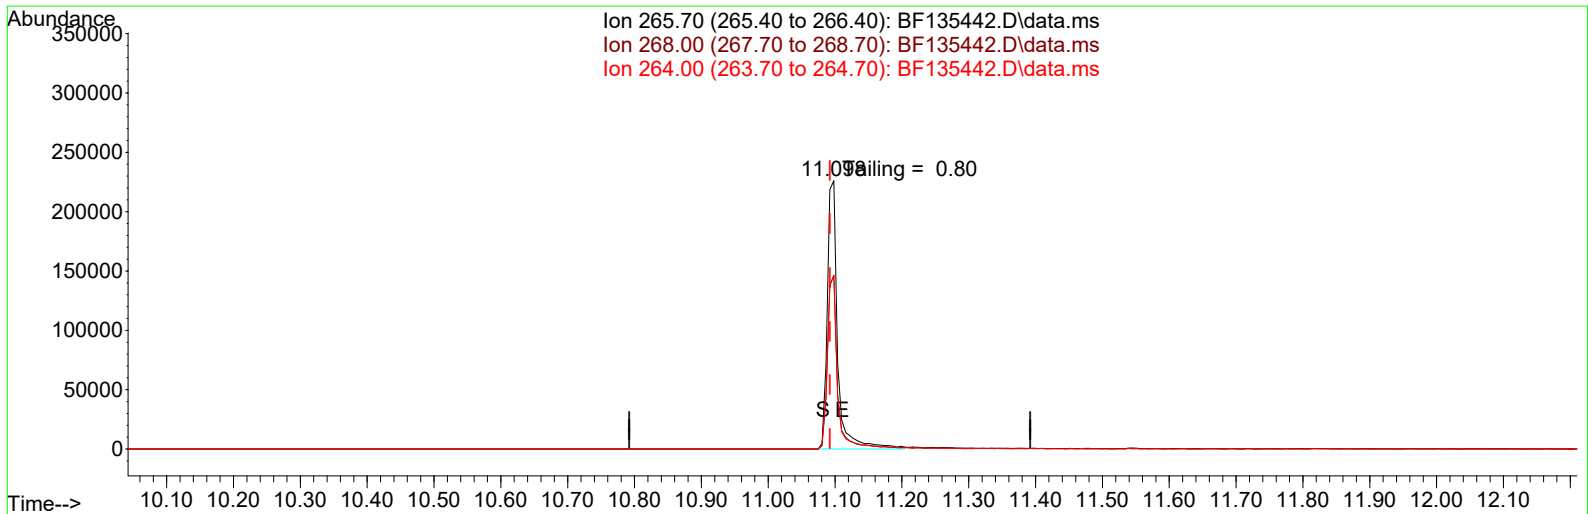

TIC: BF135442.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.006) 39240.00 ng




response 246683

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.60
264.00	63.50	64.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092623\
Data File : BF135442.D
Acq On : 26 Sep 2023 09:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 26 12:39:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration

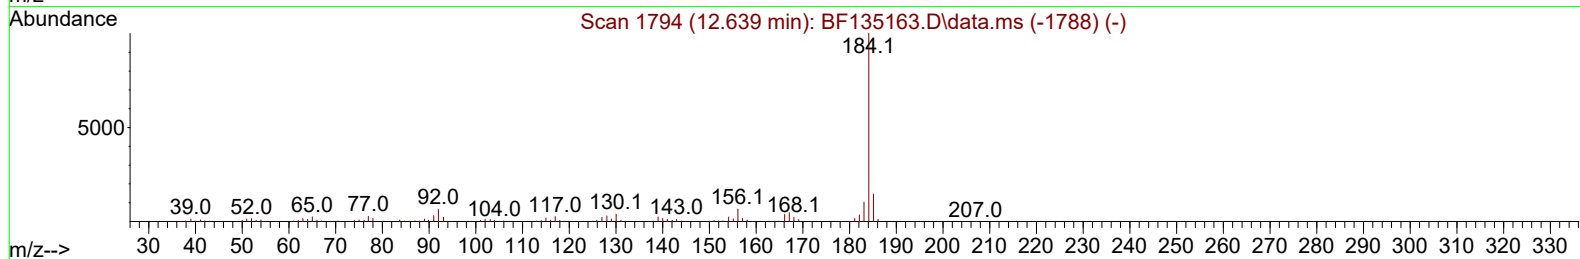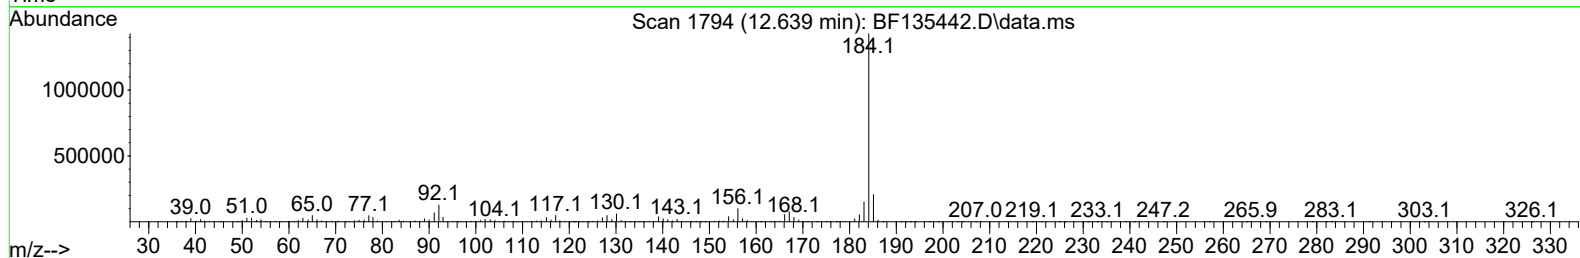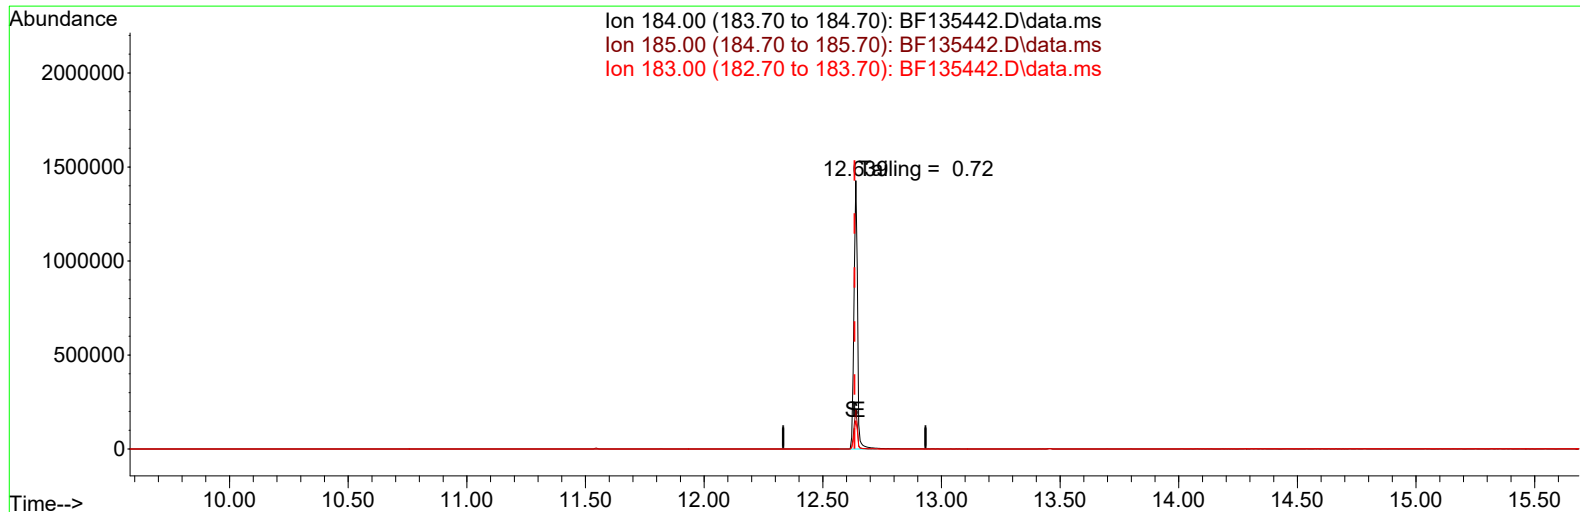

TIC: BF135442.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 133266.40 ng m

response 1427898

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.50
183.00	10.30	10.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2023	BNA_F	<u>BF135442.D</u>
Compound Name	Response	Retention Time
DDT	561916	13.457
DDD	17122	13.157
DDE	1680	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18802	580718	3.24

Instrument :
BNA_F
ClientSampleId :
DFTPP